

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
 Data File : BG052391.D
 Acq On : 15 Feb 2022 14:13
 Operator : CG/JU
 Sample : N1398-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.785	48	50	52	rBV3	678	808	0.15%	0.037%
2	3.932	73	75	77	rBV3	721	673	0.13%	0.031%
3	4.137	109	110	113	rBV3	859	700	0.13%	0.032%
4	4.267	131	132	136	rVB2	902	836	0.16%	0.038%
5	4.325	140	142	146	rVB2	1304	1700	0.33%	0.077%
6	4.478	165	168	170	rVB2	749	699	0.13%	0.032%
7	4.936	244	246	249	rBV3	536	624	0.12%	0.028%
8	5.136	279	280	284	rVB2	926	1074	0.21%	0.049%
9	5.171	284	286	290	rBV	795	1045	0.20%	0.047%
10	5.218	290	294	298	rVV2	604	843	0.16%	0.038%
11	5.441	331	332	335	rVB2	1153	699	0.13%	0.032%
12	5.471	335	337	339	rBV	809	712	0.14%	0.032%
13	5.624	361	363	365	rVB2	1047	787	0.15%	0.036%
14	5.759	384	386	387	rVB	1146	673	0.13%	0.031%
15	5.776	387	389	391	rBV	912	848	0.16%	0.039%
16	5.859	400	403	406	rBV2	430	681	0.13%	0.031%
17	5.906	410	411	414	rVB	718	579	0.11%	0.026%
18	6.076	436	440	442	rBV	564	735	0.14%	0.033%
19	6.094	442	443	447	rBV	651	730	0.14%	0.033%
20	6.223	462	465	468	rBV	631	774	0.15%	0.035%
21	6.399	492	495	498	rVB2	819	847	0.16%	0.038%
22	6.569	522	524	528	rBV	944	845	0.16%	0.038%
23	6.793	559	562	563	rVB	830	663	0.13%	0.030%
24	7.004	596	598	600	rBV2	645	720	0.14%	0.033%
25	7.104	613	615	618	rBV	588	592	0.11%	0.027%
26	7.163	623	625	628	rBV2	552	685	0.13%	0.031%
27	7.339	653	655	657	rBV	643	676	0.13%	0.031%
28	7.450	671	674	675	rVB	702	625	0.12%	0.028%
29	8.220	798	805	814	rVV	80058	139785	26.73%	6.348%
30	8.296	816	818	823	rVB2	431	624	0.12%	0.028%
31	8.725	889	891	895	rBV	409	701	0.13%	0.032%
32	9.254	979	981	984	rBV2	579	683	0.13%	0.031%
33	9.789	1070	1072	1075	rVB	743	702	0.13%	0.032%
34	9.965	1098	1102	1105	rBV	482	895	0.17%	0.041%
35	10.300	1157	1159	1163	rBV2	443	684	0.13%	0.031%
36	10.335	1163	1165	1170	rVB2	453	615	0.12%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
 Data File : BG052391.D
 Acq On : 15 Feb 2022 14:13
 Operator : CG/JU
 Sample : N1398-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	10.517	1193	1196	1198	rBV2	474	581	0.11%	0.026%
38	10.687	1223	1225	1228	rVB2	767	680	0.13%	0.031%
39	10.723	1228	1231	1233	rVB2	580	664	0.13%	0.030%
40	11.057	1280	1288	1300	rBV	108645	204370	39.08%	9.280%
41	11.639	1384	1387	1390	rVB2	491	603	0.12%	0.027%
42	12.285	1493	1497	1501	rBV2	508	884	0.17%	0.040%
43	14.329	1842	1845	1846	rBV2	606	608	0.12%	0.028%
44	14.506	1871	1875	1877	rBV	876	970	0.19%	0.044%
45	14.741	1912	1915	1918	rBV2	498	627	0.12%	0.028%
46	14.770	1918	1920	1924	rVB	608	742	0.14%	0.034%
47	14.864	1930	1936	1947	rBV	193940	318492	60.91%	14.463%
48	16.280	2174	2177	2178	rBV2	627	633	0.12%	0.029%
49	16.902	2280	2283	2286	rVB3	753	736	0.14%	0.033%
50	17.002	2297	2300	2303	rVB2	831	1220	0.23%	0.055%
51	17.049	2303	2308	2310	rBV	586	1176	0.22%	0.053%
52	17.396	2362	2367	2369	rBV2	1010	1788	0.34%	0.081%
53	17.466	2377	2379	2382	rBV3	562	622	0.12%	0.028%
54	17.613	2398	2404	2414	rBV	273333	443556	84.83%	20.142%
55	17.989	2466	2468	2470	rBV2	809	807	0.15%	0.037%
56	18.817	2607	2609	2613	rVB2	1179	1563	0.30%	0.071%
57	18.859	2613	2616	2619	rBV3	1079	1764	0.34%	0.080%
58	19.058	2647	2650	2653	rBV3	887	1208	0.23%	0.055%
59	19.152	2663	2666	2668	rBV2	692	594	0.11%	0.027%
60	19.176	2668	2670	2673	rVB3	714	832	0.16%	0.038%
61	19.235	2677	2680	2683	rVB2	1145	1789	0.34%	0.081%
62	19.264	2683	2685	2686	rBV	1471	1161	0.22%	0.053%
63	19.446	2714	2716	2718	rBV2	1174	1023	0.20%	0.046%
64	19.616	2743	2745	2747	rBV2	764	594	0.11%	0.027%
65	19.675	2753	2755	2756	rVB2	1129	584	0.11%	0.027%
66	19.875	2787	2789	2792	rVB3	1473	1364	0.26%	0.062%
67	19.904	2792	2794	2796	rBV	1193	1074	0.21%	0.049%
68	19.951	2800	2802	2803	rVB	1071	650	0.12%	0.030%
69	20.192	2841	2843	2845	rBV3	1700	1265	0.24%	0.057%
70	20.233	2849	2850	2853	rBV3	1477	828	0.16%	0.038%
71	20.750	2936	2938	2939	rBV2	2188	1345	0.26%	0.061%
72	21.931	3132	3139	3153	rVB	294843	522903	100.00%	23.745%
73	25.391	3718	3728	3742	rVB2	166004	509143	97.37%	23.120%
74	25.644	3769	3771	3773	rBV3	2815	2564	0.49%	0.116%
75	28.205	4205	4207	4210	rBV3	3232	3596	0.69%	0.163%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052391.D
Acq On : 15 Feb 2022 14:13
Operator : CG/JU
Sample : N1398-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Title : SVOA CALIBRATION




Sum of corrected areas: 2202165

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052391.D
Acq On : 15 Feb 2022 14:13
Operator : CG/JU
Sample : N1398-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

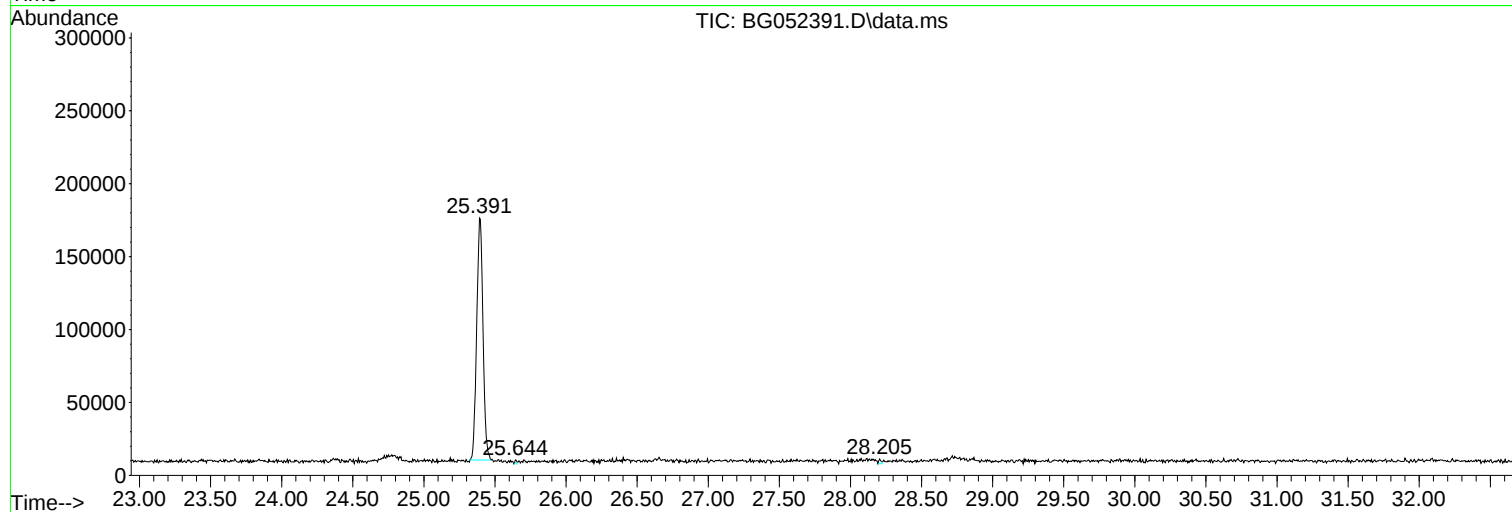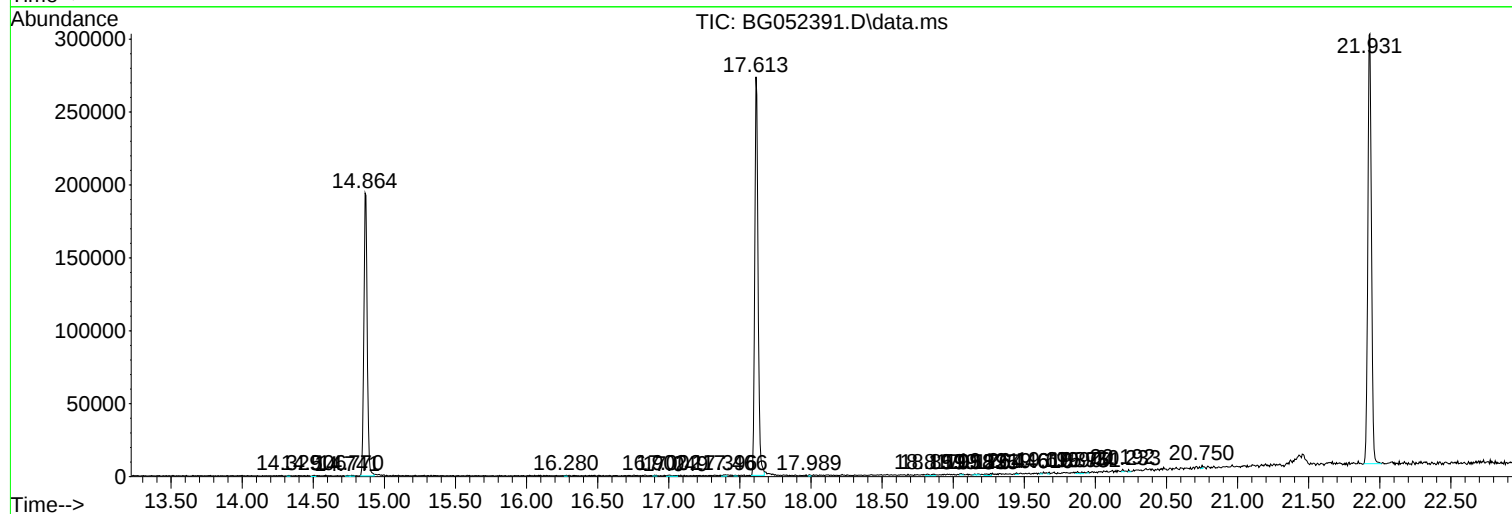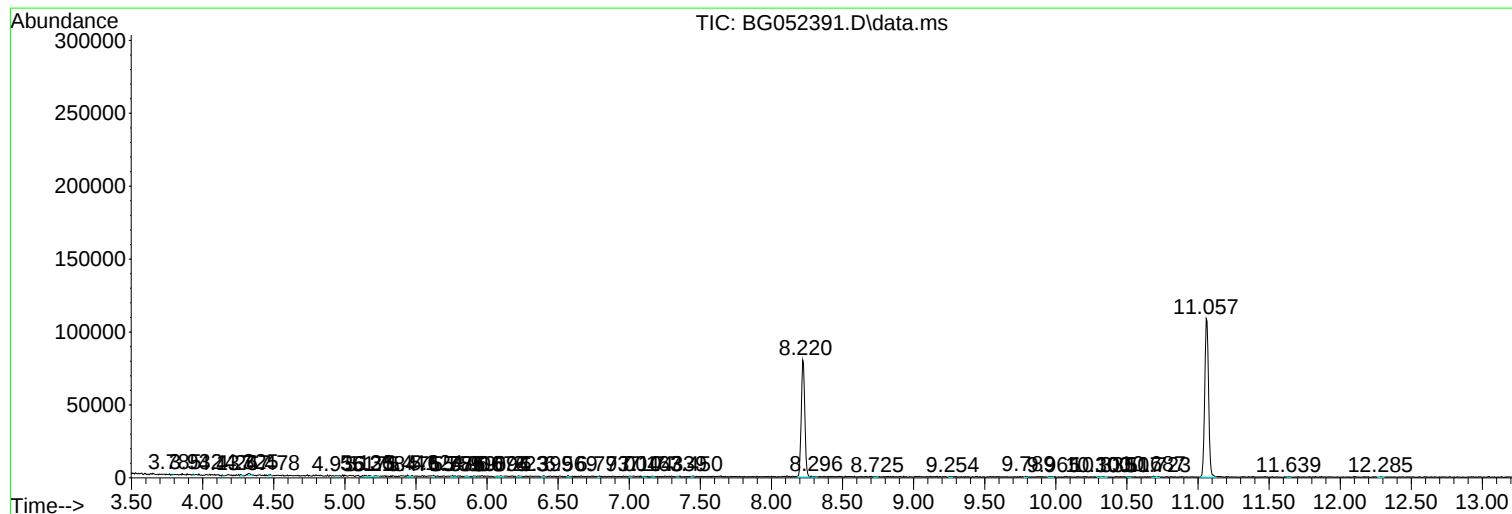

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052391.D
Acq On : 15 Feb 2022 14:13
Operator : CG/JU
Sample : N1398-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052391.D
Acq On : 15 Feb 2022 14:13
Operator : CG/JU
Sample : N1398-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc