

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
 Data File : BG052392.D
 Acq On : 15 Feb 2022 14:51
 Operator : CG/JU
 Sample : N1519-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.635	24	25	28	rVB2	1194	662	0.14%	0.033%
2	3.787	49	51	52	rBV2	756	701	0.15%	0.035%
3	3.840	59	60	62	rBV	804	699	0.15%	0.035%
4	3.887	66	68	70	rBV	737	732	0.15%	0.036%
5	3.975	81	83	87	rVB3	936	1021	0.22%	0.050%
6	4.011	87	89	91	rBV	631	806	0.17%	0.040%
7	4.252	129	130	133	rVB	732	654	0.14%	0.032%
8	4.457	162	165	166	rBV	648	635	0.13%	0.031%
9	4.586	185	187	192	rVB	512	545	0.11%	0.027%
10	4.627	192	194	196	rBV2	632	688	0.15%	0.034%
11	4.657	198	199	202	rBV2	793	945	0.20%	0.047%
12	4.686	202	204	207	rVB2	996	819	0.17%	0.040%
13	4.739	212	213	216	rBV2	982	1046	0.22%	0.052%
14	4.804	223	224	226	rBV	730	596	0.13%	0.029%
15	4.874	233	236	239	rBV	439	686	0.14%	0.034%
16	5.045	263	265	267	rBV	883	680	0.14%	0.034%
17	5.139	280	281	284	rVB2	954	816	0.17%	0.040%
18	5.274	300	304	305	rVB2	843	706	0.15%	0.035%
19	5.350	316	317	320	rBV	764	660	0.14%	0.033%
20	5.426	327	330	332	rBV	1116	777	0.16%	0.038%
21	5.526	345	347	350	rVB2	588	557	0.12%	0.028%
22	5.679	370	373	375	rVB2	771	653	0.14%	0.032%
23	6.331	479	484	487	rBV	541	879	0.19%	0.043%
24	8.140	790	792	794	rVB2	696	634	0.13%	0.031%
25	8.176	794	798	799	rBV2	676	867	0.18%	0.043%
26	8.223	799	806	814	rVB2	74150	129669	27.33%	6.410%
27	8.358	827	829	832	rVB	636	687	0.14%	0.034%
28	8.399	832	836	837	rBV2	516	585	0.12%	0.029%
29	8.528	856	858	862	rVB2	649	821	0.17%	0.041%
30	9.198	969	972	975	rBV2	672	670	0.14%	0.033%
31	9.703	1055	1058	1059	rBV2	595	583	0.12%	0.029%
32	9.926	1093	1096	1100	rBV2	518	640	0.13%	0.032%
33	10.202	1141	1143	1148	rVB2	651	941	0.20%	0.047%
34	10.249	1148	1151	1152	rBV	453	591	0.12%	0.029%
35	10.578	1204	1207	1211	rVB2	425	772	0.16%	0.038%
36	10.901	1259	1262	1265	rBV	554	593	0.12%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
 Data File : BG052392.D
 Acq On : 15 Feb 2022 14:51
 Operator : CG/JU
 Sample : N1519-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	11.060	1282	1289	1298	rBV	103173	189455	39.93%	9.365%
38	11.207	1309	1314	1315	rBV2	378	585	0.12%	0.029%
39	11.383	1340	1344	1345	rBV	706	657	0.14%	0.032%
40	12.305	1498	1501	1504	rVB2	512	717	0.15%	0.035%
41	13.545	1706	1712	1713	rBV2	458	669	0.14%	0.033%
42	13.656	1728	1731	1734	rBV2	389	646	0.14%	0.032%
43	14.032	1793	1795	1796	rBV	852	599	0.13%	0.030%
44	14.303	1838	1841	1843	rBV2	482	569	0.12%	0.028%
45	14.455	1865	1867	1871	rVB2	434	572	0.12%	0.028%
46	14.567	1883	1886	1891	rBV2	711	1134	0.24%	0.056%
47	14.867	1929	1937	1952	rBV	180066	292672	61.68%	14.467%
48	15.066	1970	1971	1974	rBV2	531	597	0.13%	0.030%
49	15.143	1981	1984	1987	rVB2	722	855	0.18%	0.042%
50	15.184	1987	1991	1995	rBV2	458	925	0.19%	0.046%
51	15.571	2054	2057	2060	rBV2	637	763	0.16%	0.038%
52	15.777	2090	2092	2096	rBV	591	766	0.16%	0.038%
53	15.824	2096	2100	2103	rVB2	523	820	0.17%	0.041%
54	16.112	2146	2149	2150	rBV	524	577	0.12%	0.029%
55	16.200	2160	2164	2169	rVB2	575	906	0.19%	0.045%
56	16.271	2175	2176	2180	rBV2	435	567	0.12%	0.028%
57	16.394	2194	2197	2199	rBV	545	594	0.13%	0.029%
58	16.817	2267	2269	2273	rBV2	553	846	0.18%	0.042%
59	16.923	2284	2287	2289	rBV2	661	645	0.14%	0.032%
60	16.946	2289	2291	2294	rBV	414	575	0.12%	0.028%
61	17.075	2309	2313	2316	rVB2	540	637	0.13%	0.031%
62	17.105	2316	2318	2320	rBV	467	572	0.12%	0.028%
63	17.616	2398	2405	2418	rBV	241793	404769	85.31%	20.008%
64	18.080	2480	2484	2486	rBV2	555	778	0.16%	0.038%
65	18.156	2495	2497	2498	rBV	922	568	0.12%	0.028%
66	18.603	2572	2573	2577	rBV2	653	773	0.16%	0.038%
67	18.879	2617	2620	2622	rBV	789	854	0.18%	0.042%
68	18.967	2634	2635	2637	rBV2	1026	730	0.15%	0.036%
69	19.090	2652	2656	2658	rBV	1078	1661	0.35%	0.082%
70	19.126	2661	2662	2665	rVV2	1089	1116	0.24%	0.055%
71	19.172	2667	2670	2672	rVV2	1081	1126	0.24%	0.056%
72	19.202	2673	2675	2678	rVB2	1085	1083	0.23%	0.054%
73	19.231	2678	2680	2681	rBV	1119	838	0.18%	0.041%
74	19.366	2702	2703	2707	rBV2	778	1242	0.26%	0.061%
75	19.460	2716	2719	2721	rBV2	1152	963	0.20%	0.048%
76	19.484	2721	2723	2725	rBV2	1091	827	0.17%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
 Data File : BG052392.D
 Acq On : 15 Feb 2022 14:51
 Operator : CG/JU
 Sample : N1519-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	19.507	2725	2727	2728	rVB2	872	547	0.12%	0.027%
78	19.554	2732	2735	2736	rBV2	941	788	0.17%	0.039%
79	19.689	2755	2758	2759	rBV3	676	704	0.15%	0.035%
80	19.842	2782	2784	2787	rVB3	1331	1105	0.23%	0.055%
81	20.036	2815	2817	2819	rVB2	1135	735	0.15%	0.036%
82	20.165	2837	2839	2840	rBV2	1315	903	0.19%	0.045%
83	20.383	2875	2876	2879	rBV3	1982	1253	0.26%	0.062%
84	20.412	2879	2881	2883	rBV3	2035	1641	0.35%	0.081%
85	20.500	2894	2896	2899	rVB3	2033	1230	0.26%	0.061%
86	21.928	3133	3139	3147	rVB	275447	474466	100.00%	23.453%
87	25.393	3720	3729	3746	rVB3	151761	466293	98.28%	23.049%
88	26.081	3844	3846	3847	rBV	2892	2101	0.44%	0.104%




Sum of corrected areas: 2023030

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052392.D
Acq On : 15 Feb 2022 14:51
Operator : CG/JU
Sample : N1519-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

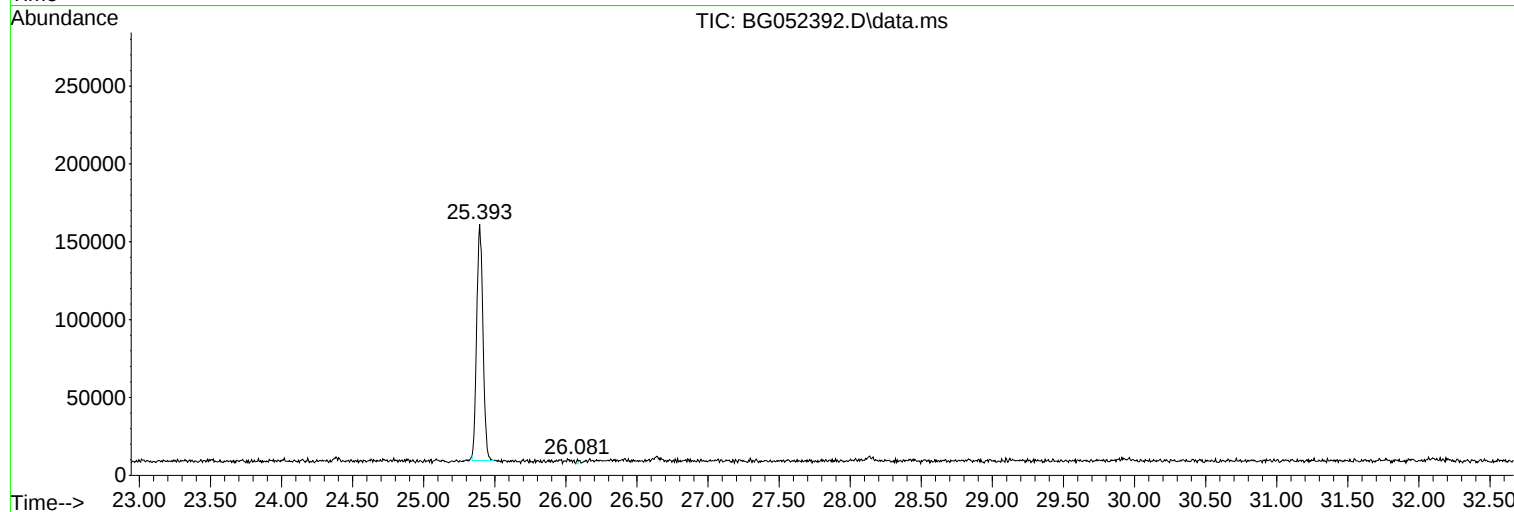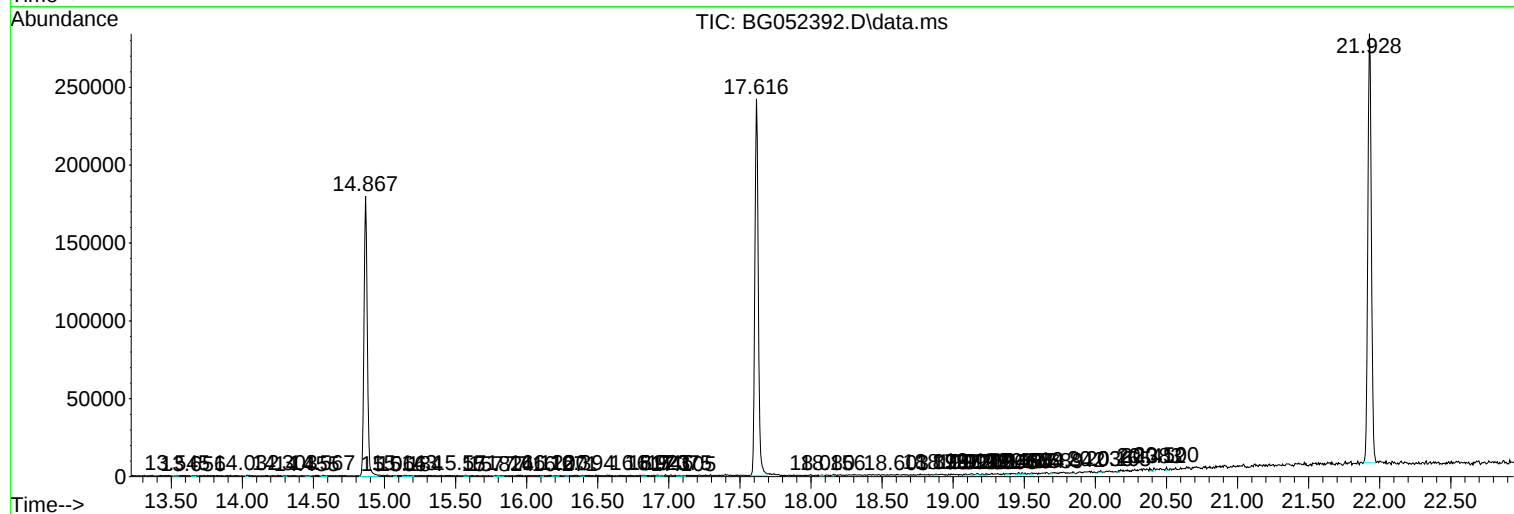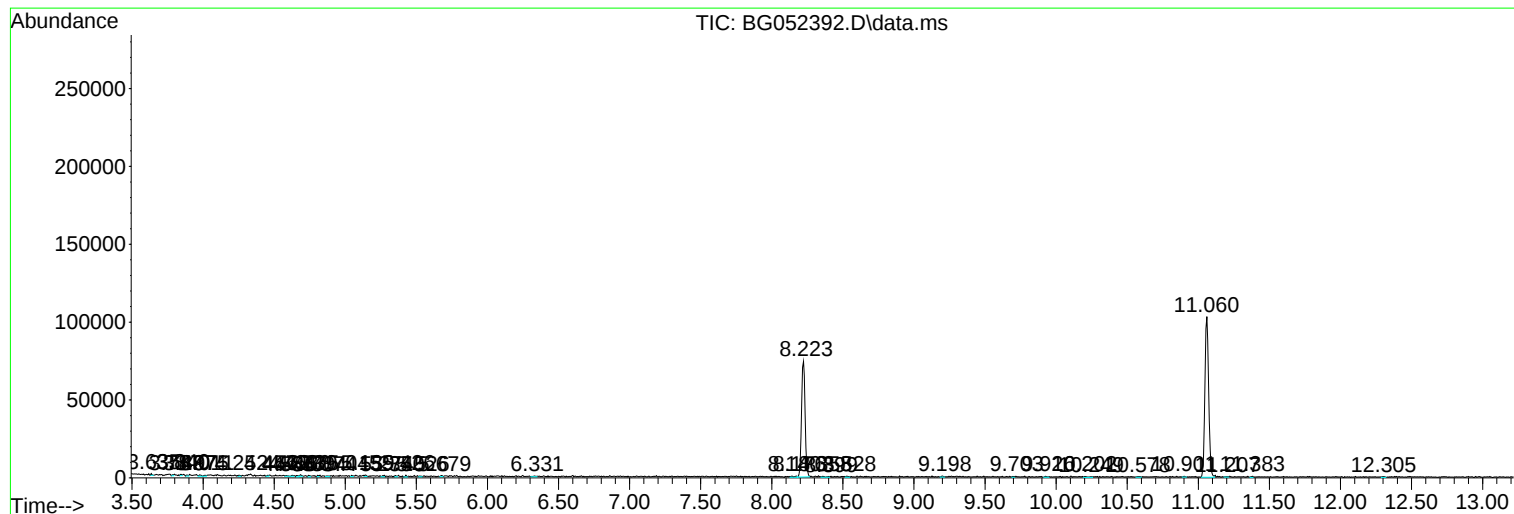

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052392.D
Acq On : 15 Feb 2022 14:51
Operator : CG/JU
Sample : N1519-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021522\
Data File : BG052392.D
Acq On : 15 Feb 2022 14:51
Operator : CG/JU
Sample : N1519-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc