


Data Path : Z:\HPCHEM1\BNA_G\Data\BG021615\
Data File : BG015991.D
Acq On : 16 Feb 2015 9:55
Operator : TP/IZ
Sample : DFTPP04
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP04

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG021015.M
Title : SVOA CALIBRATION
Last Update : Wed Feb 11 12:50:03 2015

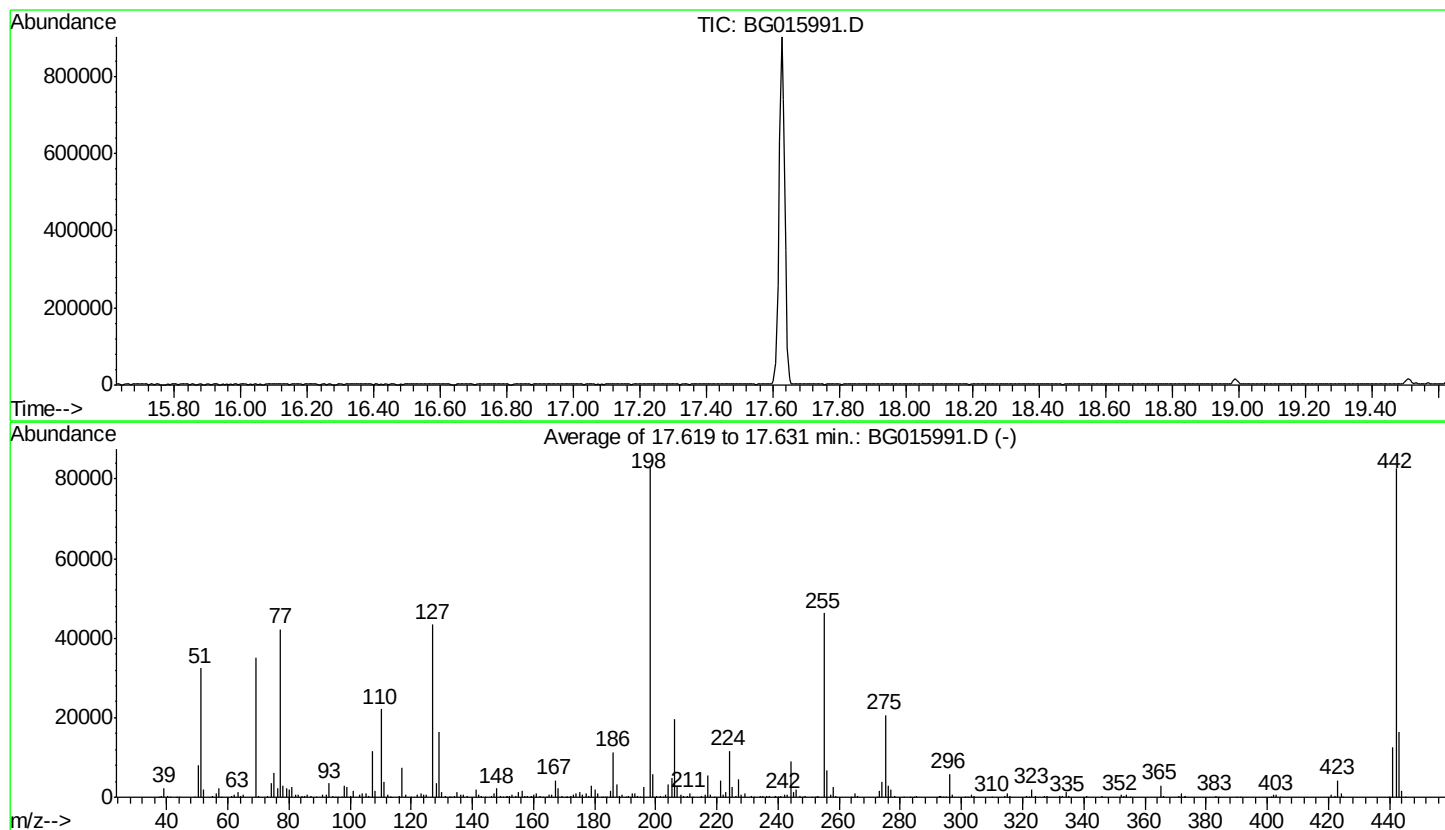

AutoFind: Scans 2542, 2543, 2544; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	32480	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.1	35101	PASS
70	69	0.00	2	0.7	259	PASS
127	198	10	80	52.0	43330	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83362	PASS
199	198	5	9	6.8	5662	PASS
275	198	10	60	24.9	20742	PASS
365	198	1	100	3.5	2941	PASS
441	443	0.01	100	76.7	12621	PASS
442	198	50	100	99.2	82730	PASS
443	442	15	24	19.9	16450	PASS