
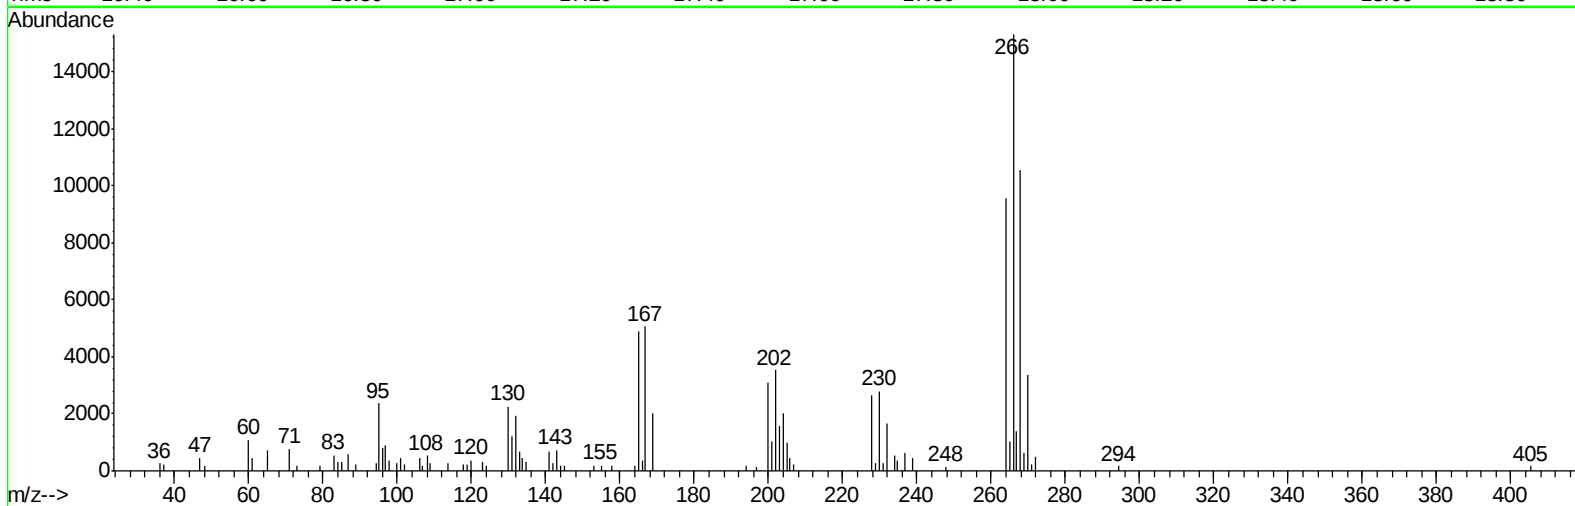


Data Path : Z:\HPCHEM1\BNA G\Data\BG021618\
Data File : BG032737.D
Acq On : 16 Feb 2018 13:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 23:05:42 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 16 18:34:49 2018
Response via : Initial Calibration

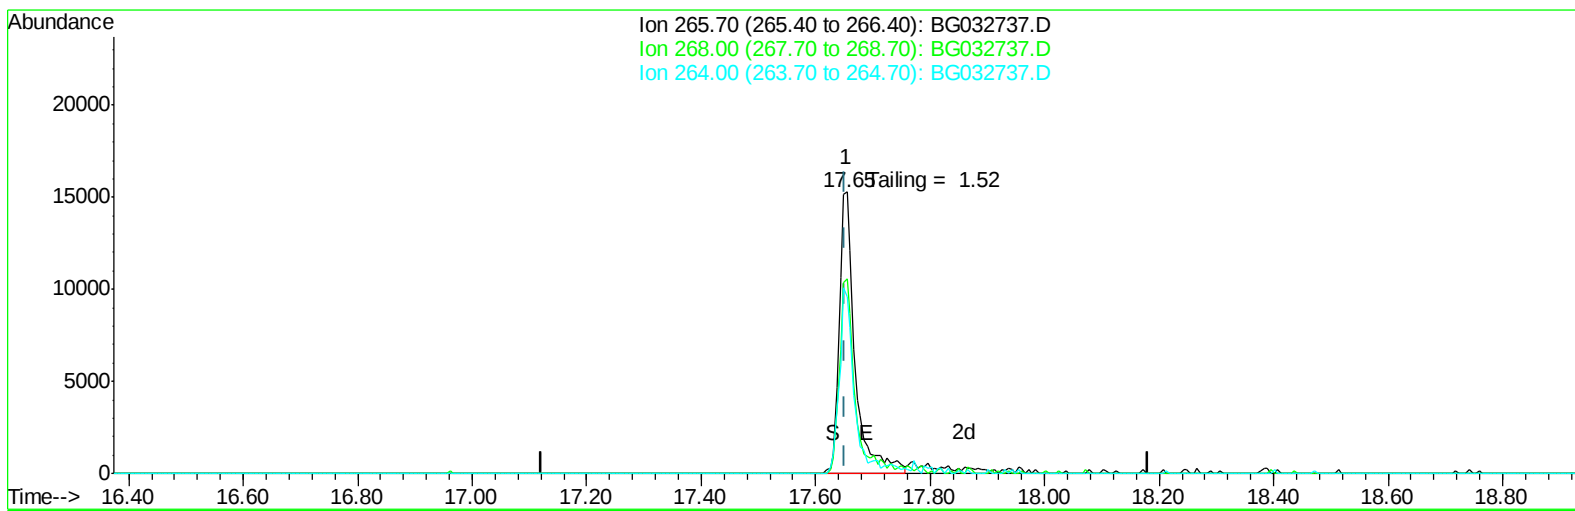

TIC: BG032737.D

(69) Pentachlorophenol (C)



17.655min (+0.002) 47385.73ng

response 29876

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.02
264.00	62.00	62.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG021618\
Data File : BG032737.D
Acq On : 16 Feb 2018 13:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 23:05:42 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 16 18:34:49 2018
Response via : Initial Calibration

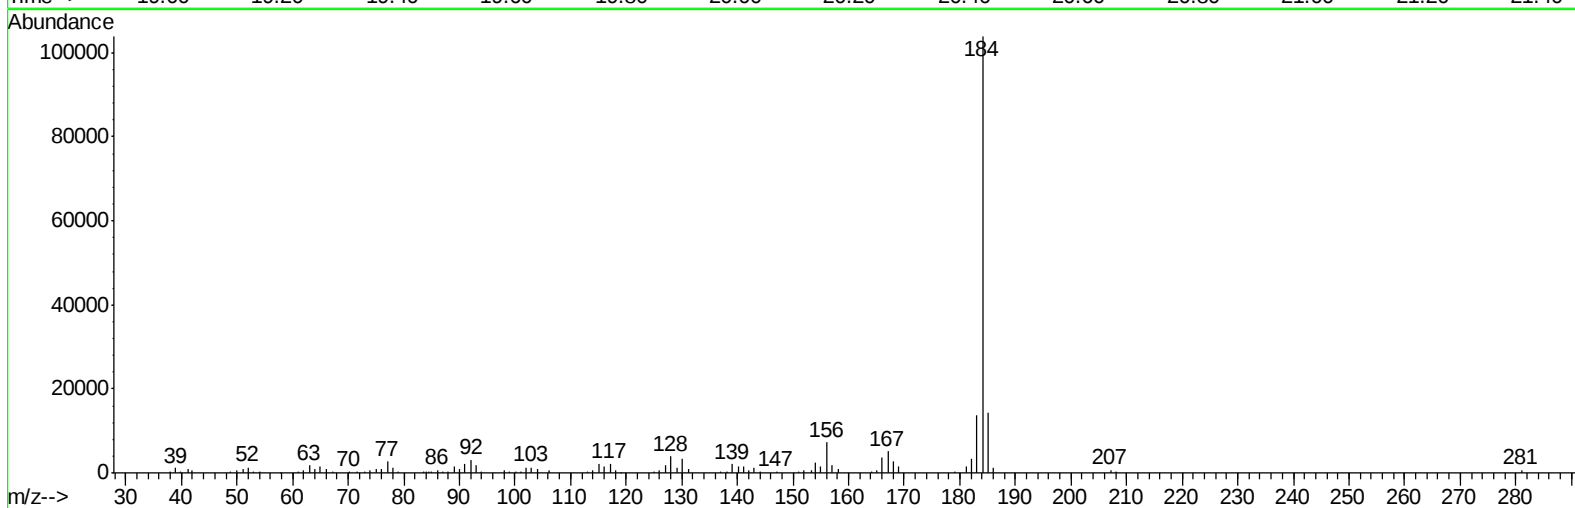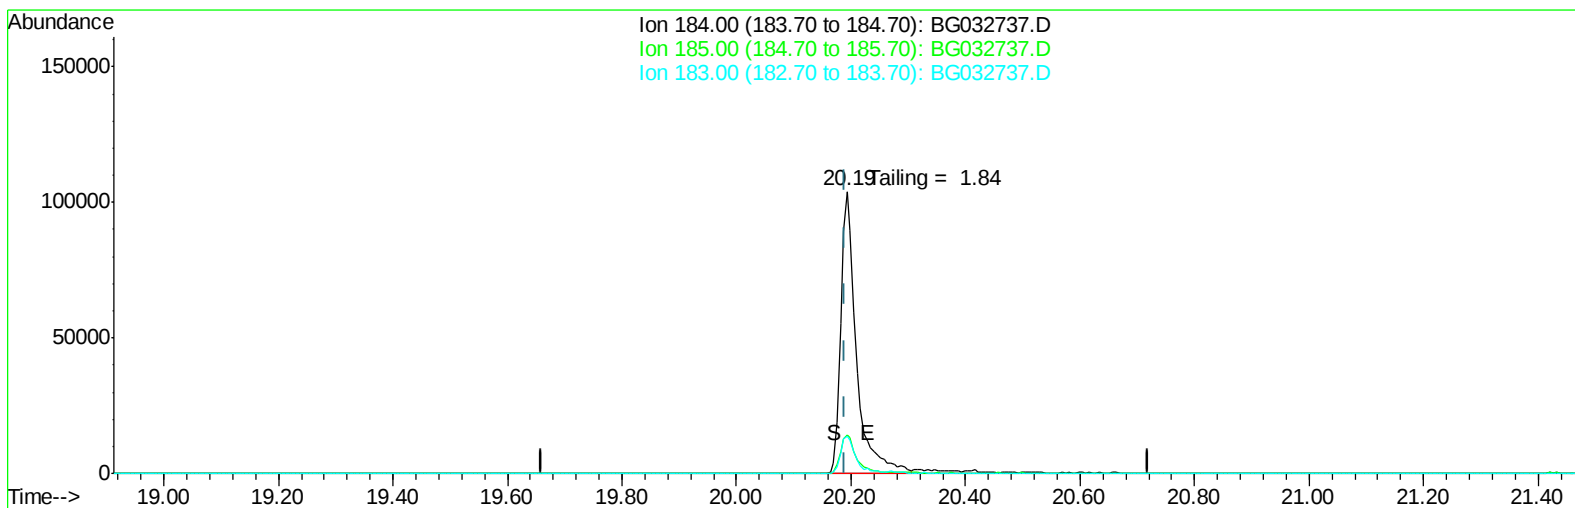

TIC: BG032737.D

(76) Benzidine

20.193min (+0.002) 129730.59ng

response 198564

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.76
183.00	13.30	13.11
0.00	0.00	0.00