


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG021618\
 Data File : BG032737.D
 Acq On : 16 Feb 2018 13:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 16 18:34:49 2018

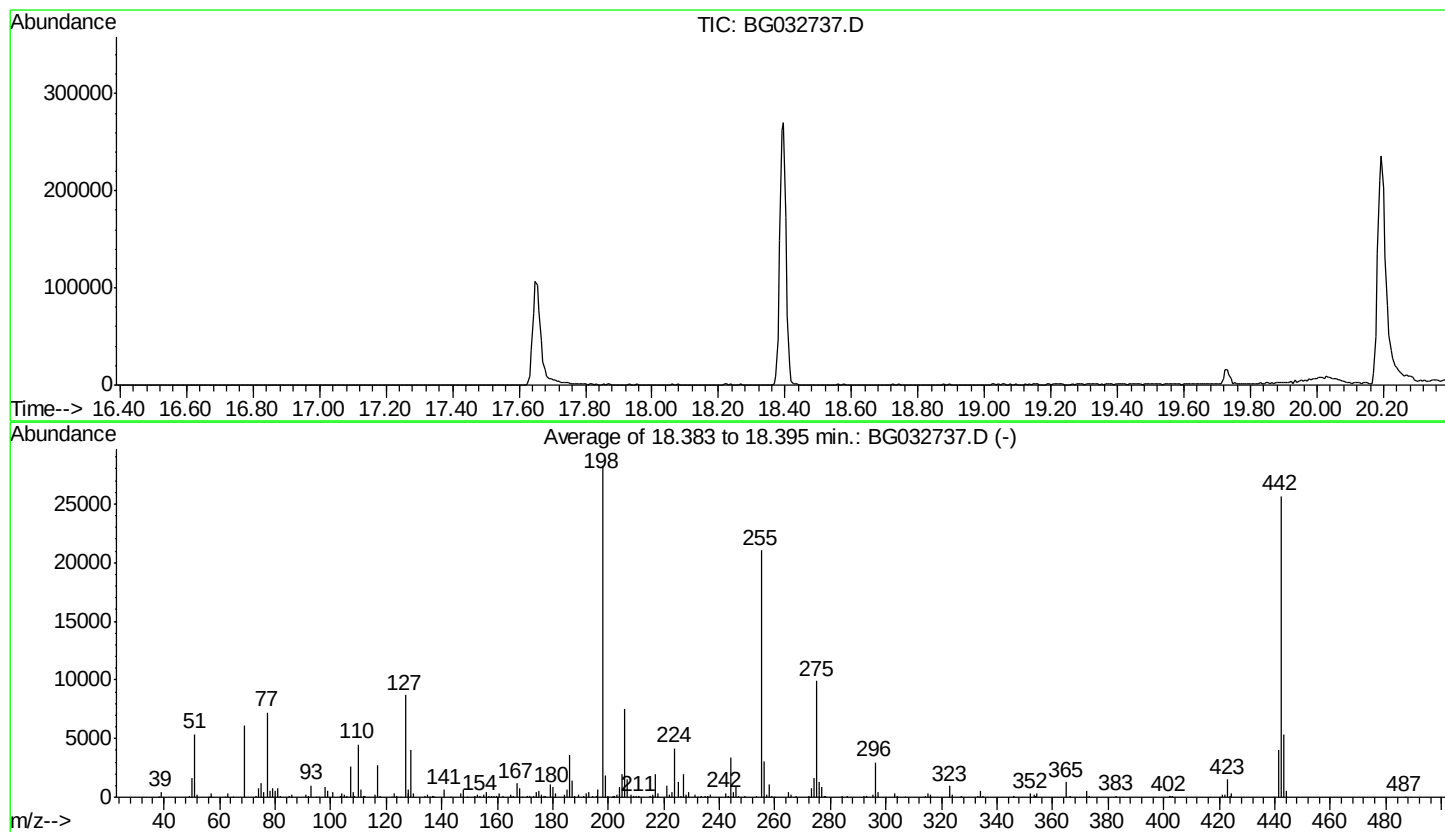

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.1	5393	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.7	6139	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	30.8	8698	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28264	PASS
199	198	5	9	6.6	1878	PASS
275	198	10	60	35.0	9900	PASS
365	198	1	100	4.5	1267	PASS
441	442	0.01	24	15.6	3994	PASS
442	198	50	100	90.8	25672	PASS
443	442	15	24	20.9	5358	PASS