

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021621\
 Data File : BG048169.D
 Acq On : 16 Feb 2021 18:58
 Operator : CG/JU
 Sample : M1407-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBGL4

Quant Time: Feb 16 23:35:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 16 23:25:09 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	55746	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	217012	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	164664	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	418592	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	456634	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	456464	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.51	96	7195	5.37	ng/uL	0.00
5) Phenol-d5	7.25	99	31121	6.63	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.42	67	82977	29.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	78073	23.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	53754	14.59	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	51144	31.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	58451	29.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	95336	24.82	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	9084	2.39	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	382277	31.34	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	451563	30.29	ng/ul	0.00
52) 4-Nitrophenol-d4	14.90	143	14920	7.20	ng/ul	0.00
58) Fluorene-d10	15.72	176	356484	32.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	85079	33.15	ng/ul	0.00
71) Anthracene-d10	17.57	188	687226	38.29	ng/ul	0.00
79) Pyrene-d10	19.85	212	851446	37.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	880630	37.82	ng/ul	0.01


Target Compounds					Ovalue	
45) Dimethylphthalate	14.17	163	14636	1.161	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021621\
Data File : BG048169.D
Acq On : 16 Feb 2021 18:58
Operator : CG/JU
Sample : M1407-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBGL4

Quant Time: Feb 16 23:35:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 16 23:25:09 2021
Response via : Initial Calibration

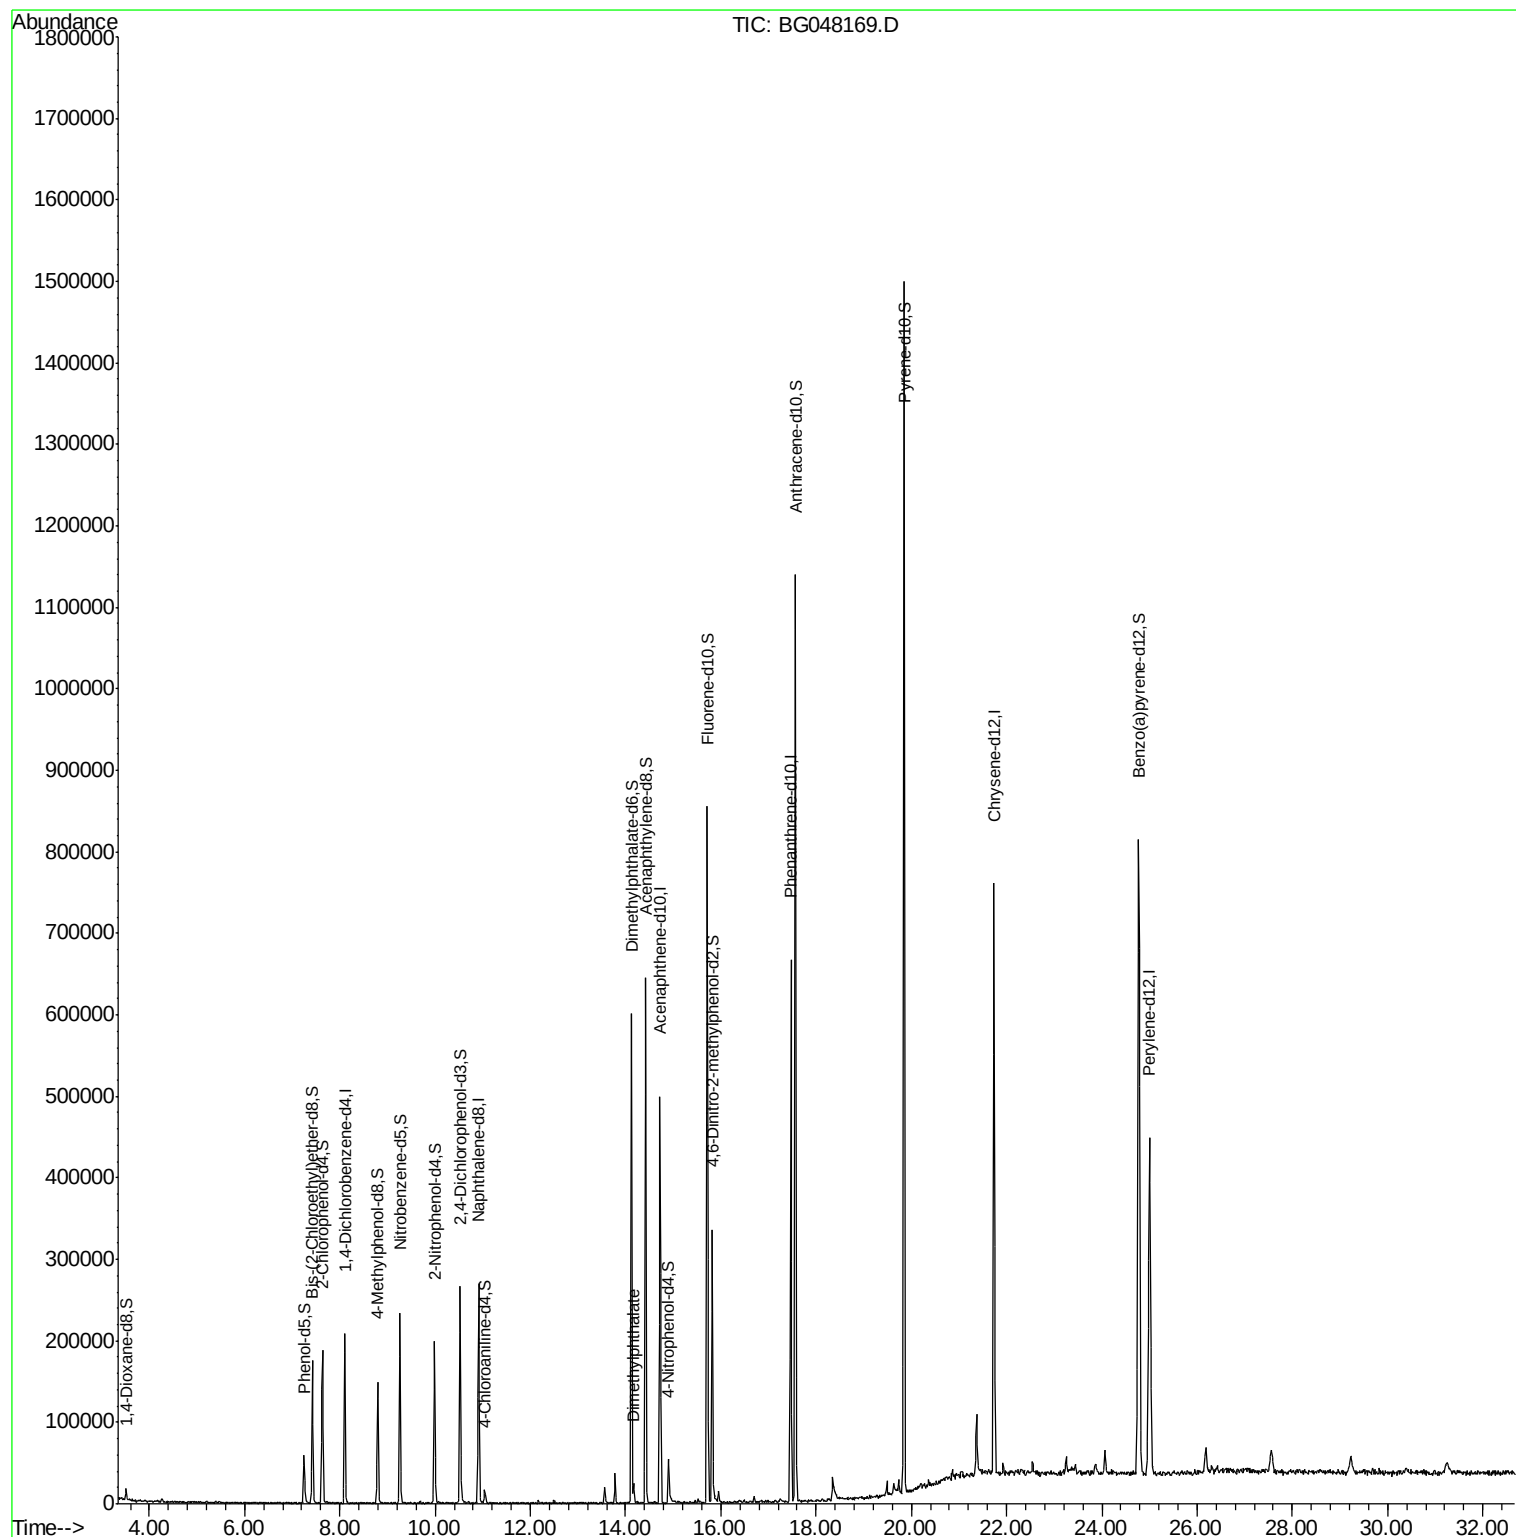

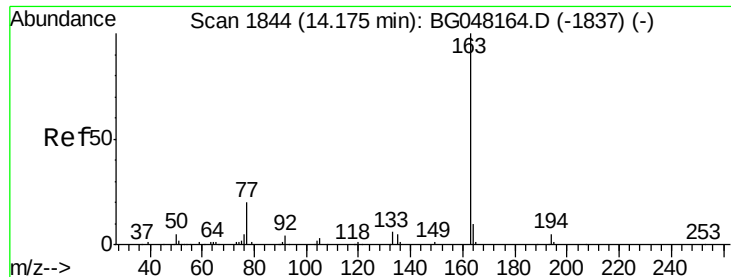

#45

Dimethylphthalate

Concen: 1.161 ng/ul

RT: 14.17 min Scan# 1844

Delta R.T. 0.00 min

Lab File: BG048169.D

Acq: 16 Feb 2021 18:58

Instrument :

BNA_G

ClientSampleId :

DBGL4


Tot Ion:163 Resp: 14636

Ion Ratio Lower Upper

163 100

194 6.0 3.0 4.6#

164 8.3 8.1 12.1

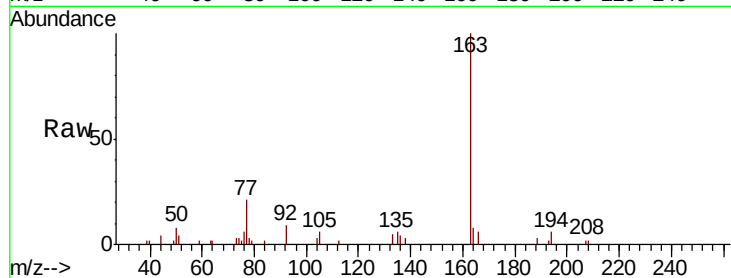

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

