

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021621\
 Data File : BG048167.D
 Acq On : 16 Feb 2021 17:36
 Operator : CG/JU
 Sample : M1407-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBGL6

Quant Time: Feb 16 23:47:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 06:21:07 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	55437	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	216039	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	160761	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	405500	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	426925	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	422883	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.51	96	6508	4.89	ng/uL	0.00
5) Phenol-d5	7.25	99	29866	6.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	77360	27.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	71905	21.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	52636	14.36	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	43679	27.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	52791	27.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	90081	23.56	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	7817	2.07	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	353513	29.69	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	410135	28.18	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	12703	6.28	ng/ul	0.00
58) Fluorene-d10	15.72	176	318747	30.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	66029	26.56	ng/ul	0.00
71) Anthracene-d10	17.57	188	568228	32.68	ng/ul	0.00
79) Pyrene-d10	19.85	212	684601	32.11	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	699835	32.44	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.17	163	13523	1.099	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021621\
Data File : BG048167.D
Acq On : 16 Feb 2021 17:36
Operator : CG/JU
Sample : M1407-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBG L6

Quant Time: Feb 16 23:47:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 15 06:21:07 2021
Response via : Initial Calibration

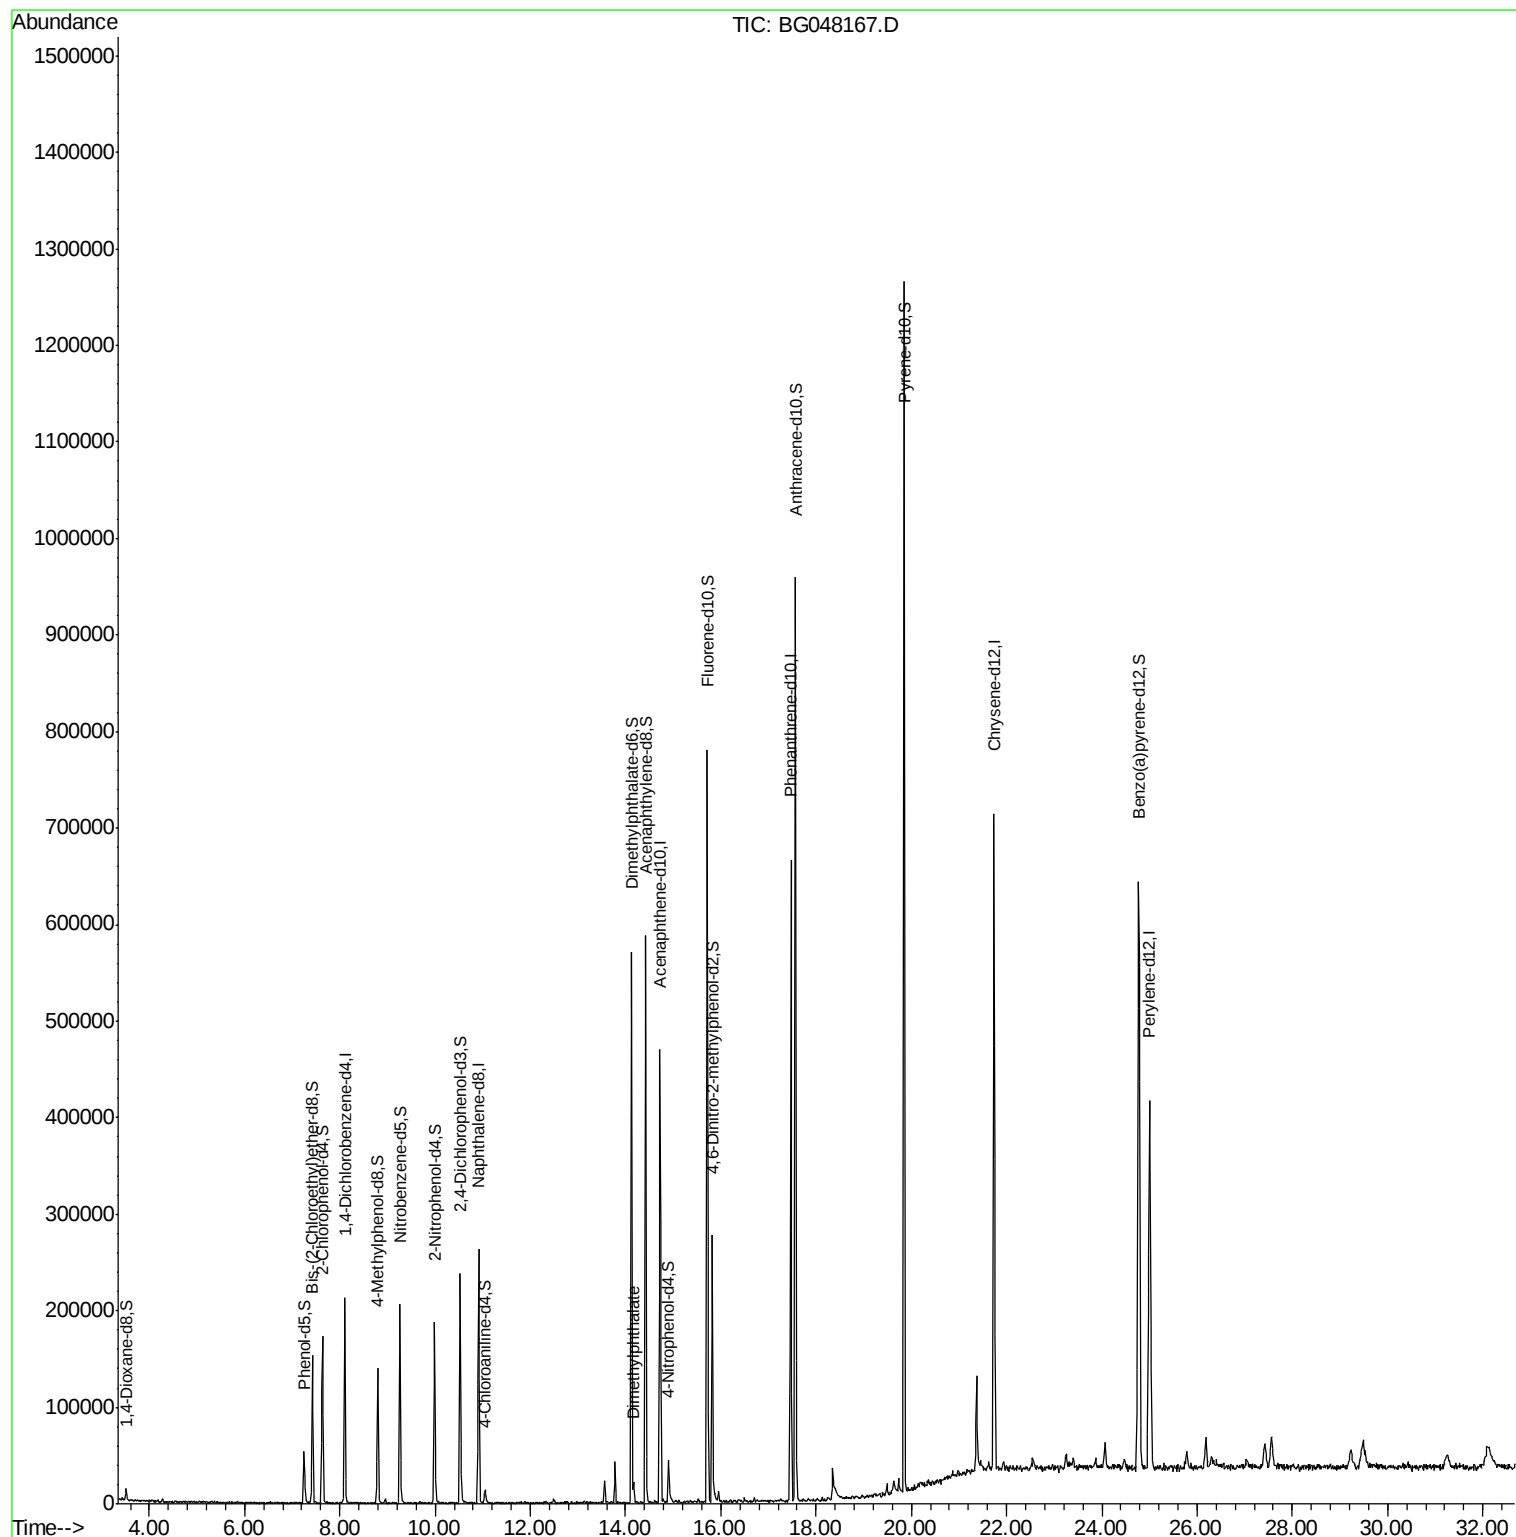

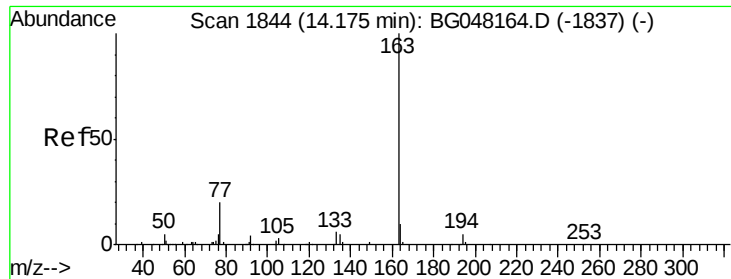

#45

Dimethylphthalate

Concen: 1.099 ng/ul

RT: 14.17 min Scan# 1843

Delta R.T. -0.00 min

Lab File: BG048167.D

Acq: 16 Feb 2021 17:36

Instrument :

BNA_G

ClientSampleId :

DBGL6


Tot Ion:163 Resp: 13523

Ion Ratio Lower Upper

163 100

194 4.8 3.0 4.6#

164 11.2 8.1 12.1

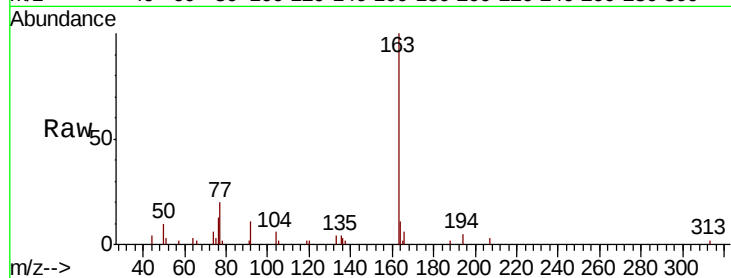

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

