
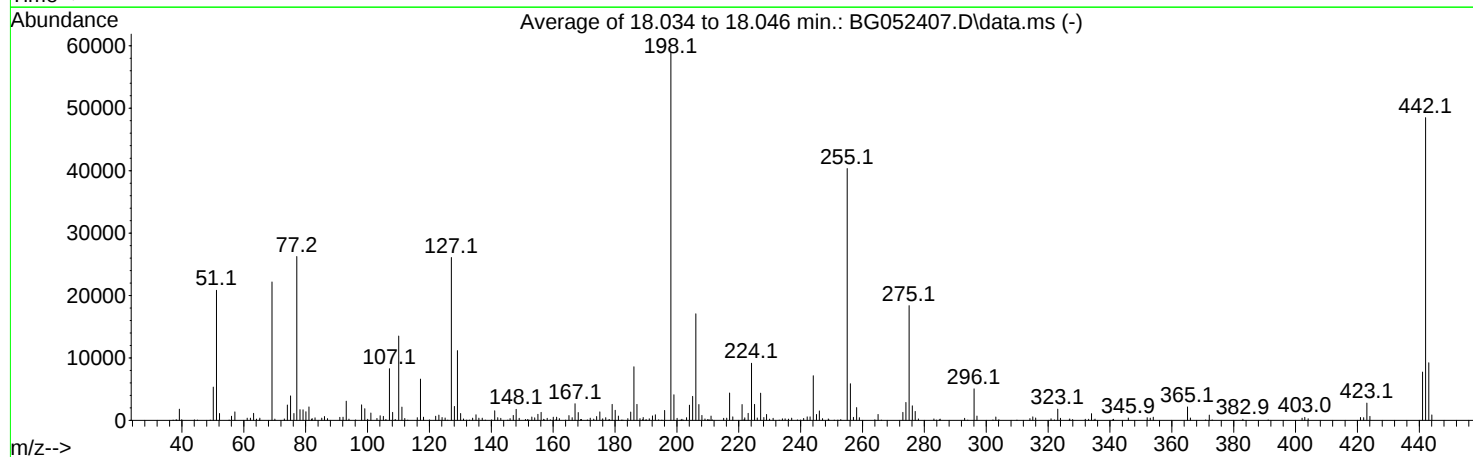


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021622\
 Data File : BG052407.D
 Acq On : 16 Feb 2022 9:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

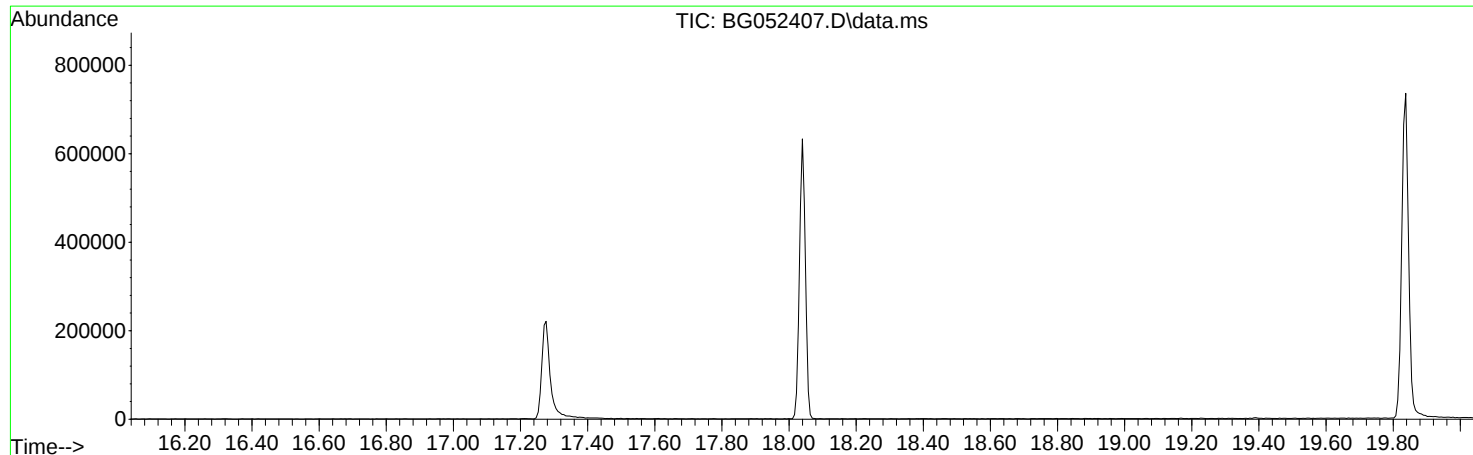




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	20853	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.6	22165	PASS
70	69	0.00	2	0.9	196	PASS
127	198	10	80	44.3	26099	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58931	PASS
199	198	5	9	6.9	4091	PASS
275	198	10	60	31.2	18376	PASS
365	198	1	100	3.7	2165	PASS
441	198	0.01	100	13.1	7733	PASS
442	442	50	100	100.0	48496	PASS
443	442	15	24	19.0	9237	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021622\
Data File : BG052407.D
Acq On : 16 Feb 2022 9:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 16 12:42:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

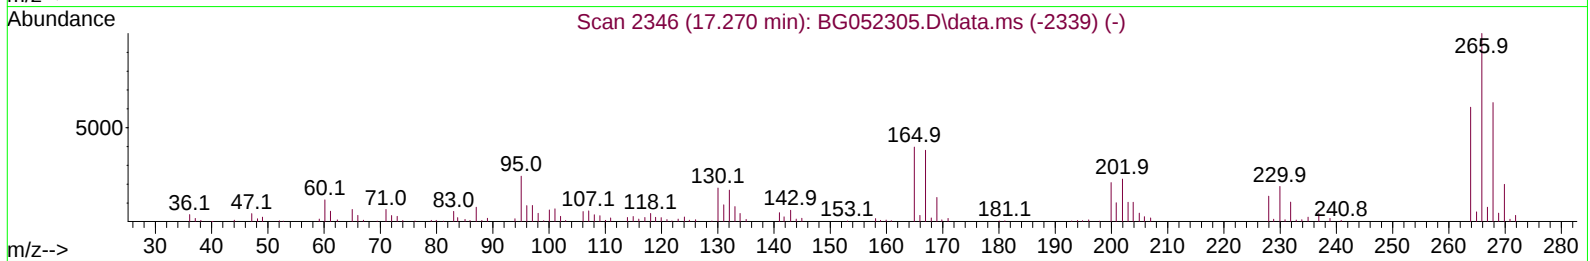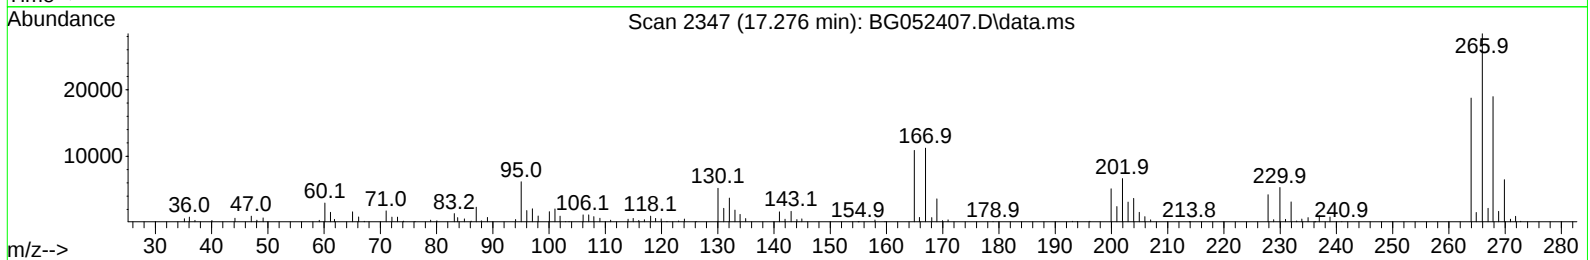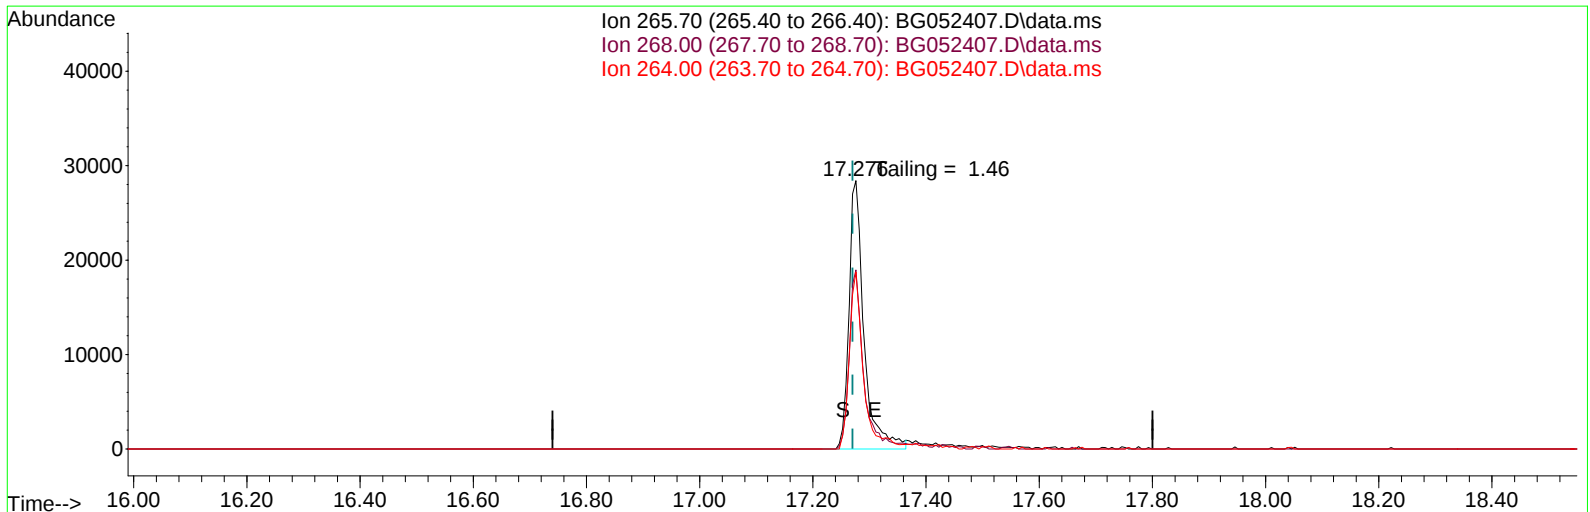

TIC: BG052407.D\data.ms

(70) Pentachlorophenol (C)

17.276min (+ 0.006) 21672.68 ng




response 54122

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	66.69
264.00	65.20	65.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021622\
Data File : BG052407.D
Acq On : 16 Feb 2022 9:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 16 12:42:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

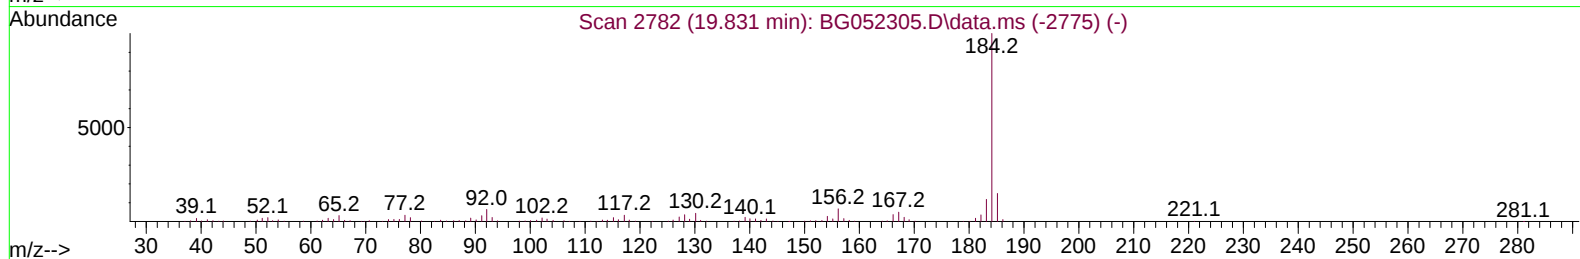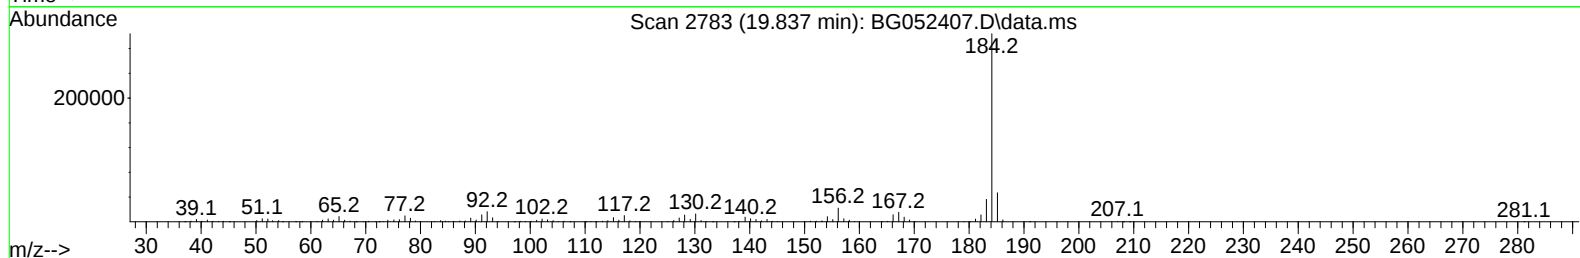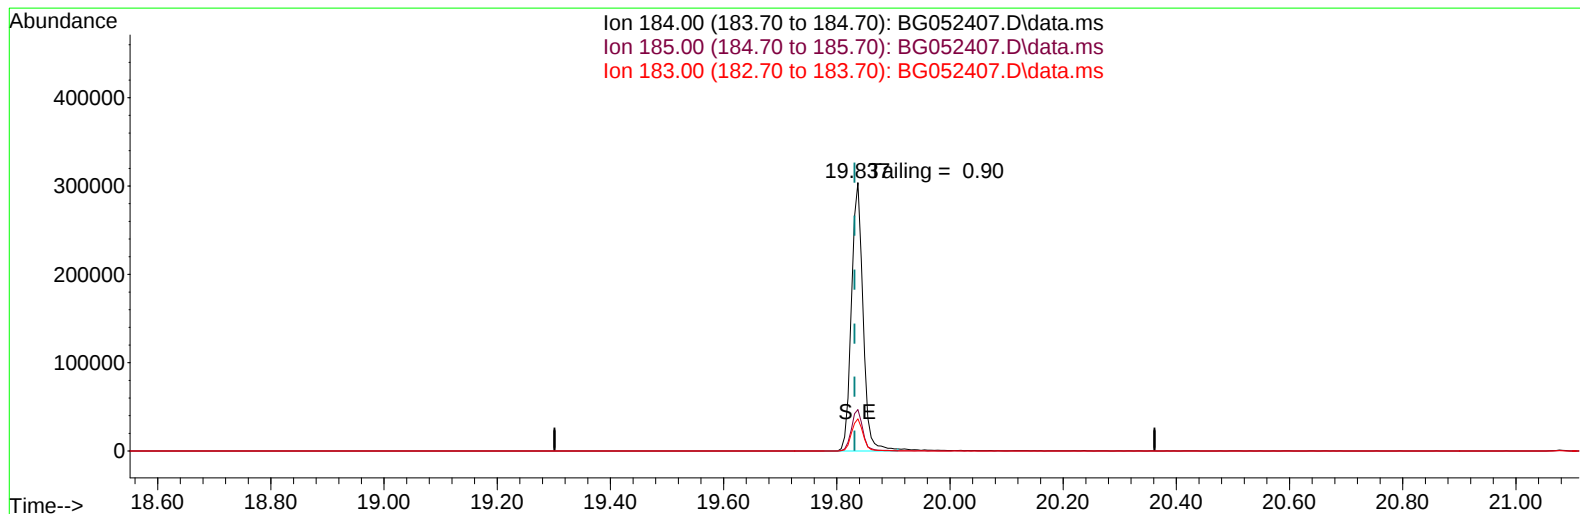

TIC: BG052407.D\data.ms

(77) Benzidine

19.837min (+ 0.006) 0.00 ng

response 438341

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.44
183.00	12.20	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/16/2022	BNA_G	<u>BG052407.D</u>
Compound Name	Response	Retention Time
DDT	236671	21.07
DDD	3490	20.62
DDE	401	20.12
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3891	240562	1.62

Instrument :
BNA_G
ClientSampleId :
DFTPP