


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021623\
Data File : BG056648.D
Acq On : 16 Feb 2023 10:10
Operator : CG/JU
Sample : DFTPP491
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP491

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG021623.M
Title : SVOA CALIBRATION
Last Update : Fri Feb 17 04:20:59 2023

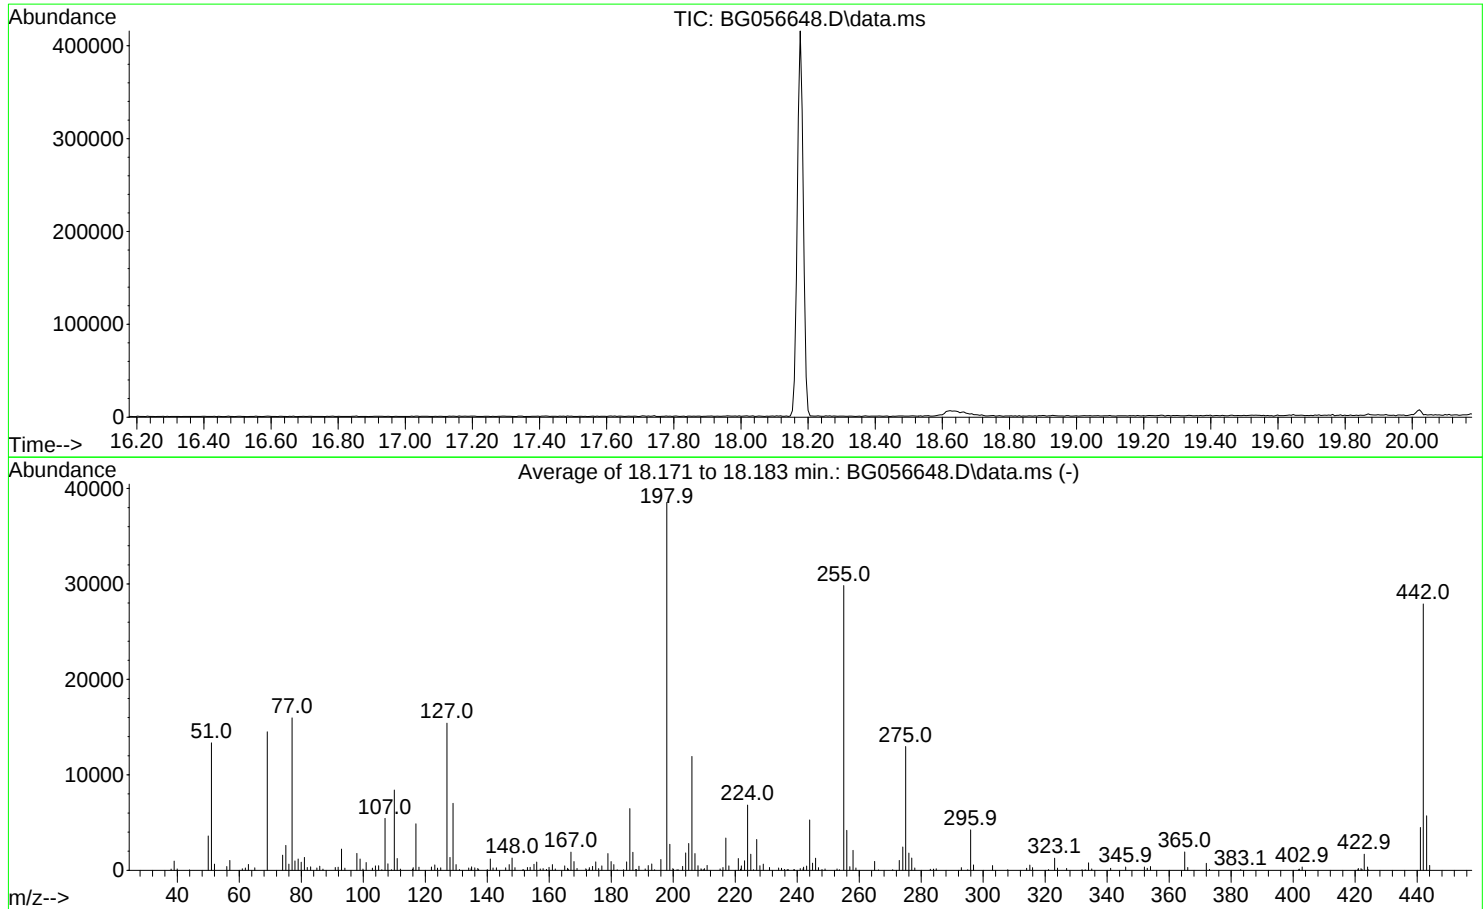

AutoFind: Scans 2533, 2534, 2535; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	13347	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.6	14503	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.0	15419	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38541	PASS
199	198	5	9	7.1	2725	PASS
275	198	10	60	33.6	12965	PASS
365	198	1	100	5.0	1915	PASS
441	198	0.01	100	11.6	4482	PASS
442	198	50	100	72.4	27896	PASS
443	442	15	24	20.5	5713	PASS

m/z	Abundance
44.00	782.0

Instrument :

BNA_G

ClientSampleId :

DFTPP491

m/z	Abundance
39.00	1033.0
40.00	192.0
44.00	831.0
50.00	3696.0
51.00	13919.0
52.00	726.0
56.00	373.0
57.00	1163.0
60.90	226.0
62.00	253.0
63.00	540.0
65.00	252.0
69.00	15090.0
74.00	1591.0
75.00	2539.0
76.00	977.0
77.00	16824.0
78.00	1137.0
79.00	1210.0
79.90	903.0
81.00	1476.0
82.00	318.0
83.00	445.0
85.10	211.0
86.00	487.0
90.90	266.0
91.90	362.0
92.90	2109.0
94.10	396.0
98.00	1994.0
98.90	1299.0
99.90	157.0
100.90	671.0
103.00	176.0
103.90	435.0
104.90	406.0
106.00	200.0
107.00	5007.0
107.90	673.0
110.00	8088.0
111.00	1295.0
115.90	377.0
117.00	4686.0
118.00	420.0
122.00	352.0
123.00	638.0
124.00	176.0
125.00	202.0
127.00	15744.0
127.90	1119.0
128.90	6767.0
130.00	412.0
134.80	507.0
136.00	244.0
137.00	342.0
140.00	225.0
141.00	1099.0
141.90	154.0
142.90	293.0
145.90	233.0
147.00	674.0
148.00	1269.0
149.00	350.0
152.90	263.0
153.80	312.0
155.10	683.0
156.00	828.0
157.10	211.0
158.00	283.0
160.00	250.0
161.00	641.0
161.90	212.0
165.00	414.0
165.90	251.0
167.00	1944.0
168.00	945.0
169.00	223.0
171.80	247.0
172.80	175.0
173.90	509.0
175.00	732.0
176.00	347.0
177.00	404.0
178.90	1549.0
179.90	780.0
180.80	470.0
184.90	823.0
186.00	5779.0
187.00	1568.0
187.90	301.0
188.90	506.0
190.90	228.0

Instrument :
BNA_G
ClientSampleId :
DFTPP491

192.00	539.0
193.00	685.0
196.00	1202.0
197.90	34792.0
198.90	2287.0
199.90	258.0
203.10	323.0
204.00	1493.0
205.00	2515.0
206.00	11406.0
207.00	1713.0
208.00	495.0
209.00	217.0
210.10	388.0
211.00	480.0
216.10	317.0
216.90	2947.0
217.90	306.0
221.00	1207.0
221.90	428.0
223.00	978.0
224.00	6039.0
225.00	1559.0
225.90	197.0
227.00	2648.0
227.90	473.0
229.00	592.0
231.00	241.0
234.00	221.0
241.90	461.0
243.00	414.0
244.00	4827.0
244.90	611.0
245.90	1225.0
246.80	260.0
248.90	165.0
255.00	24896.0
256.00	3906.0
256.90	411.0
258.00	1541.0
259.00	304.0
265.00	1080.0
273.00	955.0
274.00	1897.0
275.00	10333.0
276.00	1639.0
277.00	1195.0
277.90	187.0
283.00	159.0
293.00	203.0
295.90	3156.0
296.90	513.0
303.10	373.0
314.00	231.0
315.10	496.0
315.90	243.0
321.10	207.0
323.10	1051.0
324.10	176.0
334.00	658.0
341.20	235.0
346.00	188.0
352.10	308.0
353.00	209.0
353.90	405.0
365.00	1265.0
366.00	224.0
372.00	515.0
402.90	286.0
420.90	273.0
422.20	277.0
422.90	954.0
423.90	197.0
424.20	190.0
441.00	3242.0
442.00	20512.0
443.00	4231.0
444.00	400.0

Instrument :
BNA_G
ClientSampleId :
DFTPP491

m/z	Abundance
38.00	202.0
39.00	1072.0
44.00	913.0
50.00	4164.0
51.00	15554.0
52.00	841.0
56.00	421.0
57.00	1149.0
61.00	277.0
61.90	331.0
63.00	545.0
65.00	305.0
69.00	16728.0
74.00	1980.0
75.00	2923.0
76.00	952.0
77.00	18136.0
77.90	1085.0
79.00	1226.0
80.00	974.0
81.00	1685.0
82.00	301.0
83.00	410.0
85.00	265.0
85.90	447.0
87.00	199.0
91.00	476.0
91.90	259.0
93.00	2483.0
94.00	295.0
97.90	1976.0
99.00	1415.0
101.00	1001.0
103.00	234.0
103.90	639.0
105.00	590.0
107.00	6553.0
108.00	738.0
110.00	9809.0
110.90	1064.0
111.90	163.0
116.10	410.0
117.00	5751.0
117.90	349.0
122.00	387.0
123.10	568.0
123.90	348.0
125.00	294.0
127.00	18176.0
128.00	1825.0
129.00	8240.0
129.90	846.0
131.00	215.0
134.00	407.0
135.00	521.0
136.00	264.0
136.90	251.0
141.00	1547.0
141.80	346.0
142.90	265.0
146.00	323.0
147.10	573.0
148.00	1658.0
148.90	335.0
151.40	151.0
151.70	157.0
153.00	401.0
153.90	301.0
155.00	628.0
155.90	1092.0
157.10	236.0
158.00	234.0
159.10	283.0
159.90	457.0
161.00	860.0
165.00	453.0
165.90	384.0
167.00	2255.0
168.00	1132.0
171.80	259.0
173.00	524.0
174.00	475.0
175.00	1156.0
175.90	207.0
176.90	666.0
178.90	2135.0
180.00	1070.0
180.90	754.0
184.00	183.0
185.00	1046.0
186.00	7271.0
187.00	2166.0

Instrument :
BNA_G
ClientSampleId :
DFTPP491

189.00	433.0
192.00	445.0
193.00	593.0
194.00	168.0
196.00	1261.0
197.90	44736.0
198.90	3339.0
199.90	269.0
201.60	156.0
203.00	493.0
204.00	2362.0
205.00	3456.0
206.00	14008.0
207.00	2016.0
208.00	715.0
208.90	272.0
209.90	168.0
211.00	617.0
215.10	417.0
216.00	267.0
216.90	4101.0
218.00	571.0
221.00	1541.0
222.00	545.0
223.00	1112.0
224.00	7884.0
225.00	1856.0
226.90	3857.0
228.00	576.0
229.00	738.0
231.00	346.0
234.00	315.0
234.90	437.0
235.90	279.0
237.10	252.0
238.90	226.0
241.00	281.0
242.10	512.0
243.00	439.0
244.00	6017.0
245.00	929.0
246.00	1518.0
246.90	435.0
248.00	227.0
249.00	283.0
252.80	216.0
255.00	35136.0
256.00	4506.0
256.90	412.0
258.00	2570.0
258.90	412.0
264.90	965.0
266.20	152.0
270.80	187.0
272.90	1179.0
274.10	2552.0
275.00	16201.0
276.00	2346.0
277.00	1265.0
278.00	321.0
282.90	158.0
283.90	202.0
284.90	294.0
292.90	304.0
295.00	157.0
296.00	5037.0
296.90	648.0
303.00	549.0
307.90	160.0
314.00	236.0
315.00	557.0
316.00	381.0
323.00	1373.0
324.00	301.0
326.90	328.0
331.90	159.0
334.00	919.0
335.10	227.0
341.00	225.0
346.00	505.0
352.00	382.0
353.00	219.0
353.90	302.0
365.00	2452.0
366.00	400.0
372.00	960.0
401.80	232.0
402.80	342.0
421.10	151.0
421.90	328.0
423.00	2034.0
424.00	279.0
441.00	5113.0
442.00	31464.0
443.00	6462.0
444.10	640.0

Instrument :
BNA_G
ClientSampleId :
DFTPP491

m/z	Abundance
38.00	190.0
39.00	781.0
39.90	240.0
43.90	751.0
50.00	2919.0
51.00	10569.0
52.00	376.0
55.90	386.0
56.90	793.0
62.00	159.0
62.90	756.0
65.00	198.0
69.00	11692.0
74.00	1209.0
75.00	2365.0
77.00	12943.0
78.00	705.0
79.00	1120.0
79.90	666.0
81.00	900.0
81.90	281.0
82.90	229.0
85.00	273.0
86.00	372.0
87.00	182.0
91.00	168.0
91.90	375.0
93.00	2071.0
98.00	1337.0
98.90	836.0
99.90	214.0
101.00	773.0
102.90	258.0
103.80	307.0
105.00	457.0
107.00	4781.0
107.90	645.0
109.10	191.0
110.00	7335.0
111.00	1323.0
112.00	235.0
116.10	423.0
117.00	4185.0
118.00	223.0
122.00	279.0
123.00	472.0
123.90	178.0
125.00	297.0
127.00	12337.0
128.00	1132.0
129.00	6069.0
130.00	509.0
134.00	347.0
134.90	563.0
135.90	266.0
137.20	249.0
141.00	897.0
141.80	207.0
143.00	220.0
145.90	245.0
147.10	529.0
148.00	918.0
149.00	163.0
153.00	245.0
153.90	318.0
155.00	559.0
156.00	700.0
160.00	224.0
161.00	282.0
162.00	215.0
165.00	517.0
166.10	326.0
167.00	1503.0
168.00	659.0
168.80	186.0
169.00	184.0
172.00	191.0
172.90	296.0
174.00	261.0
175.00	760.0
177.00	337.0
178.90	1562.0
180.00	894.0
180.90	556.0
181.90	177.0
185.00	783.0
186.00	6335.0
187.00	1922.0
188.10	232.0
188.90	323.0
191.00	205.0
191.90	481.0

Instrument :
BNA_G
ClientSampleId :
DFTPP491

193.10	692.0
196.00	915.0
197.90	36096.0
198.90	2550.0
200.10	268.0
201.20	173.0
203.00	403.0
204.00	1618.0
205.00	2471.0
206.00	10369.0
207.00	1512.0
208.00	243.0
209.20	155.0
209.80	181.0
210.90	421.0
216.00	317.0
217.00	3082.0
217.90	484.0
221.00	951.0
221.70	357.0
222.10	413.0
223.00	885.0
224.00	6586.0
225.00	1653.0
227.00	3172.0
228.00	373.0
229.10	633.0
231.10	304.0
234.00	189.0
235.00	205.0
236.80	210.0
239.10	197.0
240.90	234.0
242.00	475.0
243.10	490.0
244.00	4966.0
244.90	707.0
246.00	1048.0
246.90	151.0
252.90	213.0
253.60	160.0
255.00	29464.0
256.00	4156.0
257.00	293.0
258.00	2177.0
265.00	763.0
273.00	950.0
274.00	2859.0
275.00	12362.0
276.00	1438.0
276.90	1395.0
278.00	209.0
284.00	152.0
284.80	180.0
293.00	348.0
296.00	4485.0
296.90	537.0
302.90	563.0
314.00	173.0
315.00	573.0
316.00	218.0
323.00	1352.0
323.90	215.0
326.90	248.0
332.90	191.0
334.00	788.0
335.00	217.0
341.10	161.0
345.90	346.0
351.90	357.0
352.90	210.0
354.00	467.0
365.00	2029.0
366.00	239.0
372.00	713.0
373.00	296.0
383.10	209.0
402.00	364.0
403.00	413.0
421.00	421.0
421.90	204.0
423.00	2074.0
424.00	542.0
441.10	5091.0
442.00	31712.0
443.10	6446.0
444.00	472.0

Instrument :
BNA_G
ClientSampleId :
DFTPP491