

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021716\
 Data File : BG020926.D
 Acq On : 17 Feb 2016 14:50
 Operator : SJ/UM
 Sample : H1477-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 0311-S03-0003

Quant Time: Feb 18 01:05:00 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 18 00:59:48 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.26	152	15943	20.00	ng/ul	0.00
18) Naphthalene-d8	11.09	136	86701	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.87	164	55459	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.61	188	122637	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	114183	20.00	ng/ul	0.00
86) Perylene-d12	25.26	264	106864	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.60	96	2109	6.42	ng/uL	0.00
5) Phenol-d5	7.40	99	47885	29.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	27215	31.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.79	132	40020	31.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	44240	31.51	ng/ul	0.00
19) Nitrobenzene-d5	9.43	128	22255	31.99	ng/ul	0.00
22) 2-Nitrophenol-d4	10.16	143	24354	35.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.69	165	41318	31.03	ng/ul	0.00
29) 4-Chloroaniline-d4	11.21	131	69729	39.32	ng/ul	0.00
44) Dimethylphthalate-d6	14.27	166	155649	32.62	ng/ul	0.00
47) Acenaphthylene-d8	14.57	160	192504	33.02	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	26528	27.77	ng/ul	0.00
58) Fluorene-d10	15.86	176	135827	33.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	15112	25.43	ng/ul	0.00
71) Anthracene-d10	17.71	188	200016	33.01	ng/ul	0.00
79) Pyrene-d10	19.97	212	196258	33.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.03	264	198910	33.59	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.31	163	79184	15.94	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021716\
Data File : BG020926.D
Acq On : 17 Feb 2016 14:50
Operator : SJ/UM
Sample : H1477-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0311-S03-0003

Quant Time: Feb 18 01:05:00 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 18 00:59:48 2016
Response via : Initial Calibration

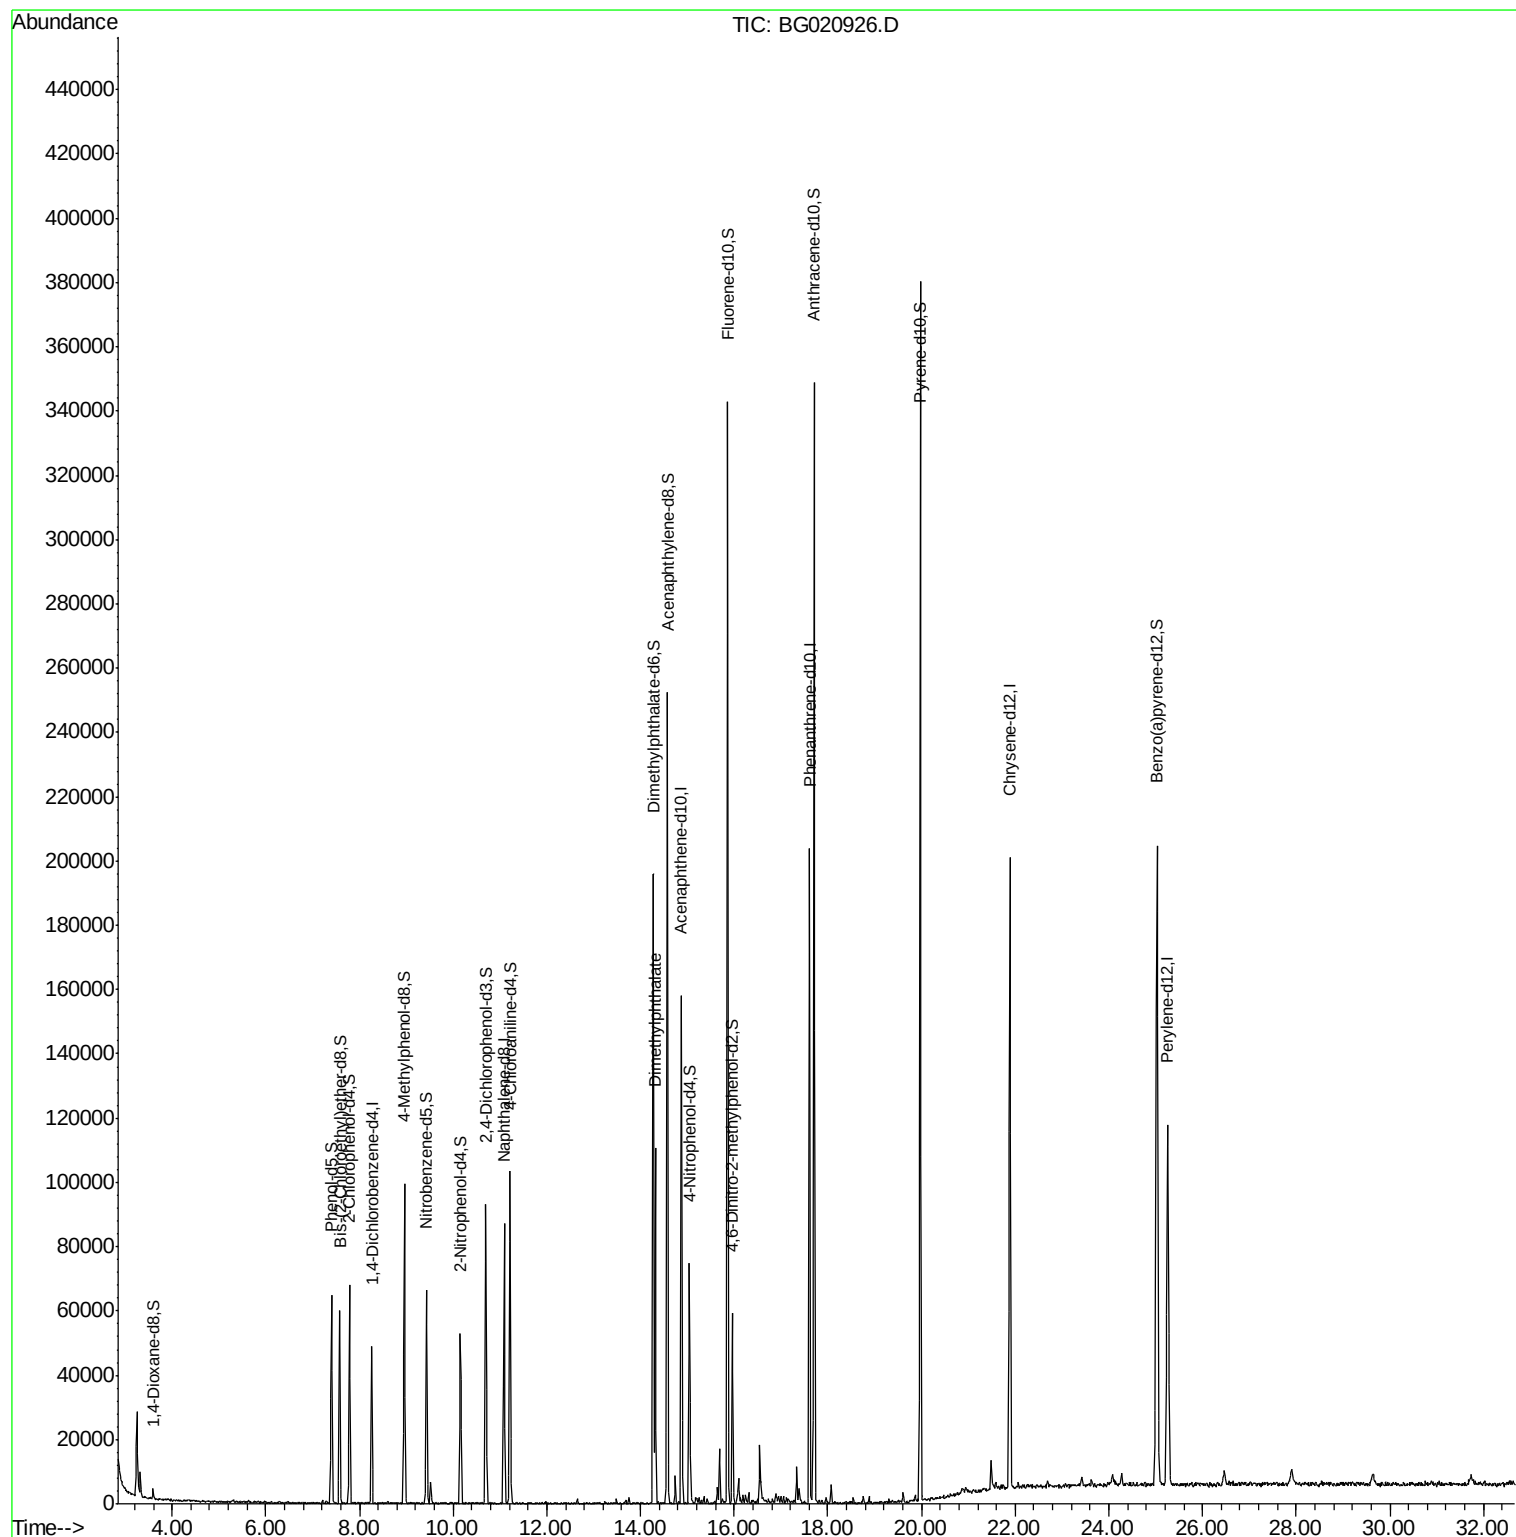

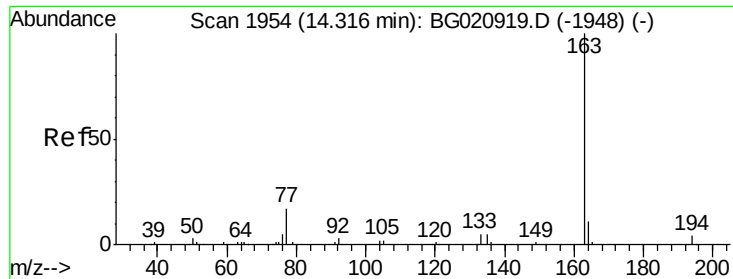

#45

Dimethylphthalate

Concen: 15.94 ng/ul

RT: 14.31 min Scan# 1953

Delta R.T. -0.00 min

Lab File: BG020926.D


Acq: 17 Feb 2016 14:50

Instrument :

BNA_G

ClientSampleId :

0311-S03-0003

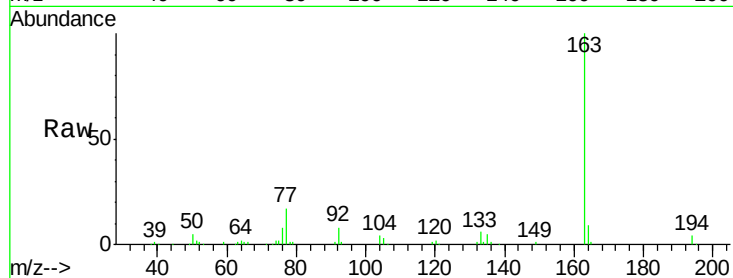


Tgt Ion:163 Resp: 79184

Ion Ratio Lower Upper

163 100

194 3.6 3.0 4.6

164 9.3 7.7 11.5

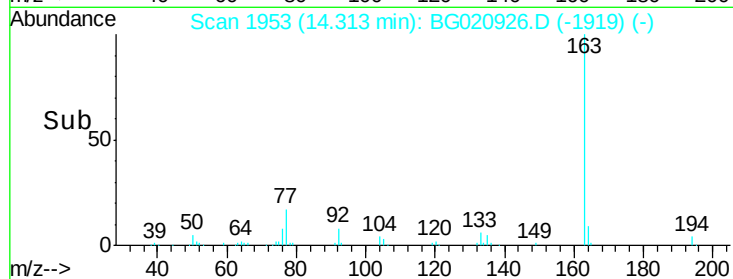

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

