

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021716\
 Data File : BG020929.D
 Acq On : 17 Feb 2016 16:48
 Operator : SJ/UM
 Sample : H1477-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 0311-S04-0312

Quant Time: Feb 18 01:05:22 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 18 00:59:48 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.26	152	16482	20.00	ng/ul	0.00
18) Naphthalene-d8	11.09	136	89238	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.88	164	56544	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.61	188	123275	20.00	ng/ul	0.00
78) Chrysene-d12	21.88	240	113874	20.00	ng/ul	0.00
86) Perylene-d12	25.26	264	106374	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.60	96	2009	5.92	ng/uL	0.00
5) Phenol-d5	7.40	99	48152	28.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.57	67	27462	30.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.79	132	40253	30.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.95	113	43257	29.80	ng/ul	0.00
19) Nitrobenzene-d5	9.43	128	22364	31.23	ng/ul	0.00
22) 2-Nitrophenol-d4	10.16	143	23934	33.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	41883	30.56	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	68026	37.27	ng/ul	0.00
44) Dimethylphthalate-d6	14.27	166	156456	32.16	ng/ul	0.00
47) Acenaphthylene-d8	14.57	160	192775	32.43	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	27144	27.87	ng/ul	0.00
58) Fluorene-d10	15.86	176	136264	32.91	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	15463	25.88	ng/ul	0.00
71) Anthracene-d10	17.71	188	203437	33.40	ng/ul	0.00
79) Pyrene-d10	19.97	212	202222	34.54	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.03	264	202094	34.28	ng/ul	0.00


Target Compounds						Qvalue
45) Dimethylphthalate	14.32	163	66219	13.07	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021716\
Data File : BG020929.D
Acq On : 17 Feb 2016 16:48
Operator : SJ/UM
Sample : H1477-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0311-S04-0312

Quant Time: Feb 18 01:05:22 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 18 00:59:48 2016
Response via : Initial Calibration

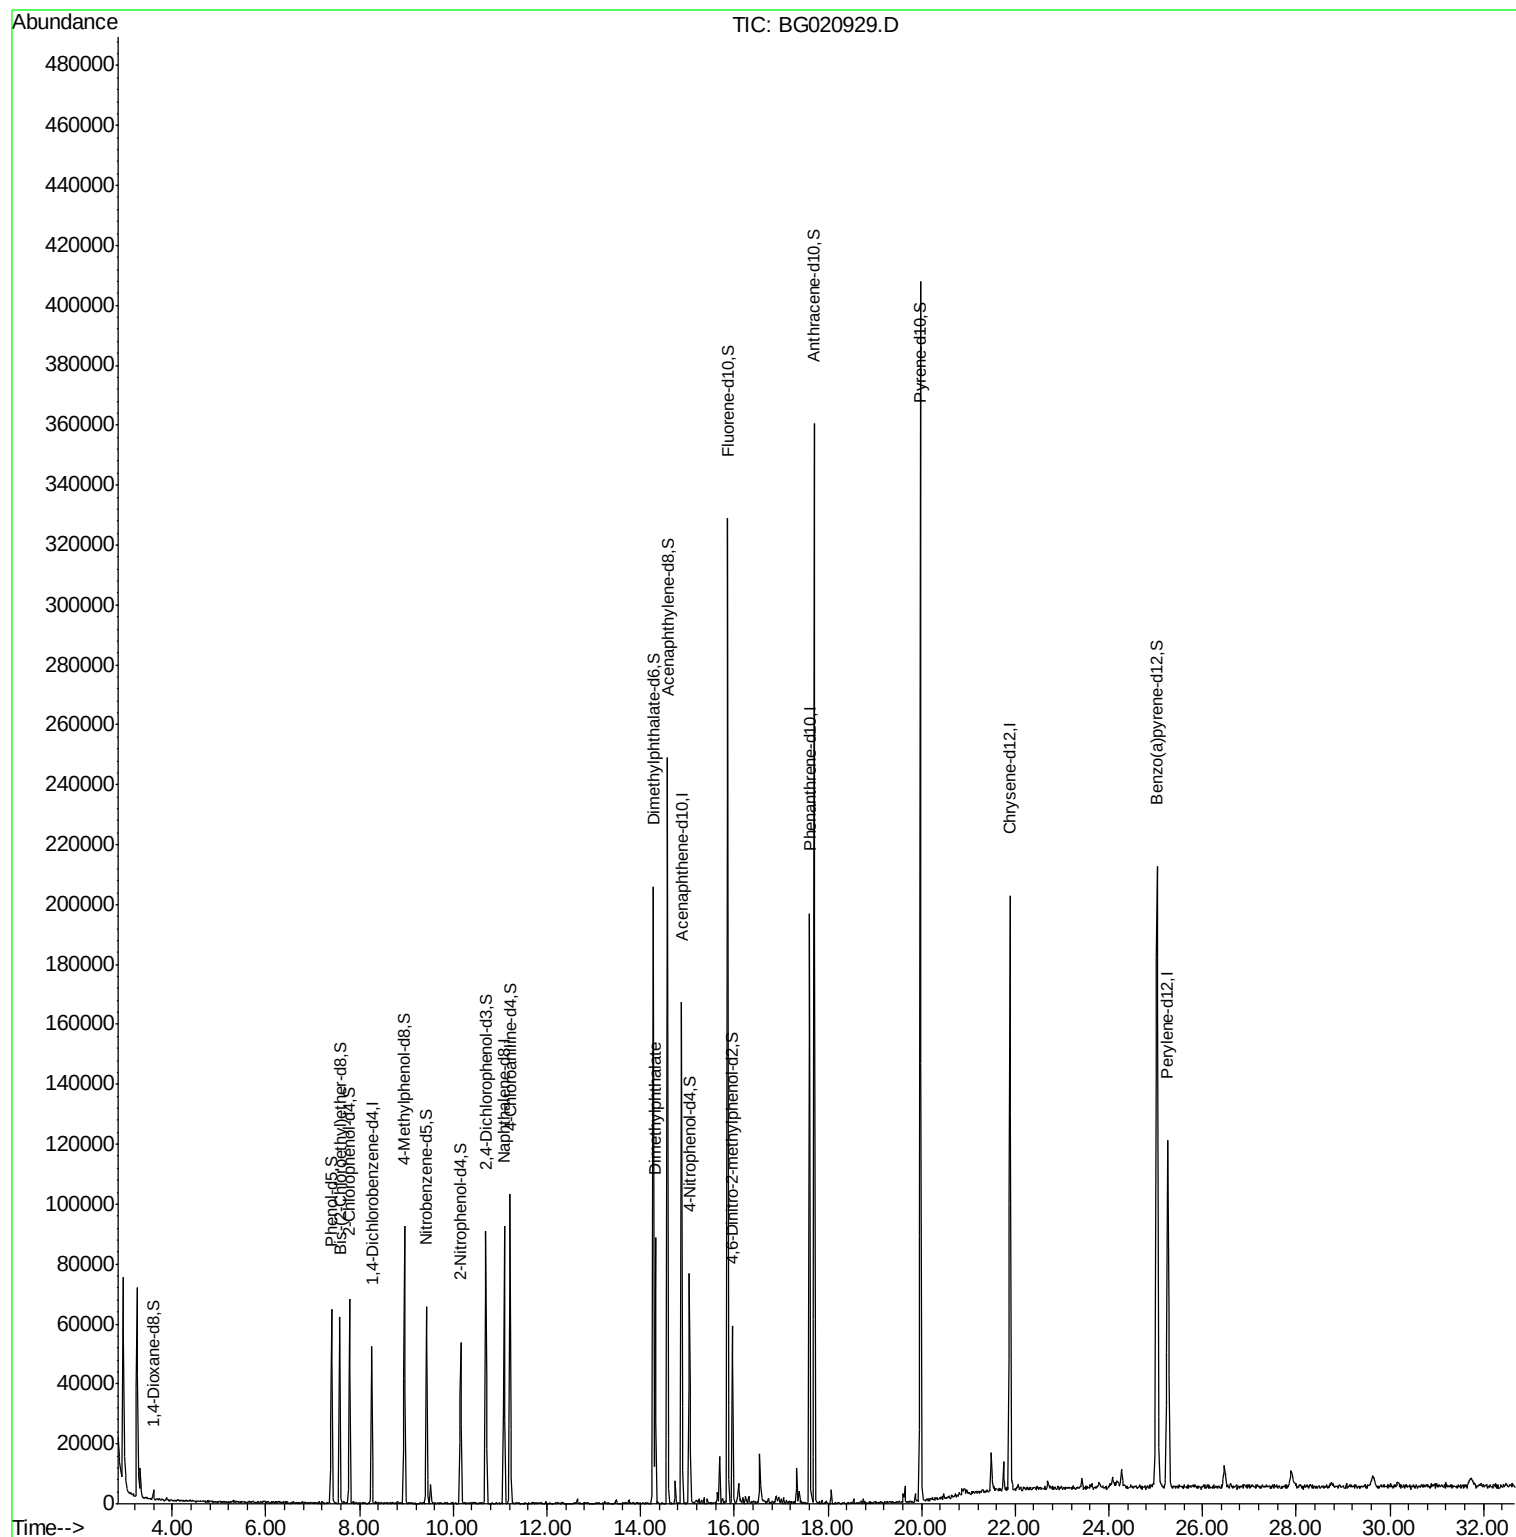

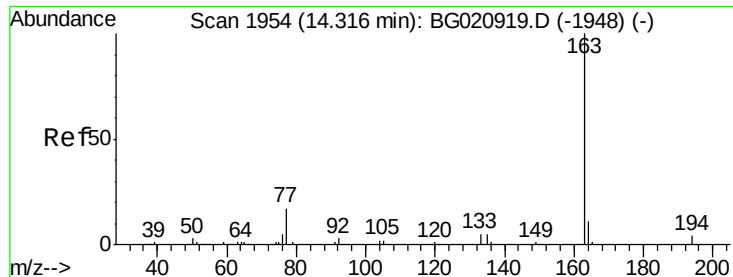

#45

Dimethylphthalate

Concen: 13.07 ng/ul

RT: 14.32 min Scan# 1954

Delta R.T. 0.00 min

Lab File: BG020929.D


Acq: 17 Feb 2016 16:48

Instrument :

BNA_G

ClientSampleId :

0311-S04-0312

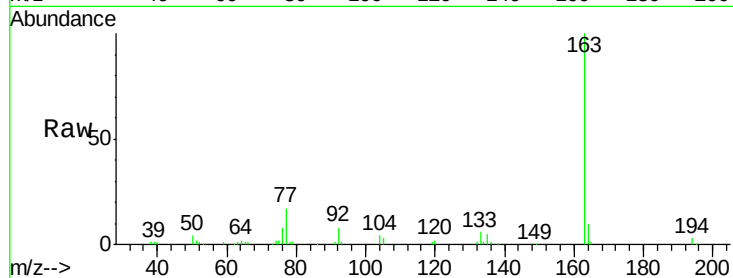

Tgt Ion:163 Resp: 66219

Ion Ratio Lower Upper

163 100

194 3.3 3.0 4.6

164 10.3 7.7 11.5

