

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021716\
 Data File : BG020930.D
 Acq On : 17 Feb 2016 17:27
 Operator : SJ/UM
 Sample : H1477-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 0311-S05-0003

Quant Time: Feb 18 01:05:28 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 18 00:59:48 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.26	152	17448	20.00	ng/ul	0.00
18) Naphthalene-d8	11.09	136	96892	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.87	164	61432	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.61	188	132290	20.00	ng/ul	0.00
78) Chrysene-d12	21.88	240	119785	20.00	ng/ul	0.00
86) Perylene-d12	25.25	264	113569	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.59	96	1878	5.23	ng/uL	0.00
5) Phenol-d5	7.40	99	48657	27.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.57	67	27510	29.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.79	132	40620	29.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	41633	27.10	ng/ul	0.00
19) Nitrobenzene-d5	9.43	128	23433	30.14	ng/ul	0.00
22) 2-Nitrophenol-d4	10.16	143	25078	32.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	44679	30.02	ng/ul	0.00
29) 4-Chloroaniline-d4	11.21	131	65666	33.13	ng/ul	0.00
44) Dimethylphthalate-d6	14.27	166	162914	30.82	ng/ul	0.00
47) Acenaphthylene-d8	14.57	160	200653	31.07	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	28937	27.34	ng/ul	0.00
58) Fluorene-d10	15.86	176	143904	31.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	18082	28.20	ng/ul	0.00
71) Anthracene-d10	17.71	188	211432	32.35	ng/ul	0.00
79) Pyrene-d10	19.97	212	203122	32.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.03	264	206567	32.82	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.32	163	62804	11.41	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021716\
Data File : BG020930.D
Acq On : 17 Feb 2016 17:27
Operator : SJ/UM
Sample : H1477-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0311-S05-0003

Quant Time: Feb 18 01:05:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 18 00:59:48 2016
Response via : Initial Calibration

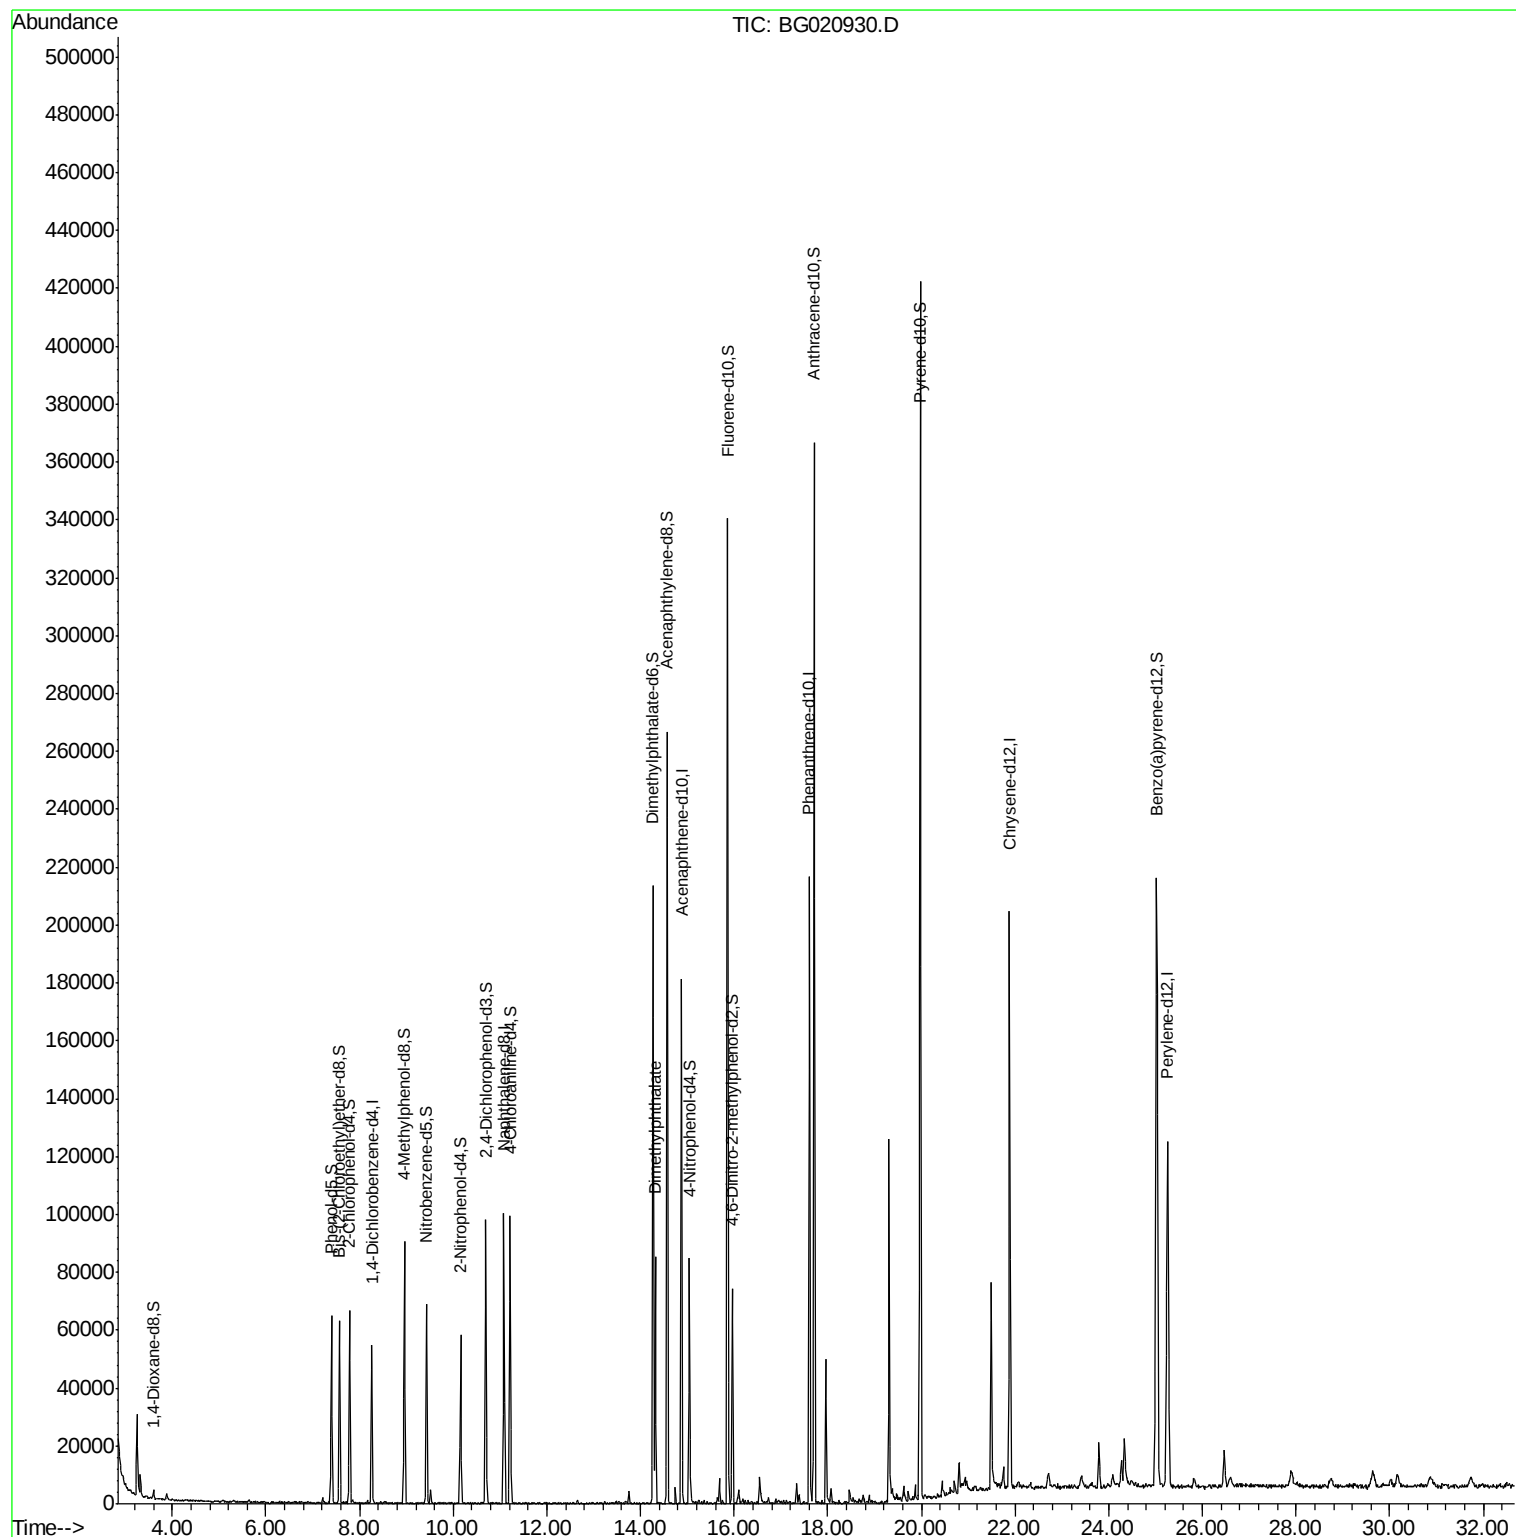

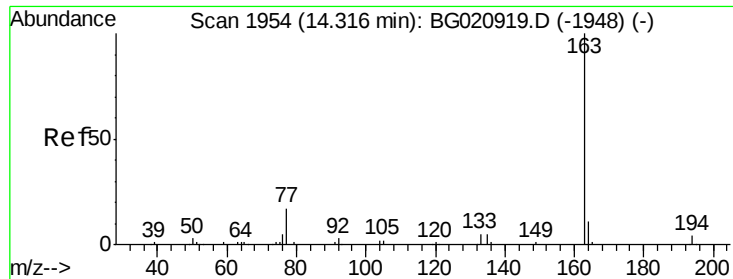

#45

Dimethylphthalate

Concen: 11.41 ng/ul

RT: 14.32 min Scan# 1954

Delta R.T. 0.00 min

Lab File: BG020930.D


Acq: 17 Feb 2016 17:27

Instrument :

BNA_G

ClientSampleId :

0311-S05-0003

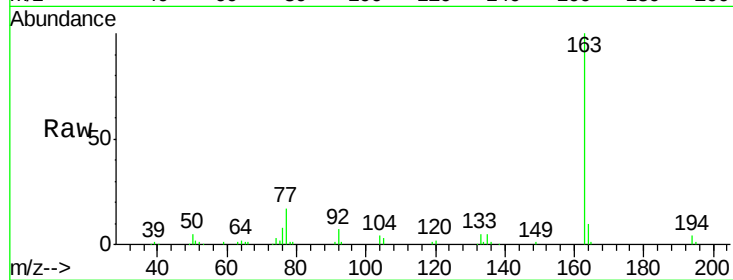

Tgt Ion:163 Resp: 62804

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6

164 9.9 7.7 11.5

