

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021716\
 Data File : BG020922.D
 Acq On : 17 Feb 2016 12:13
 Operator : SJ/UM
 Sample : H1477-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 0311-S01-0312

Quant Time: Feb 18 01:04:28 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 18 00:59:48 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.26	152	15920	20.00	ng/ul	0.00
18) Naphthalene-d8	11.08	136	84333	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.87	164	52743	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.61	188	120166	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	112320	20.00	ng/ul	0.00
86) Perylene-d12	25.26	264	103248	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.60	96	2075	6.33	ng/uL	0.00
5) Phenol-d5	7.40	99	50437	31.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.57	67	28910	33.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.79	132	42169	33.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	43184	30.80	ng/ul	0.00
19) Nitrobenzene-d5	9.43	128	23458	34.66	ng/ul	0.00
22) 2-Nitrophenol-d4	10.16	143	25273	37.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	43046	33.23	ng/ul	0.00
29) 4-Chloroaniline-d4	11.21	131	64205	37.22	ng/ul	0.00
44) Dimethylphthalate-d6	14.27	166	164651	36.28	ng/ul	0.00
47) Acenaphthylene-d8	14.57	160	200892	36.24	ng/ul	0.00
52) 4-Nitrophenol-d4	15.04	143	28045	30.87	ng/ul	0.00
58) Fluorene-d10	15.86	176	141656	36.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	17116	29.39	ng/ul	0.00
71) Anthracene-d10	17.71	188	214755	36.17	ng/ul	0.00
79) Pyrene-d10	19.97	212	212211	36.75	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.03	264	209056	36.54	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.32	163	64926	13.74	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021716\
Data File : BG020922.D
Acq On : 17 Feb 2016 12:13
Operator : SJ/UM
Sample : H1477-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0311-S01-0312

Quant Time: Feb 18 01:04:28 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 18 00:59:48 2016
Response via : Initial Calibration

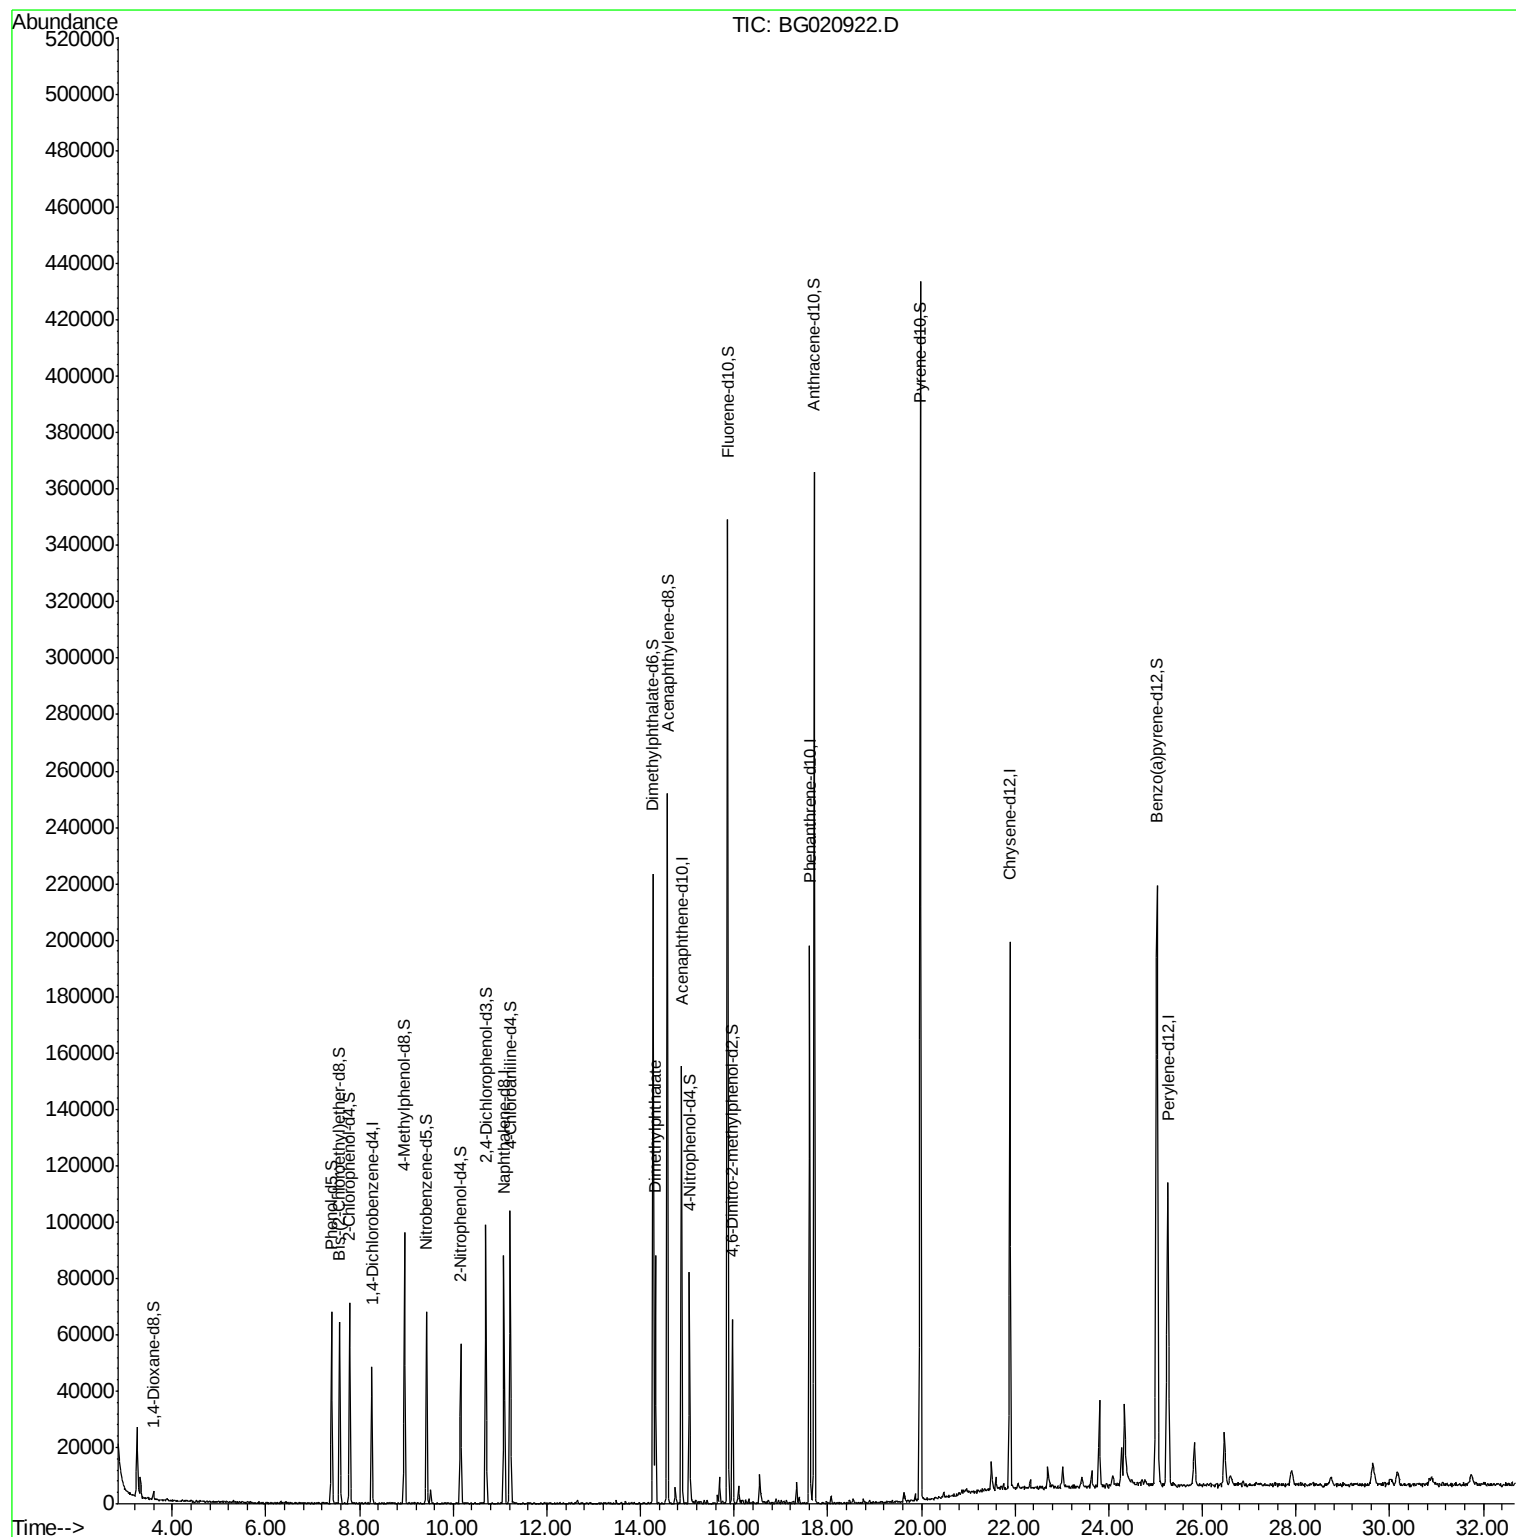

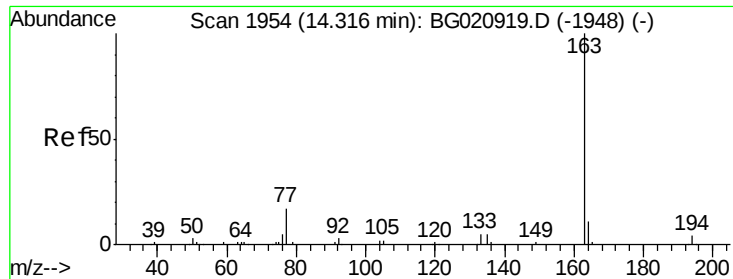

#45

Dimethylphthalate

Concen: 13.74 ng/ul

RT: 14.32 min Scan# 1954

Delta R.T. 0.00 min

Lab File: BG020922.D


Acq: 17 Feb 2016 12:13

Instrument :

BNA_G

ClientSampleId :

0311-S01-0312

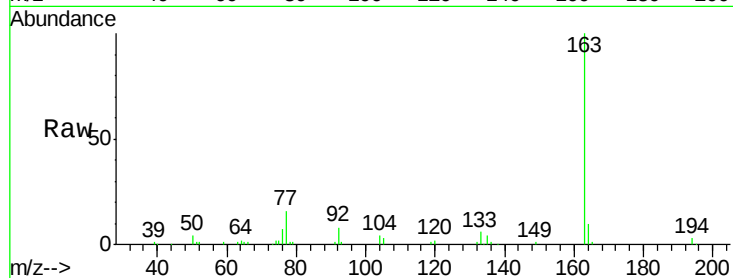

Tot Ion:163 Resp: 64926

Ion Ratio Lower Upper

163 100

194 3.4 3.0 4.6

164 10.4 7.7 11.5

