

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021716\
 Data File : BG020925.D
 Acq On : 17 Feb 2016 14:11
 Operator : SJ/UM
 Sample : H1477-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 0311-S35-0003

Quant Time: Feb 18 01:04:52 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 18 00:59:48 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.26	152	17010	20.00	ng/ul	0.00
18) Naphthalene-d8	11.09	136	89304	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.88	164	56426	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.61	188	124339	20.00	ng/ul	0.00
78) Chrysene-d12	21.88	240	115472	20.00	ng/ul	0.00
86) Perylene-d12	25.26	264	107878	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.60	96	1878	5.36	ng/uL	0.00
5) Phenol-d5	7.40	99	44773	25.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.57	67	25511	27.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.79	132	37551	27.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	40725	27.19	ng/ul	0.00
19) Nitrobenzene-d5	9.43	128	21037	29.36	ng/ul	0.00
22) 2-Nitrophenol-d4	10.16	143	22309	31.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.69	165	38233	27.87	ng/ul	0.00
29) 4-Chloroaniline-d4	11.21	131	63678	34.86	ng/ul	0.00
44) Dimethylphthalate-d6	14.27	166	142557	29.36	ng/ul	0.00
47) Acenaphthylene-d8	14.57	160	176754	29.80	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	24036	24.73	ng/ul	0.00
58) Fluorene-d10	15.86	176	124124	30.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	13584	22.54	ng/ul	0.00
71) Anthracene-d10	17.71	188	185046	30.12	ng/ul	0.00
79) Pyrene-d10	19.98	212	182561	30.75	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.03	264	181070	30.29	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.31	163	61216	12.11	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021716\
Data File : BG020925.D
Acq On : 17 Feb 2016 14:11
Operator : SJ/UM
Sample : H1477-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0311-S35-0003

Quant Time: Feb 18 01:04:52 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 18 00:59:48 2016
Response via : Initial Calibration

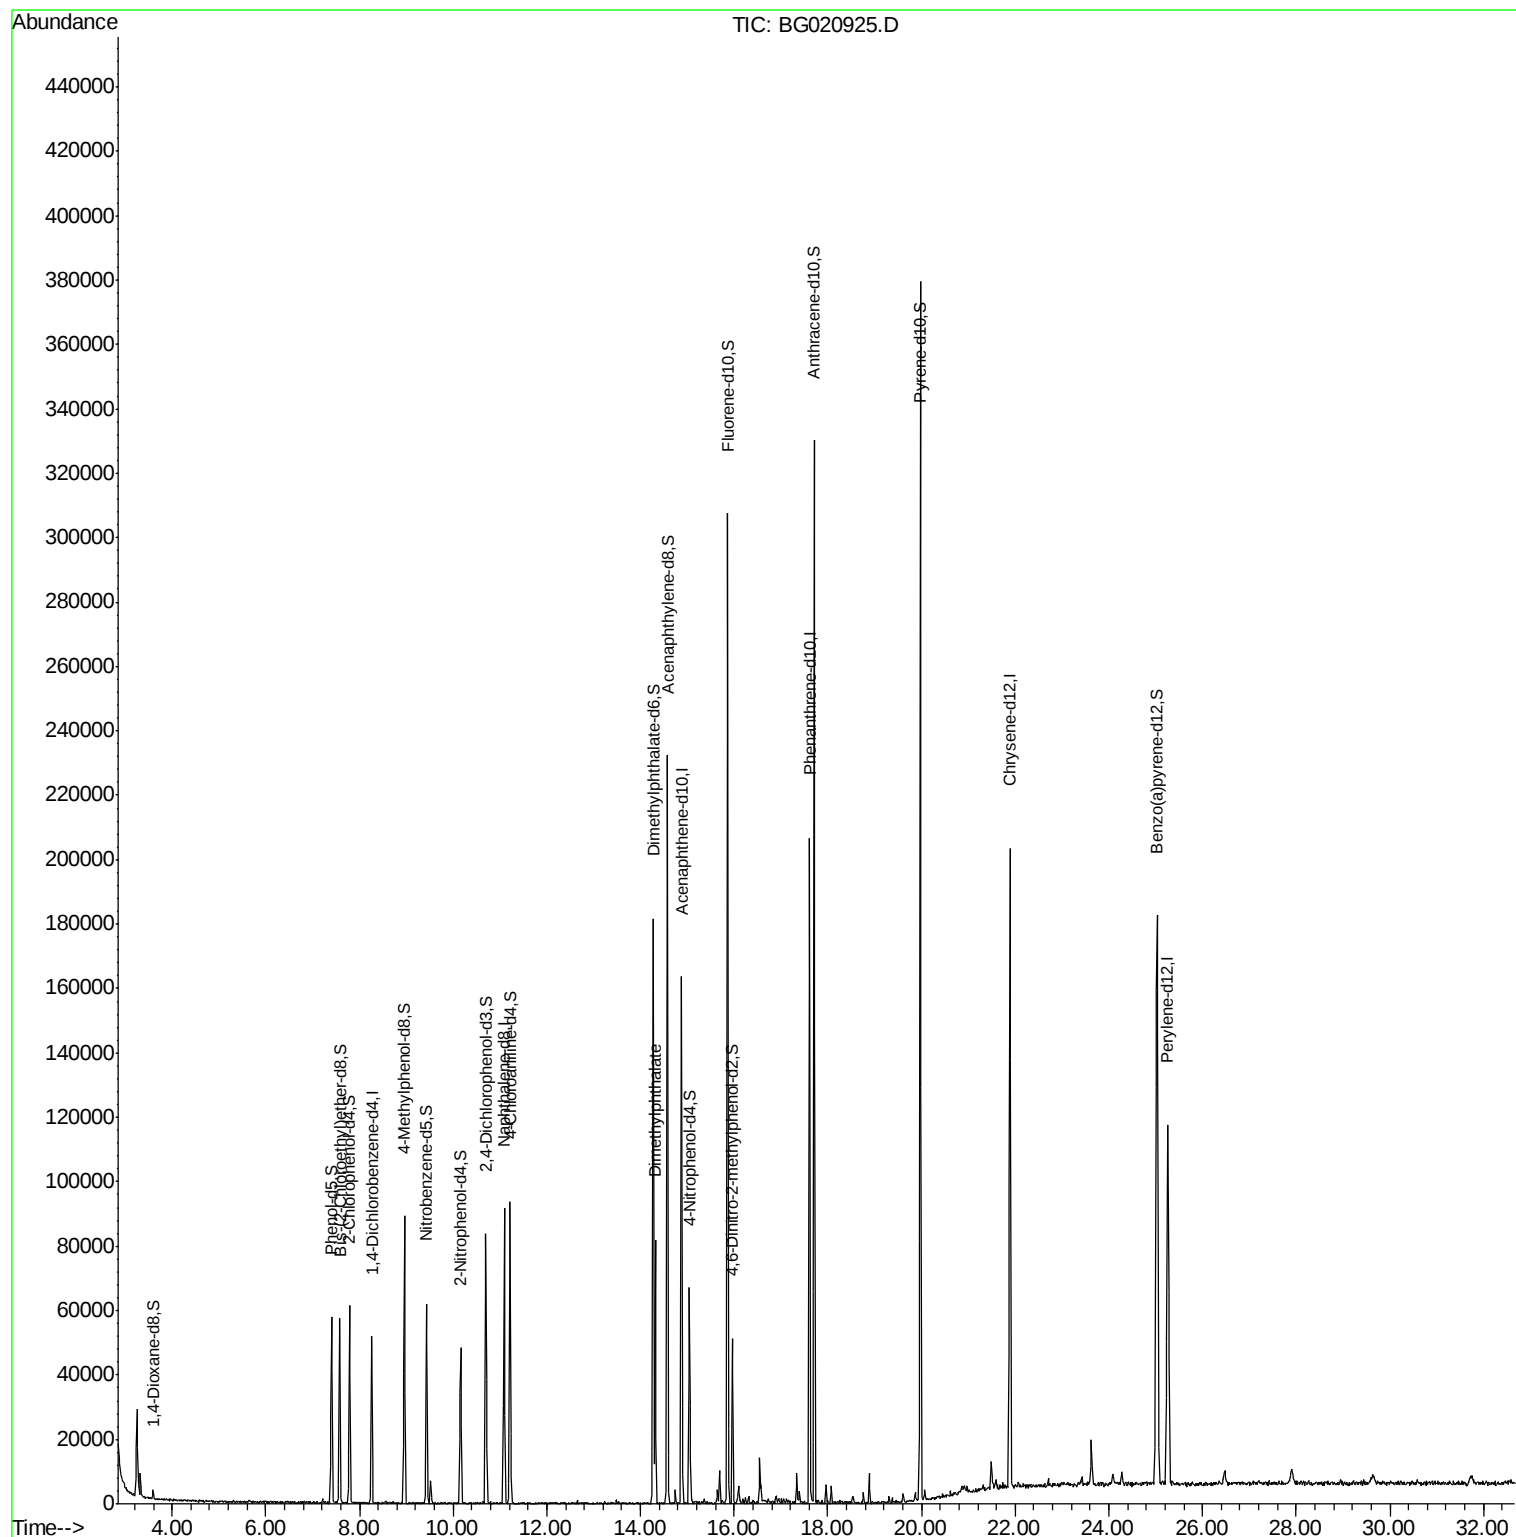

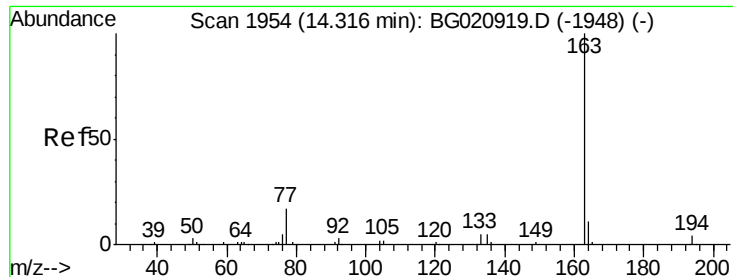

#45
 Dimethylphthalate
 Concen: 12.11 ng/ul
 RT: 14.31 min Scan# 1953
 Delta R.T. -0.00 min
 Lab File: BG020925.D
 Acq: 17 Feb 2016 14:11

Instrument :
 BNA_G
 ClientSampleId :
 0311-S35-0003

Tot Ion:163 Resp: 61216
 Ion Ratio Lower Upper
 163 100
 194 3.7 3.0 4.6
 164 9.7 7.7 11.5

