

Data File : BG025861.D
Acq On : 17 Feb 2017 16:16
Operator : SJ/MA
Sample : I1880-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MANHOLE

Quant Time: Feb 17 22:26:43 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	91938	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	446145	20.00	ng	0.00
38) Acenaphthene-d10	14.69	164	325242	20.00	ng	0.00
63) Phenanthrene-d10	17.42	188	738088	20.00	ng	0.00
75) Chrysene-d12	21.67	240	768652	20.00	ng	0.00
86) Perylene-d12	24.88	264	739014	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	11554	2.19	ng	0.00
7) Phenol-d6	7.23	99	12642	1.62	ng	0.00
23) Nitrobenzene-d5	9.24	82	28285	4.00	ng	0.00
41) 2,4,6-Tribromophenol	16.16	330	8823	2.94	ng	0.00
44) 2-Fluorobiphenyl	13.32	172	87099	4.68	ng	0.00
78) Terphenyl-d14	20.02	244	114963	3.64	ng	0.00
Target Compounds						
10) Phenol	7.26	94	45728	5.39	ng	Qvalue # 75
49) Dimethylphthalate	14.13	163	105708	4.74	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG025861.D

Acq On : 17 Feb 2017 16:16

Operator : SJ/MA

Sample : I1880-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

MANHOLE


Quant Time: Feb 17 22:26:43 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 17 15:48:21 2017

Response via : Initial Calibration

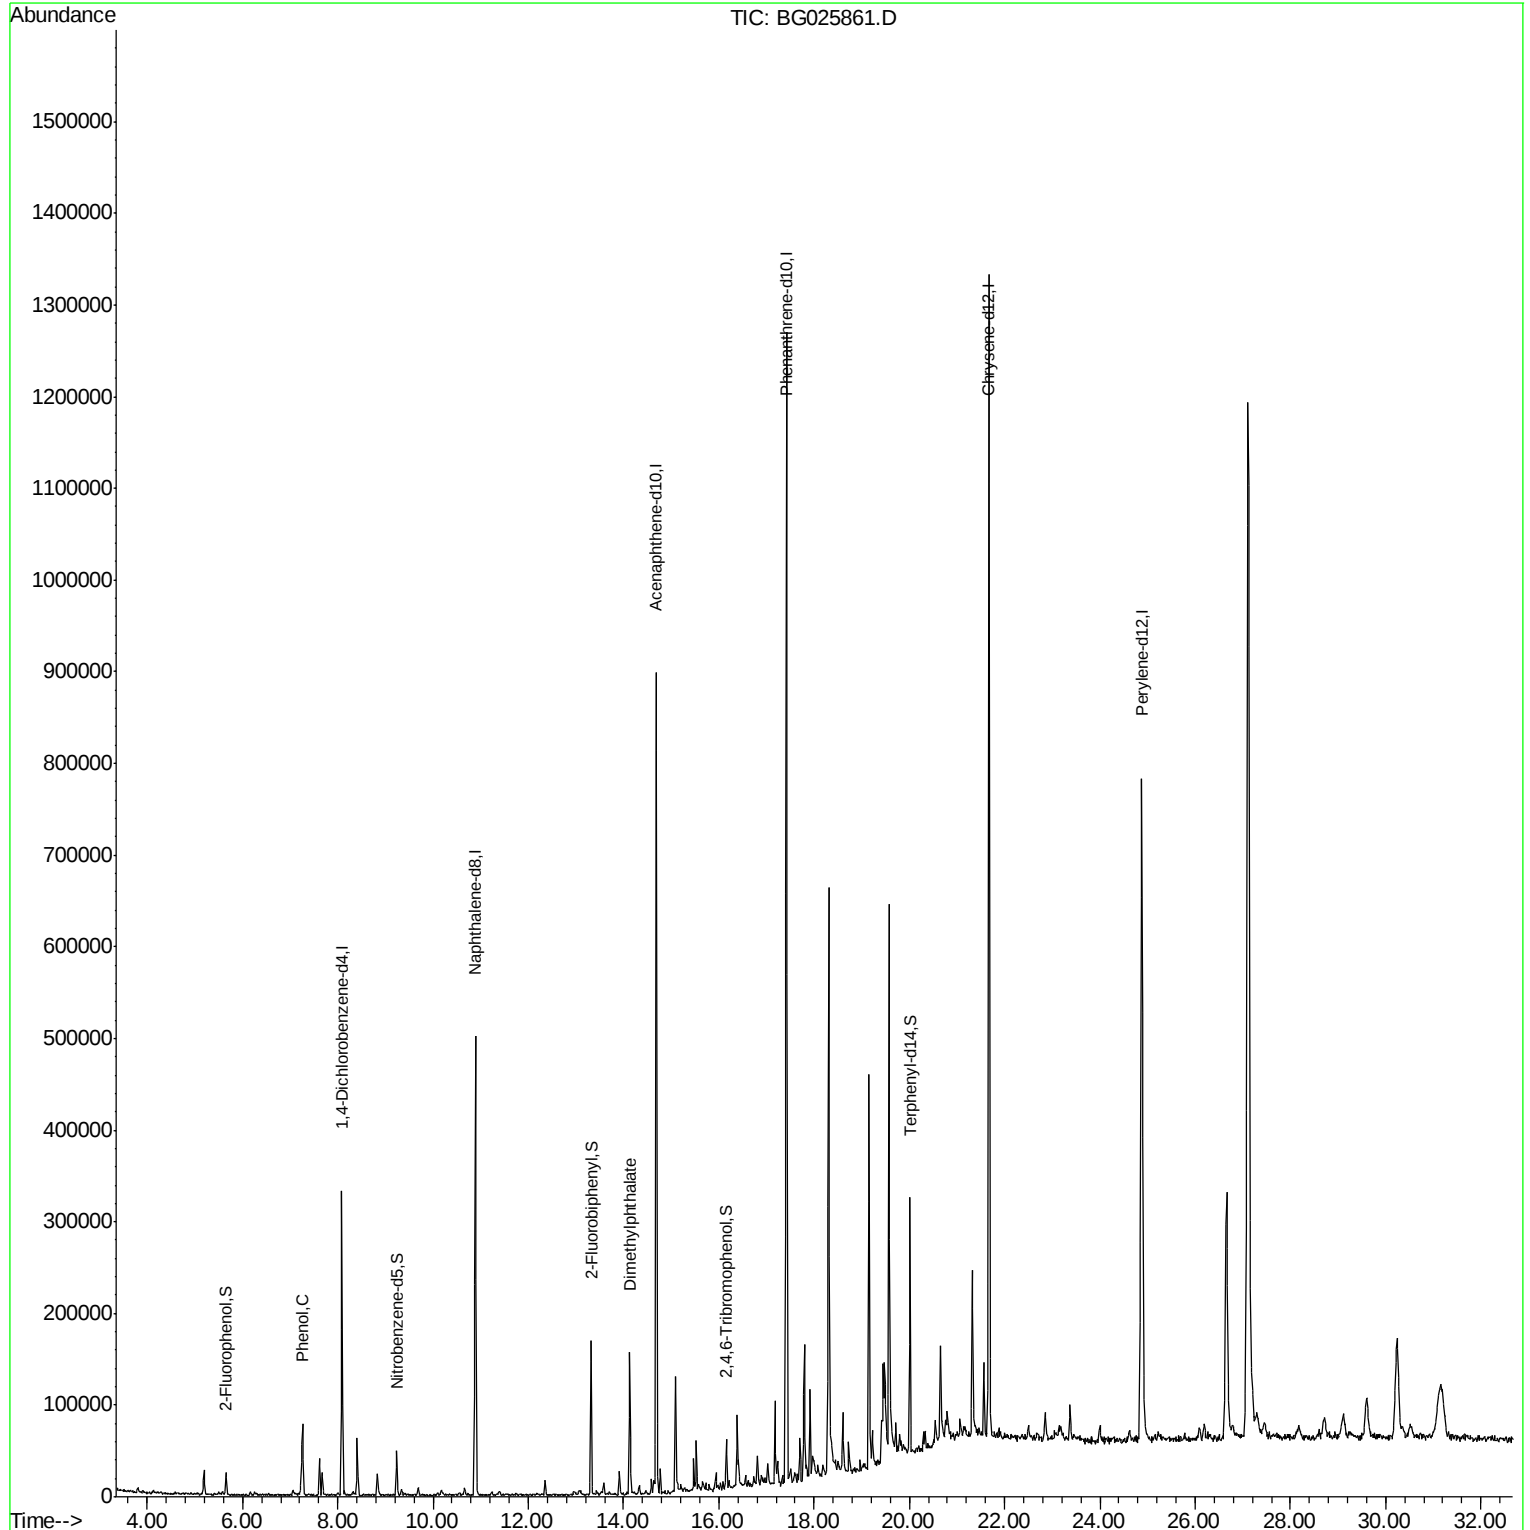



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.09 min Scan# 808

Delta R.T. 0.00 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16

Instrument :

BNA_G

ClientSampleId :

MANHOLE


Tgt Ion:152 Resp: 91938

Ion Ratio Lower Upper

152 100

150 161.6 114.0 171.0




115 59.9 48.1 72.1

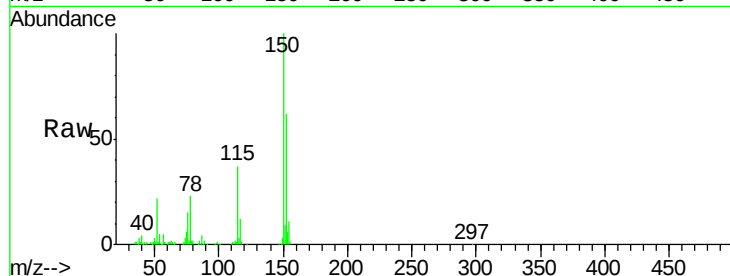

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

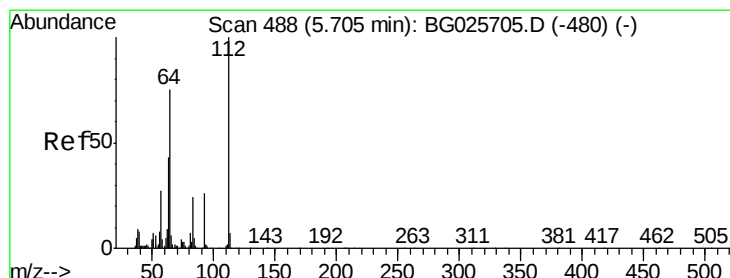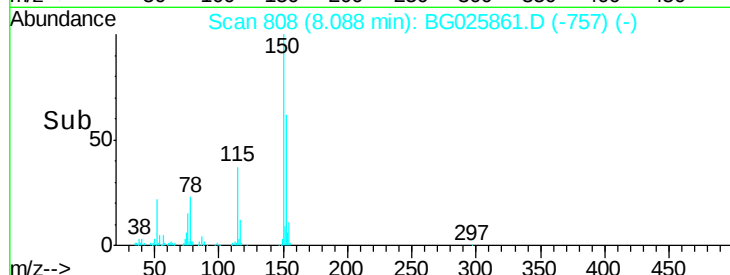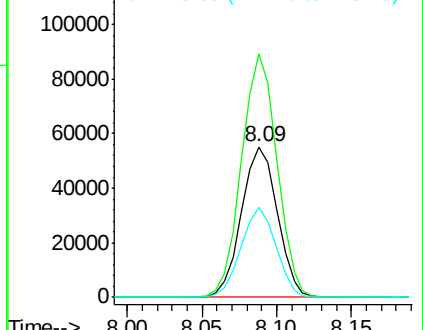

#5

2-Fluorophenol

Concen: 2.19 ng

RT: 5.66 min Scan# 394

Delta R.T. 0.00 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16


Tgt Ion:112 Resp: 11554

Ion Ratio Lower Upper

112 100

64 59.5 61.8 92.6#



63 28.6 37.2 55.8#


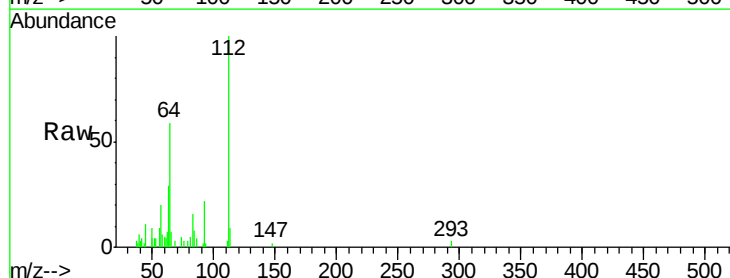


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

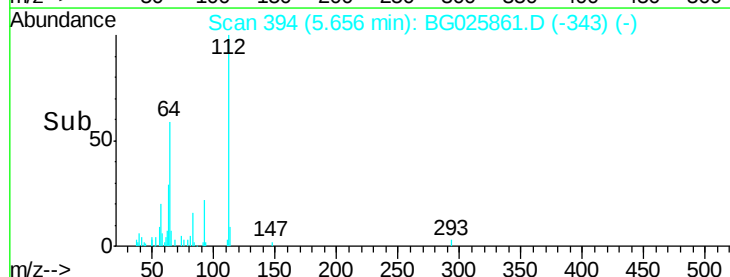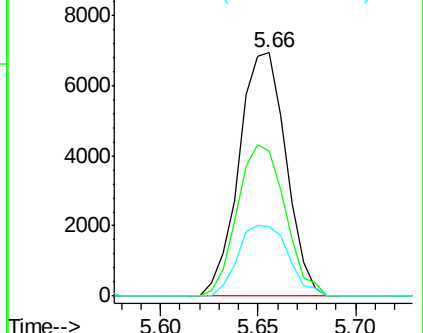

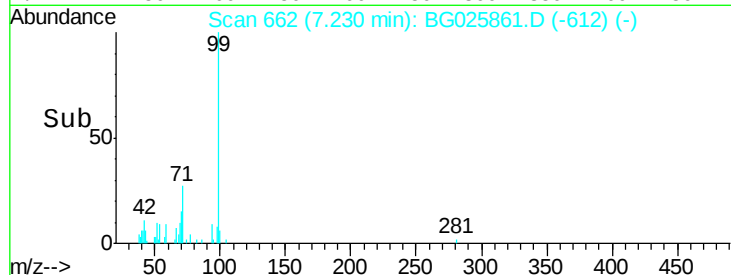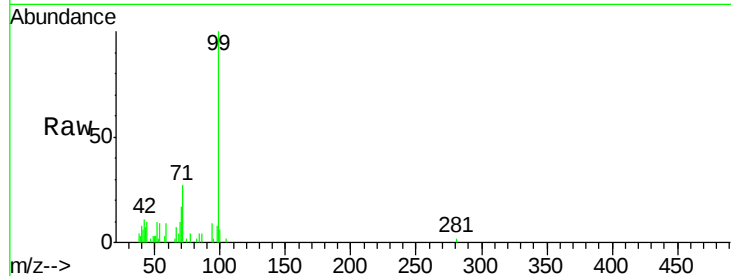

#7

Phenol-d6

Concen: 1.62 ng

RT: 7.23 min Scan# 662

Delta R.T. -0.01 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16

Instrument :

BNA_G

ClientSampleId :

MANHOLE





Tgt Ion: 99 Resp: 12642

Ion Ratio Lower Upper

99 100

42 10.9 20.5 30.7#

71 26.7 37.6 56.4#

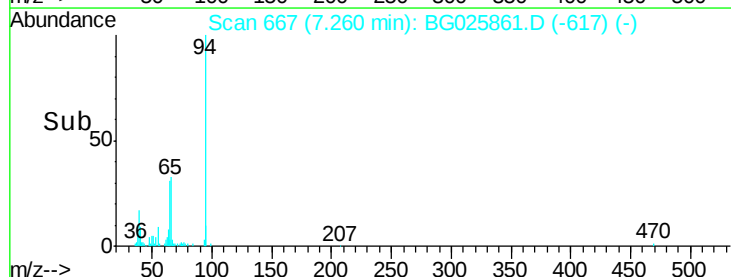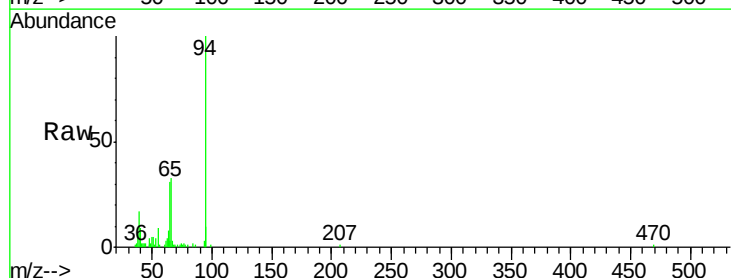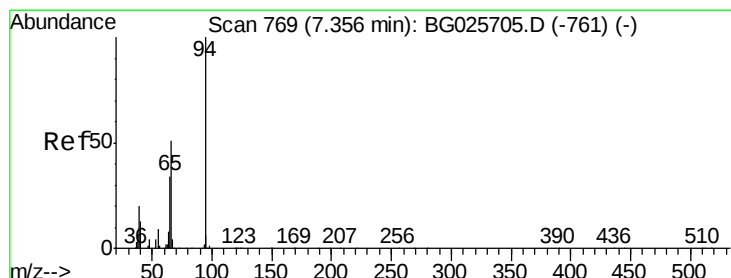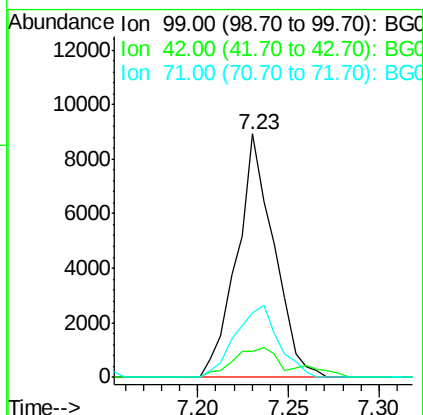

#10

Phenol

Concen: 5.39 ng

RT: 7.26 min Scan# 667

Delta R.T. -0.01 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16


Tgt Ion: 94 Resp: 45728


Ion Ratio Lower Upper

94 100

65 30.7 20.6 60.6

66 33.1 35.5 75.5#

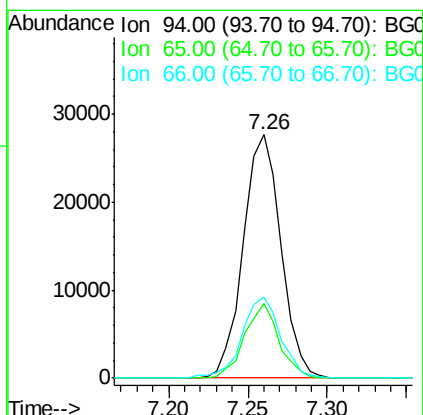


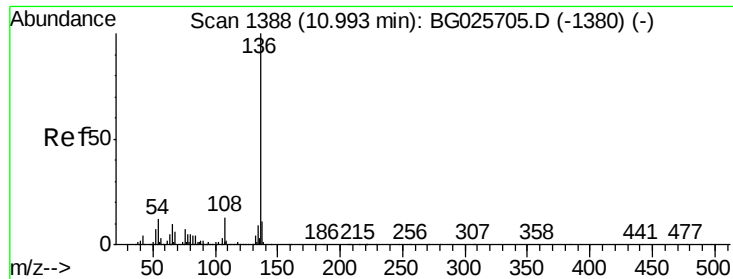




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.88 min Scan# 1284
Delta R.T. -0.01 min
Lab File: BG025861.D
Acq: 17 Feb 2017 16:16

Instrument :
BNA_G
ClientSampleId :
MANHOLE

Tgt Ion:	136	Resp:	446145
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.9	13.3
54	9.5	9.3	13.9
68	6.5	5.1	7.7

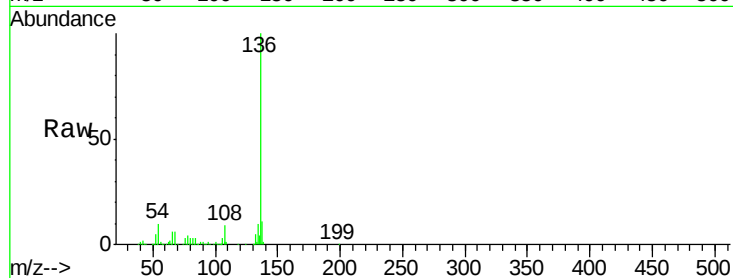


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

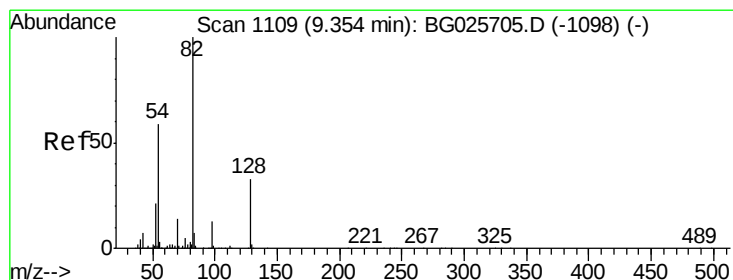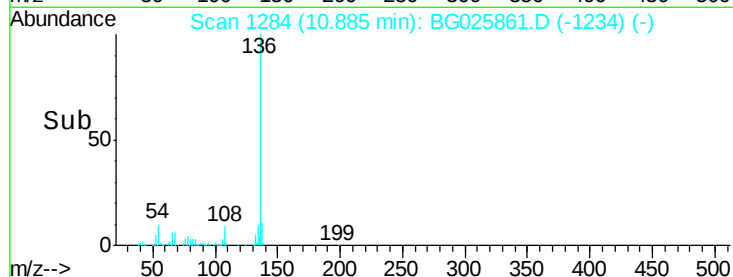
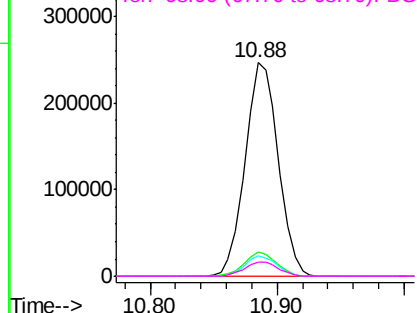



#23
Nitrobenzene-d5
Concen: 4.00 ng
RT: 9.24 min Scan# 1004
Delta R.T. -0.01 min
Lab File: BG025861.D
Acq: 17 Feb 2017 16:16

Tgt Ion:	82	Resp:	28285
Ion	Ratio	Lower	Upper
82	100		
128	44.5	26.4	39.6#
54	55.4	49.4	74.2

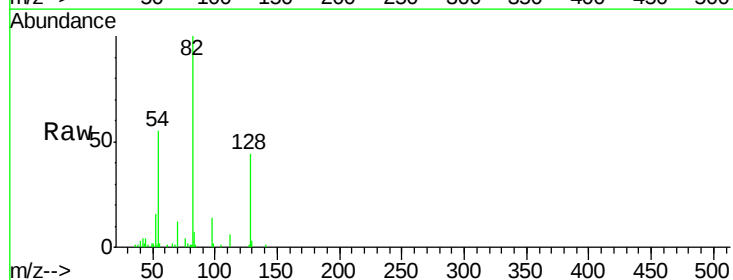

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC



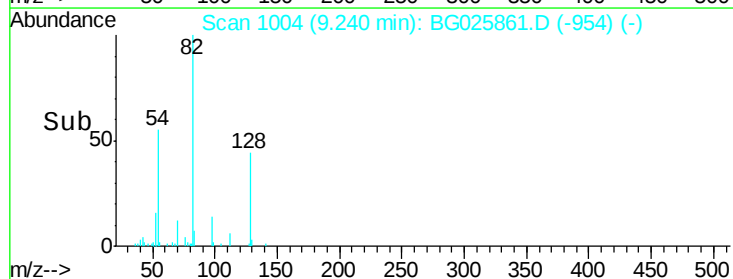
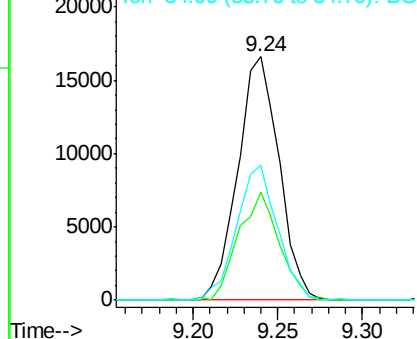


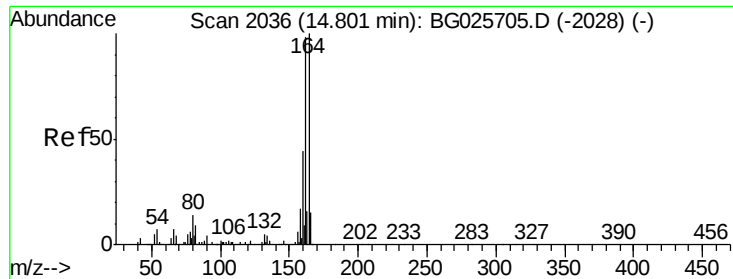

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.69 min Scan# 1931
 Delta R.T. -0.01 min
 Lab File: BG025861.D
 Acq: 17 Feb 2017 16:16




Instrument :
 BNA_G
 ClientSampleId :
 MANHOLE


Tgt Ion:164 Resp: 325242
 Ion Ratio Lower Upper
 164 100
 162 101.1 85.1 127.7
 160 43.0 34.7 52.1

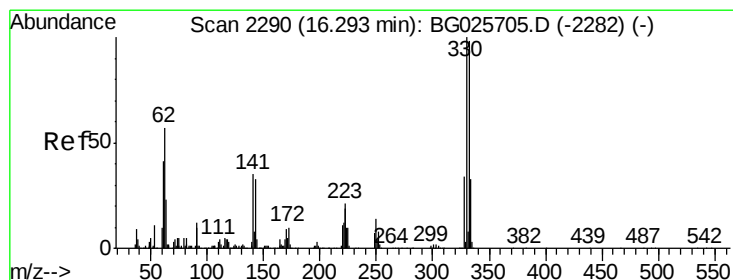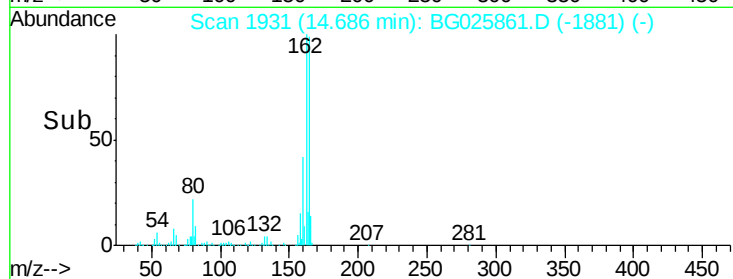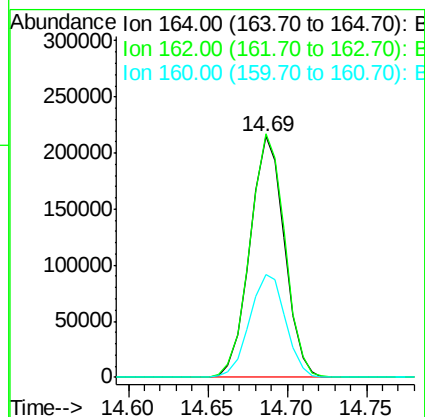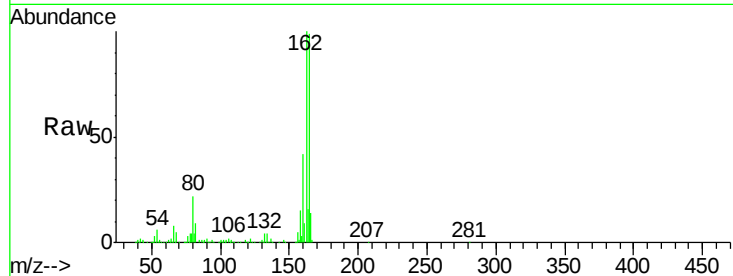

#41
 2,4,6-Tribromophenol
 Concen: 2.94 ng
 RT: 16.16 min Scan# 2182
 Delta R.T. -0.01 min
 Lab File: BG025861.D
 Acq: 17 Feb 2017 16:16

Tgt Ion:330 Resp: 8823
 Ion Ratio Lower Upper
 330 100
 332 89.4 77.3 115.9
 141 38.6 32.1 48.1

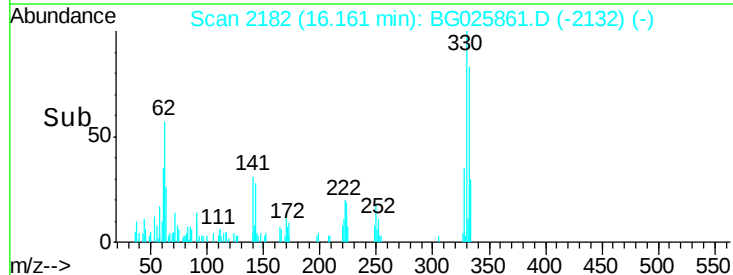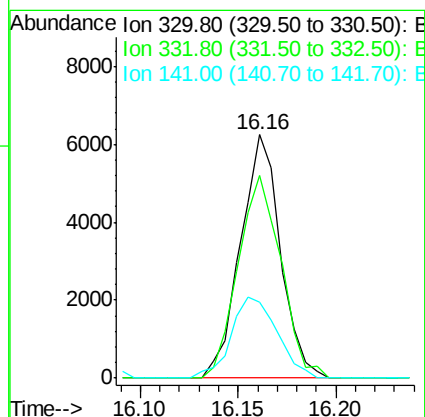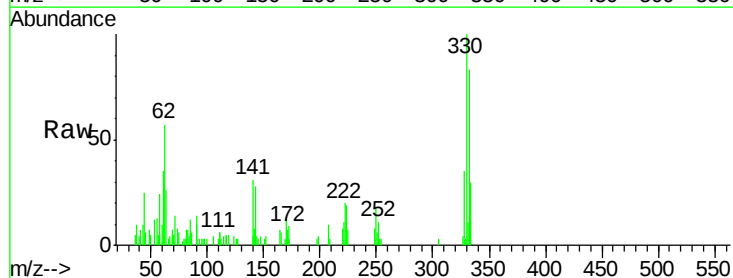

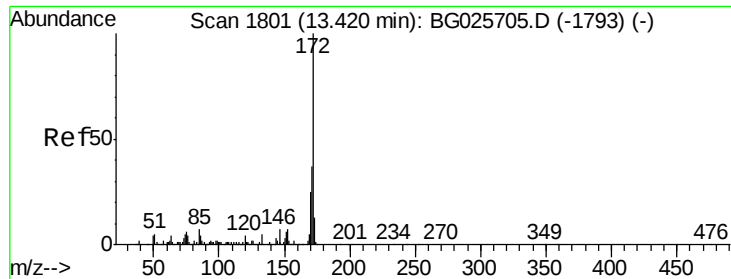

#44

2-Fluorobiphenyl

Concen: 4.68 ng

RT: 13.32 min Scan# 1698

Delta R.T. -0.01 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16

Instrument :

BNA_G

ClientSampleId :

MANHOLE





Tgt Ion:172 Resp: 87099

Ion Ratio Lower Upper

172 100

171 36.1 32.2 48.2

170 25.0 21.8 32.6

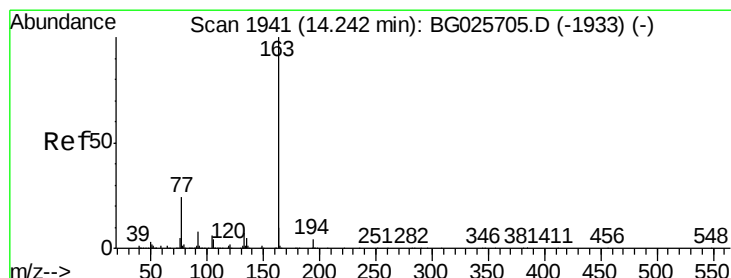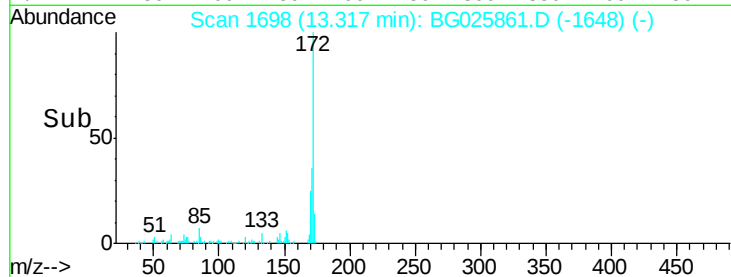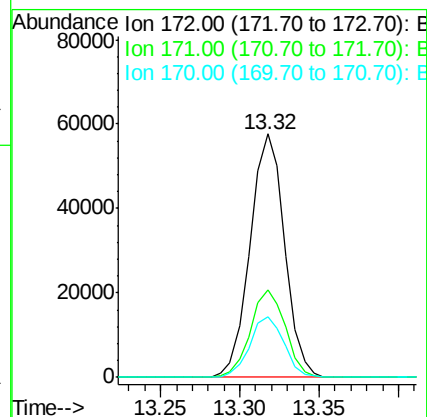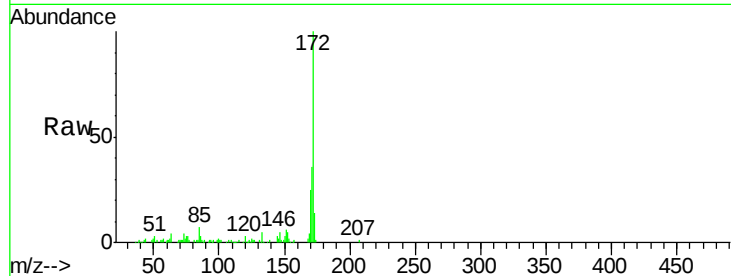

#49

Dimethylphthalate

Concen: 4.74 ng

RT: 14.13 min Scan# 1837

Delta R.T. -0.01 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16




Tgt Ion:163 Resp: 105708


Ion Ratio Lower Upper

163 100

194 3.8 3.8 5.6

164 9.8 9.3 13.9

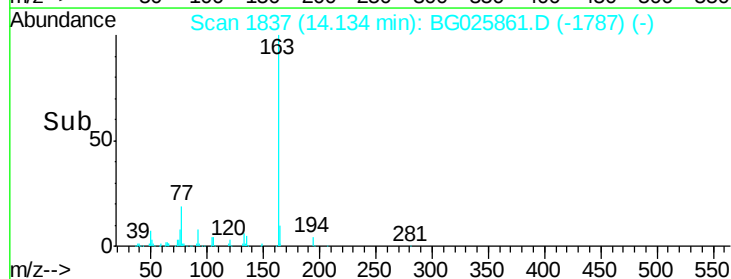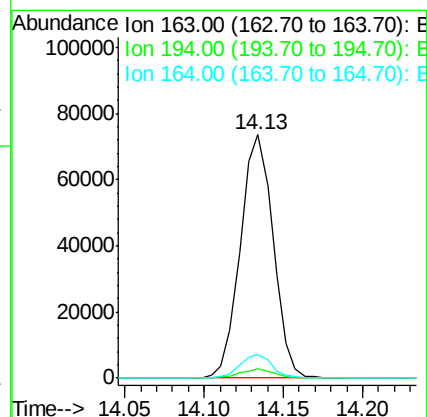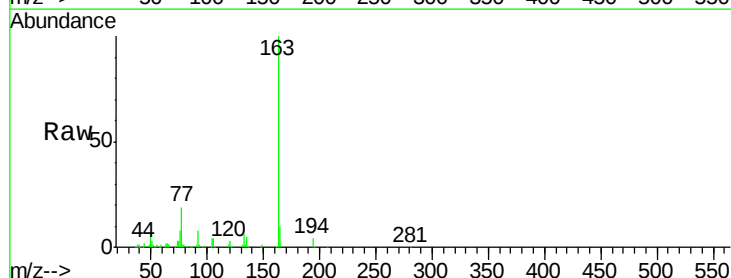

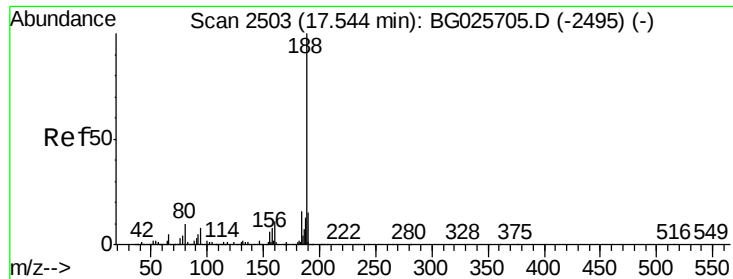

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.42 min Scan# 2396

Delta R.T. 0.00 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16

Instrument :

BNA_G

ClientSampleId :

MANHOLE


Tgt Ion:188 Resp: 738088

Ion Ratio Lower Upper

188 100

94 9.9 5.8 8.8#




80 11.1 7.5 11.3

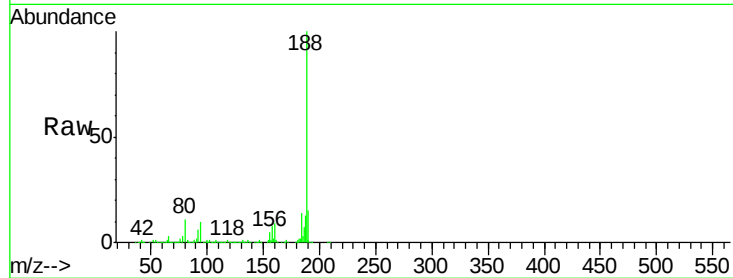

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

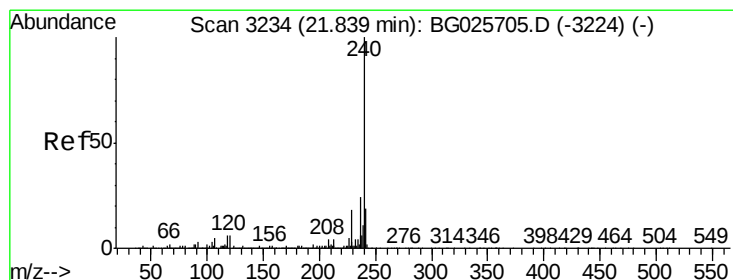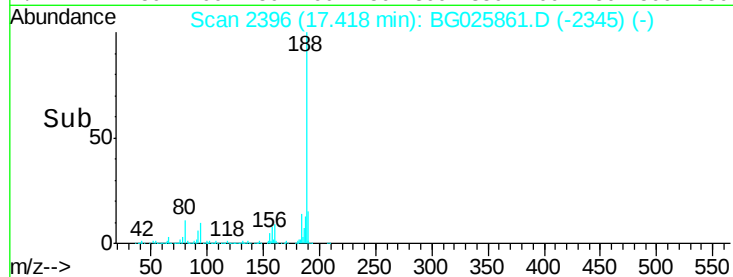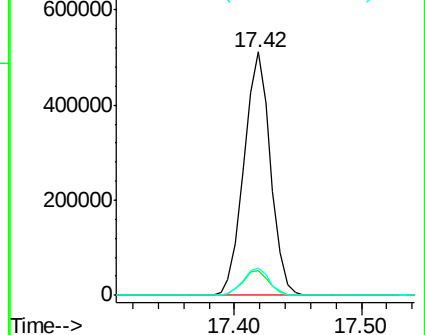

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.67 min Scan# 3120

Delta R.T. -0.01 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16


Tgt Ion:240 Resp: 768652

Ion Ratio Lower Upper

240 100

120 11.8 5.7 8.5#



236 26.3 22.2 33.4

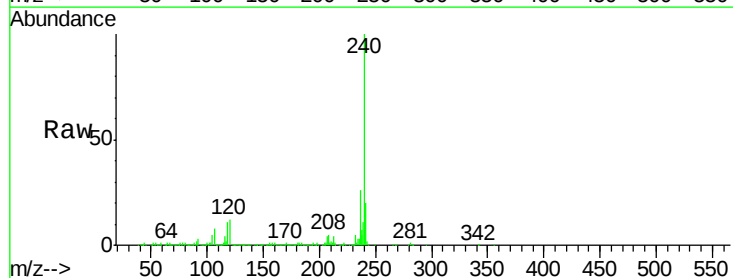


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

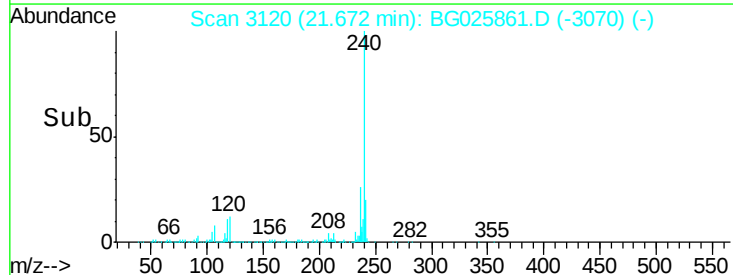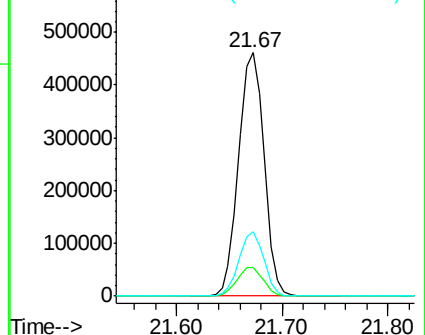

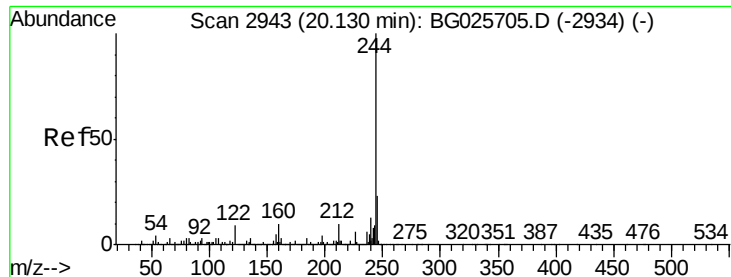

#78

Terphenyl-d14

Concen: 3.64 ng

RT: 20.02 min Scan# 2838

Delta R.T. -0.01 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16

Instrument :

BNA_G

ClientSampleId :

MANHOLE


Tgt Ion:244 Resp: 114963

Ion Ratio Lower Upper

244 100

212 6.6 10.0 15.0#




122 11.0 8.6 12.8

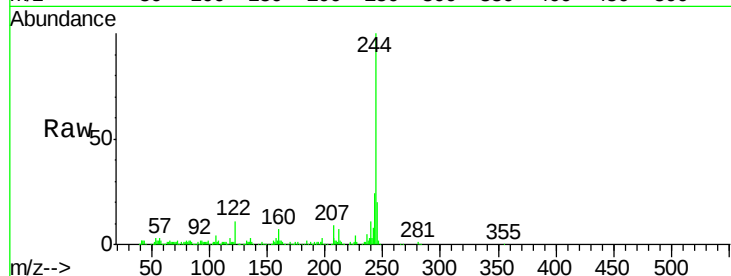

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

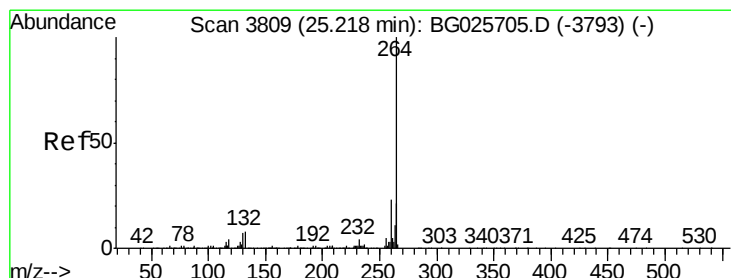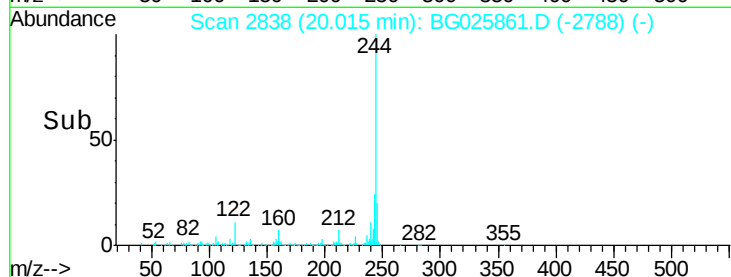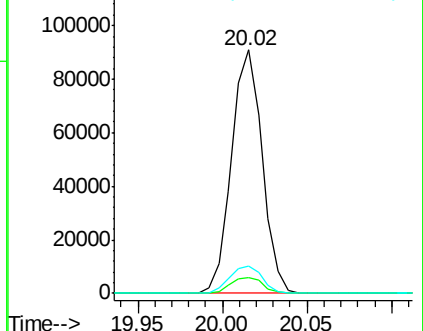

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.88 min Scan# 3666

Delta R.T. -0.01 min

Lab File: BG025861.D

Acq: 17 Feb 2017 16:16


Tgt Ion:264 Resp: 739014

Ion Ratio Lower Upper

264 100

260 24.2 21.8 32.8

265 21.7 18.2 27.4

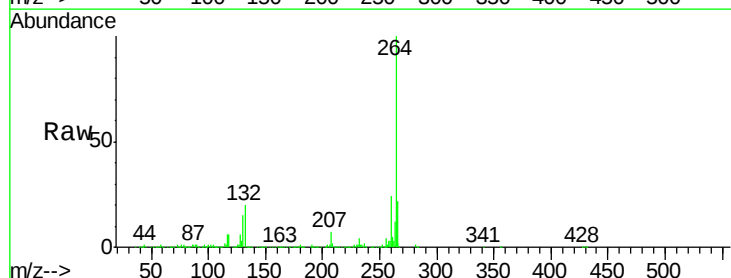

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

