
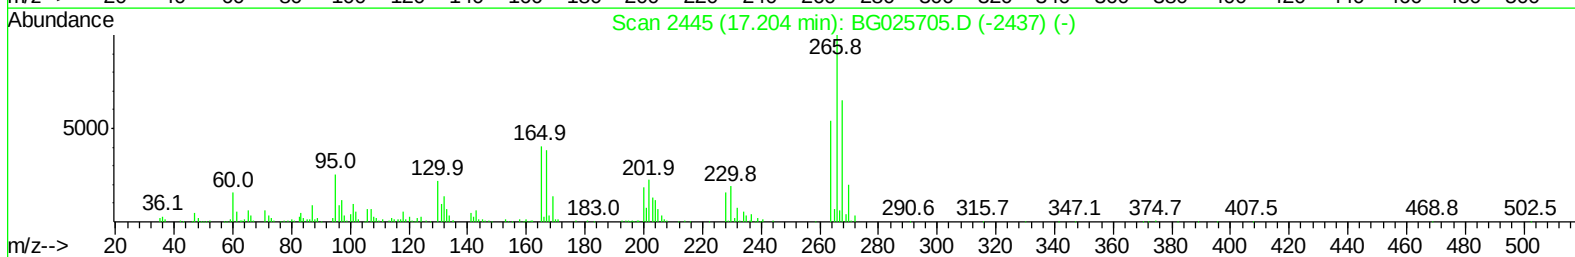
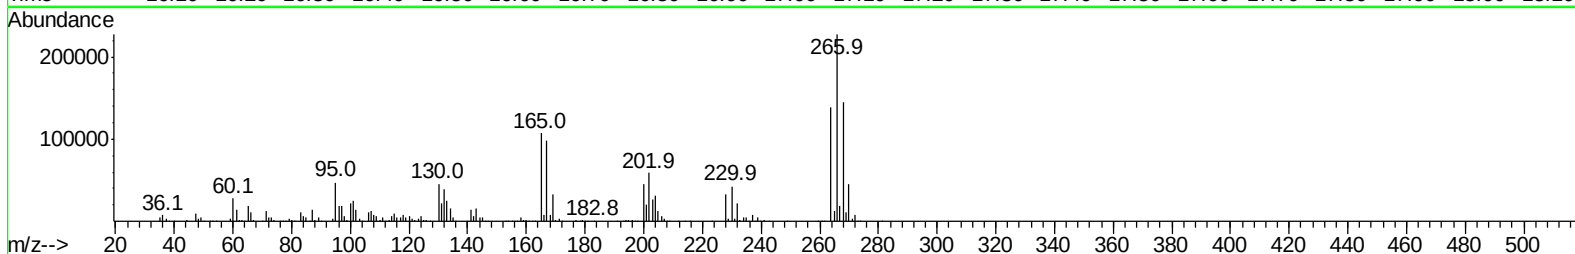


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021717\
Data File : BG025852.D
Acq On : 17 Feb 2017 10:24
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 17:54:02 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

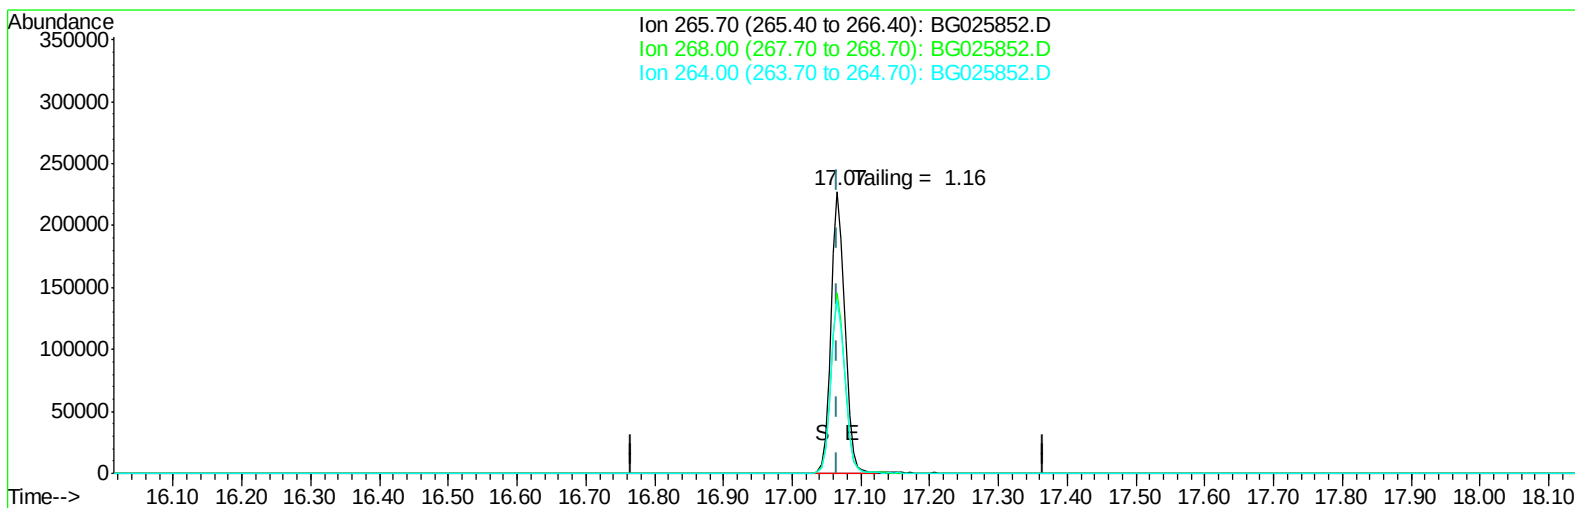

TIC: BG025852.D

(69) Pentachlorophenol (C)




17.066min (-0.000) 769528.26ng

response 317918

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	63.88
264.00	62.60	61.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021717\
Data File : BG025852.D
Acq On : 17 Feb 2017 10:24
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 17:54:02 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

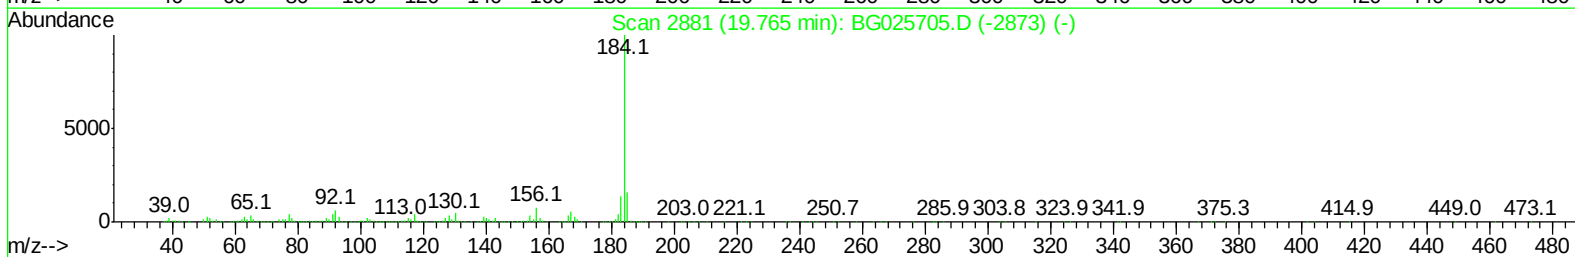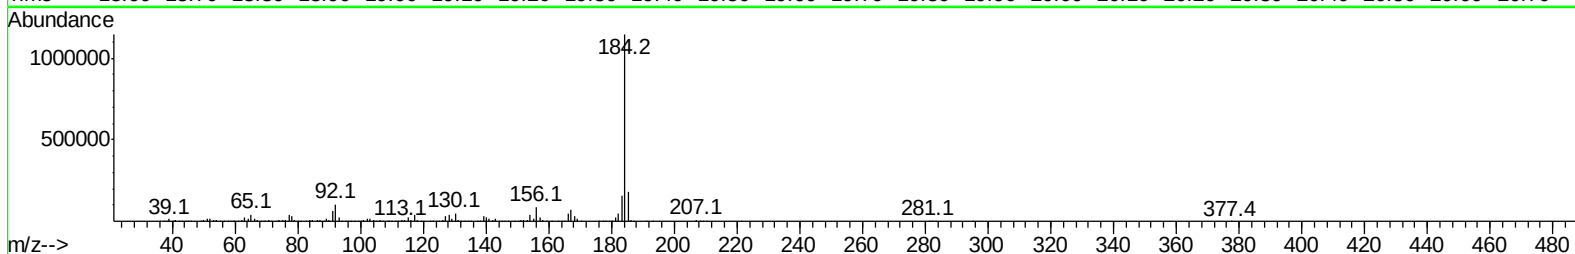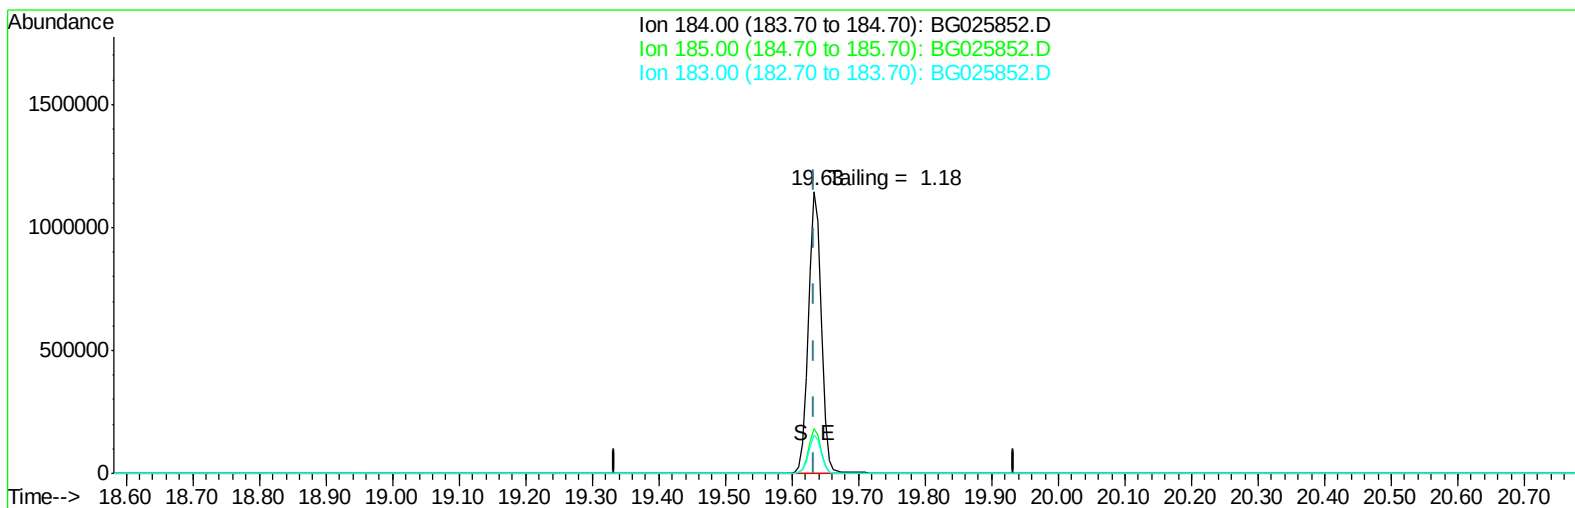

TIC: BG025852.D

(76) Benzidine

19.633min (-0.000) 204001.38ng

response 1571307

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.70
183.00	13.80	13.64
0.00	0.00	0.00