


Data Path : Z:\HPCHEM1\BNA_G\Data\BG021717\
 Data File : BG025852.D
 Acq On : 17 Feb 2017 10:24
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 15:48:21 2017

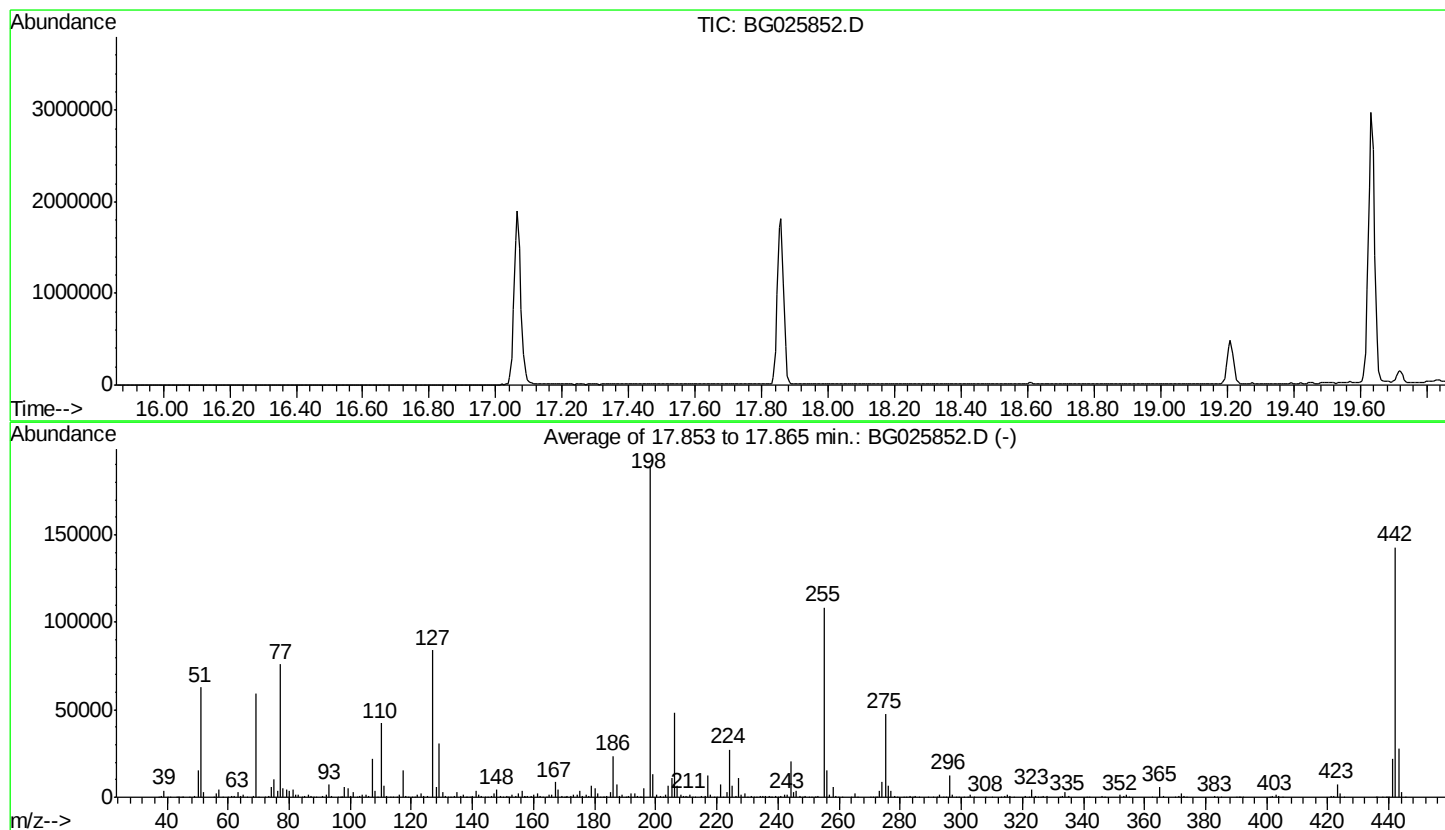

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	62709	PASS
68	69	0.00	2	0.9	503	PASS
69	198	0.00	100	31.2	59136	PASS
70	69	0.00	2	0.6	373	PASS
127	198	10	80	44.2	83781	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	189440	PASS
199	198	5	9	7.1	13406	PASS
275	198	10	60	25.2	47685	PASS
365	198	1	100	3.1	5865	PASS
441	442	0.01	24	15.4	21933	PASS
442	198	50	100	75.3	142714	PASS
443	442	15	24	19.3	27480	PASS