

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021722\
 Data File : BG052415.D
 Acq On : 17 Feb 2022 10:23
 Operator : CG/JU
 Sample : PB142443BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB142443BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.753	378	385	394	rBV	520526	852422	28.16%	8.058%
2	7.375	653	661	674	rBV	537772	921440	30.44%	8.710%
3	8.226	798	806	814	rVB	99738	163642	5.41%	1.547%
4	9.401	998	1006	1014	rBV	326493	599301	19.80%	5.665%
5	11.064	1282	1289	1297	rBV	130425	236478	7.81%	2.235%
6	13.490	1695	1702	1713	rBV	951109	1493402	49.33%	14.116%
7	14.870	1930	1937	1945	rBV	231222	362808	11.99%	3.429%
8	16.357	2183	2190	2211	rBV	718684	1165057	38.49%	11.013%
9	17.620	2399	2405	2415	rBV	336635	514521	17.00%	4.864%
10	20.210	2840	2846	2852	rBV	2322060	3027158	100.00%	28.614%
11	21.931	3132	3139	3149	rBV	362885	617921	20.41%	5.841%
12	25.397	3717	3729	3743	rBV2	199394	624990	20.65%	5.908%




Sum of corrected areas: 10579140

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021722\
Data File : BG052415.D
Acq On : 17 Feb 2022 10:23
Operator : CG/JU
Sample : PB142443BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142443BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

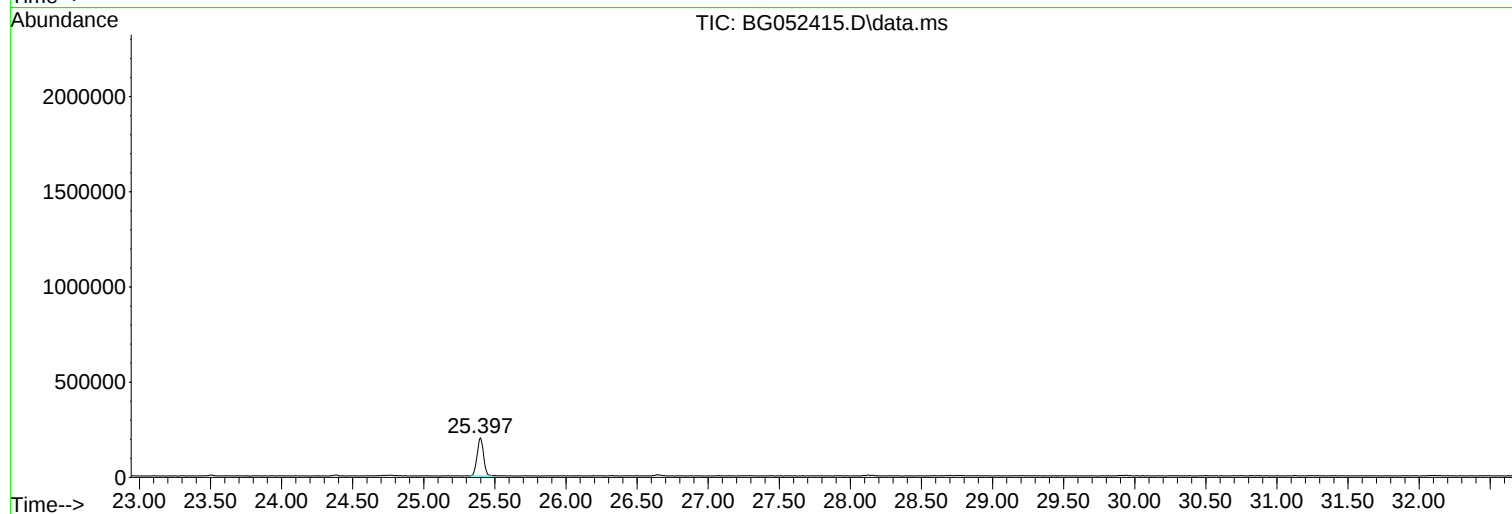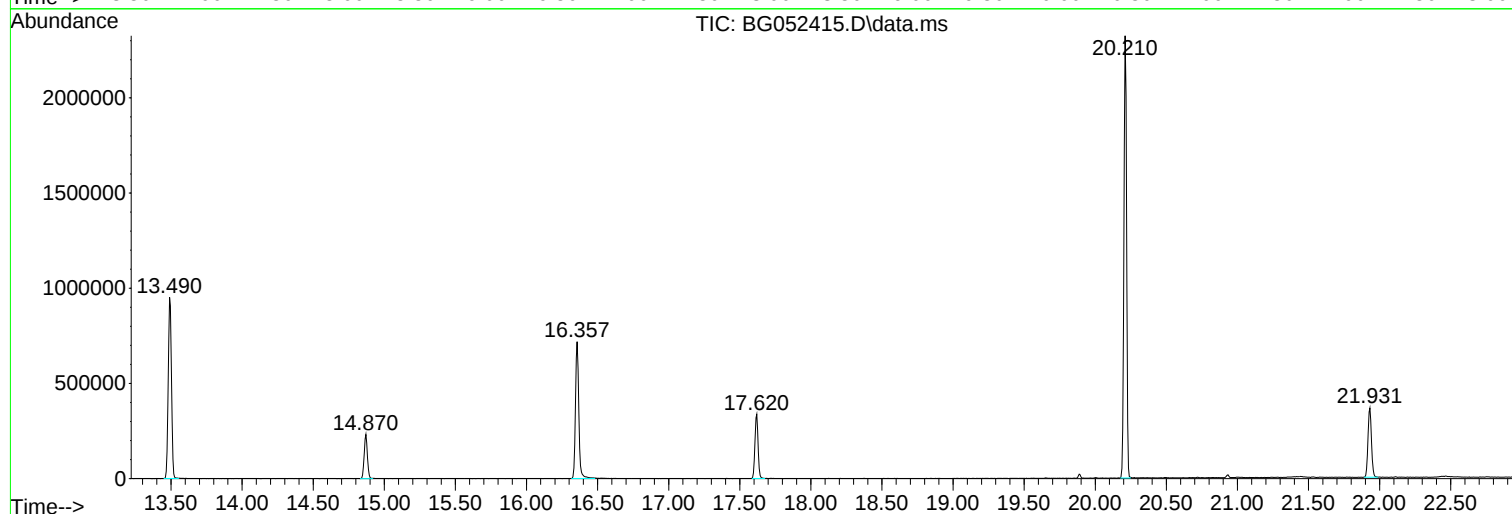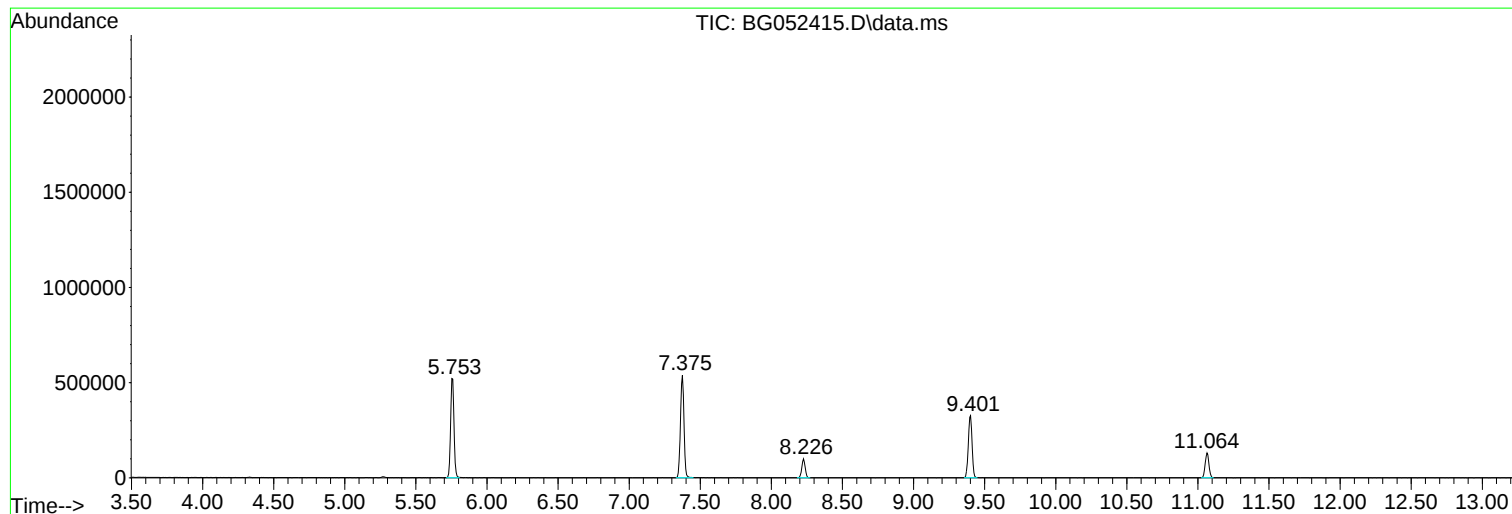

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021722\
Data File : BG052415.D
Acq On : 17 Feb 2022 10:23
Operator : CG/JU
Sample : PB142443BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142443BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021722\
Data File : BG052415.D
Acq On : 17 Feb 2022 10:23
Operator : CG/JU
Sample : PB142443BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB142443BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------