
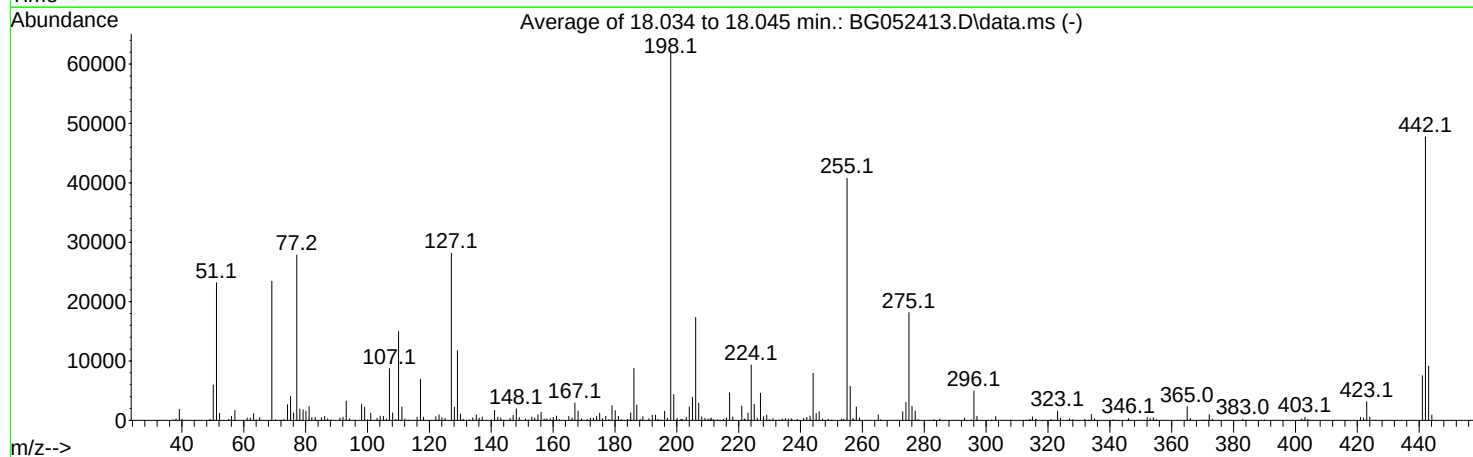


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021722\
 Data File : BG052413.D
 Acq On : 17 Feb 2022 9:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

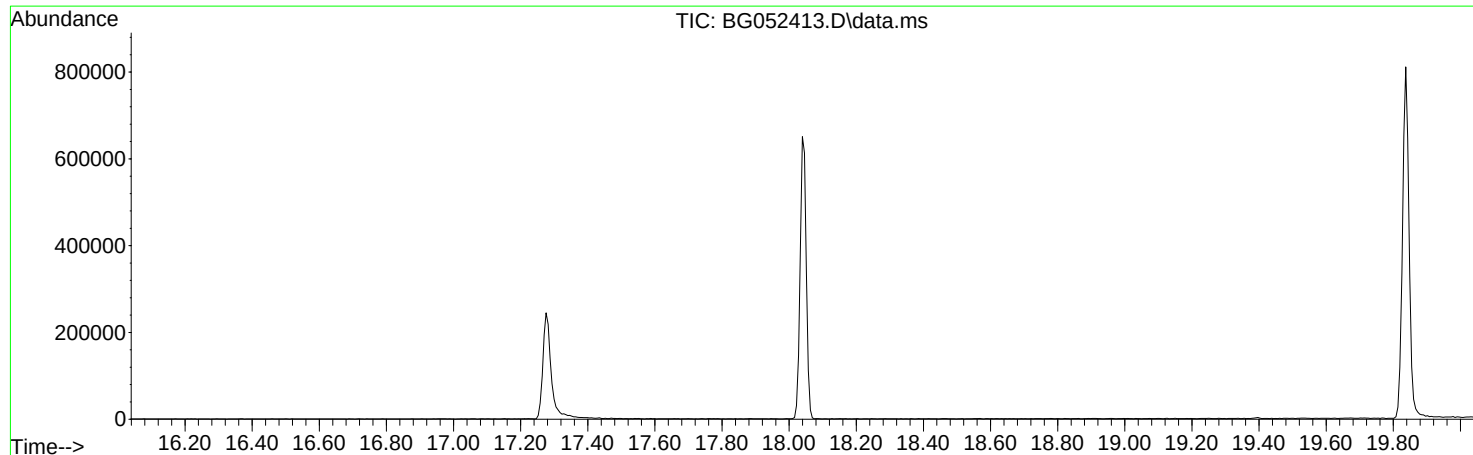

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	23165	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.8	23443	PASS
70	69	0.00	2	0.4	96	PASS
127	198	10	80	45.5	28168	PASS
197	198	0.00	2	0.6	396	PASS
198	198	100	100	100.0	61949	PASS
199	198	5	9	7.1	4370	PASS
275	198	10	60	29.3	18155	PASS
365	198	1	100	3.7	2323	PASS
441	198	0.01	100	12.1	7514	PASS
442	442	50	100	100.0	47755	PASS
443	442	15	24	19.1	9143	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/17/2022	BNA_G	BG052413.D
Compound Name	Response	Retention Time
DDT	250459	21.08
DDD	3433	20.62
DDE	256	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3689	254148	1.45

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021722\
Data File : BG052413.D
Acq On : 17 Feb 2022 9:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 17 10:11:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

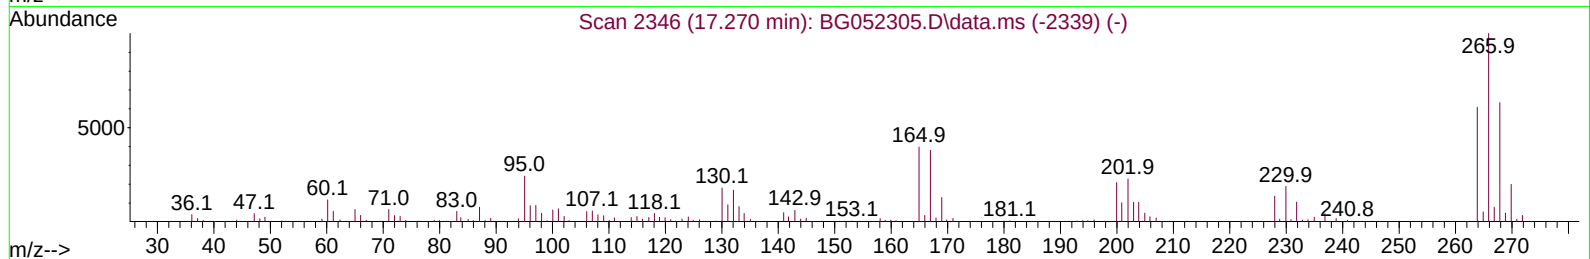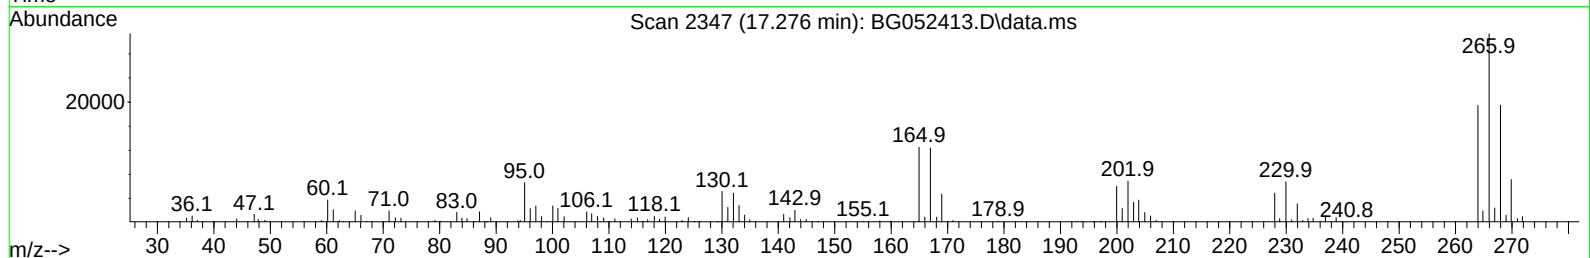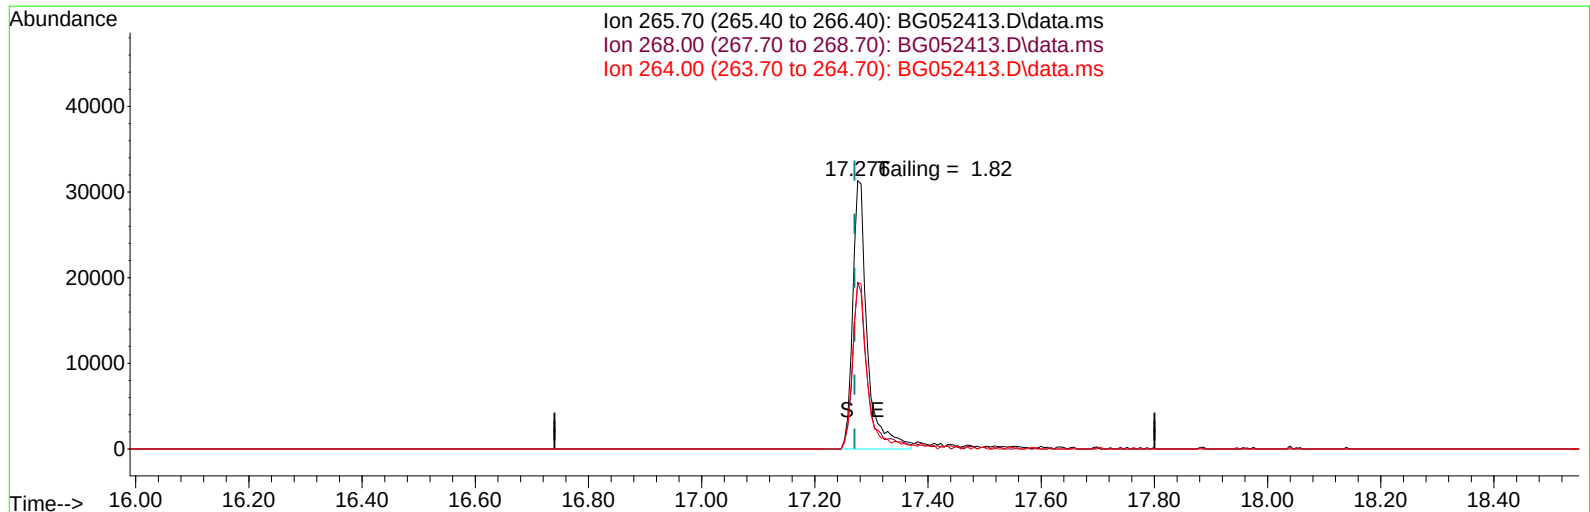

TIC: BG052413.D\data.ms

(70) Pentachlorophenol (C)

17.276min (+ 0.006) 120062.02 ng




response 56556

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	62.22
264.00	65.20	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021722\
Data File : BG052413.D
Acq On : 17 Feb 2022 9:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 17 10:11:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

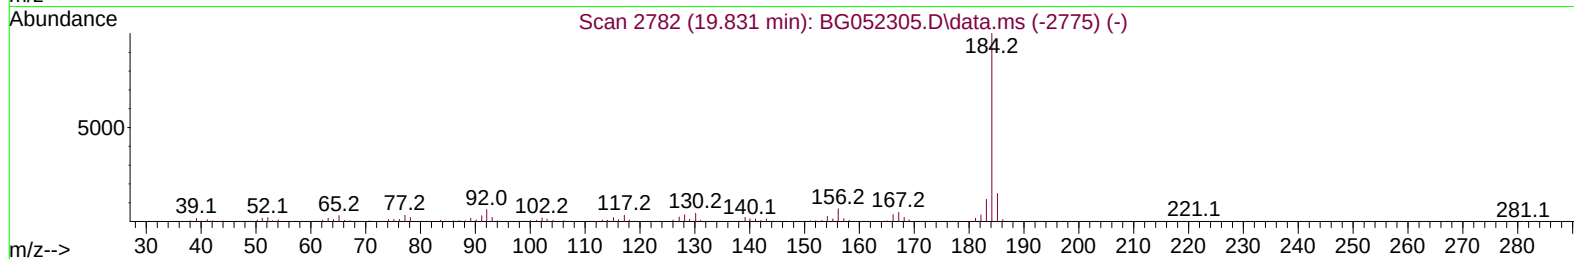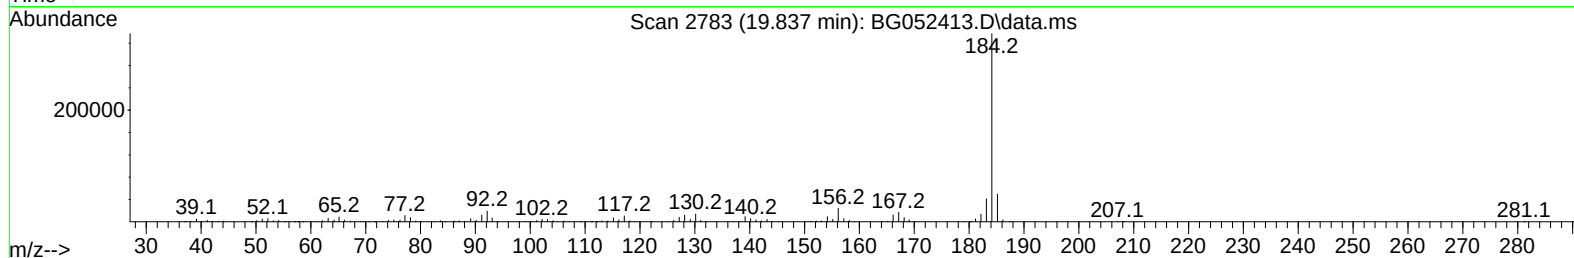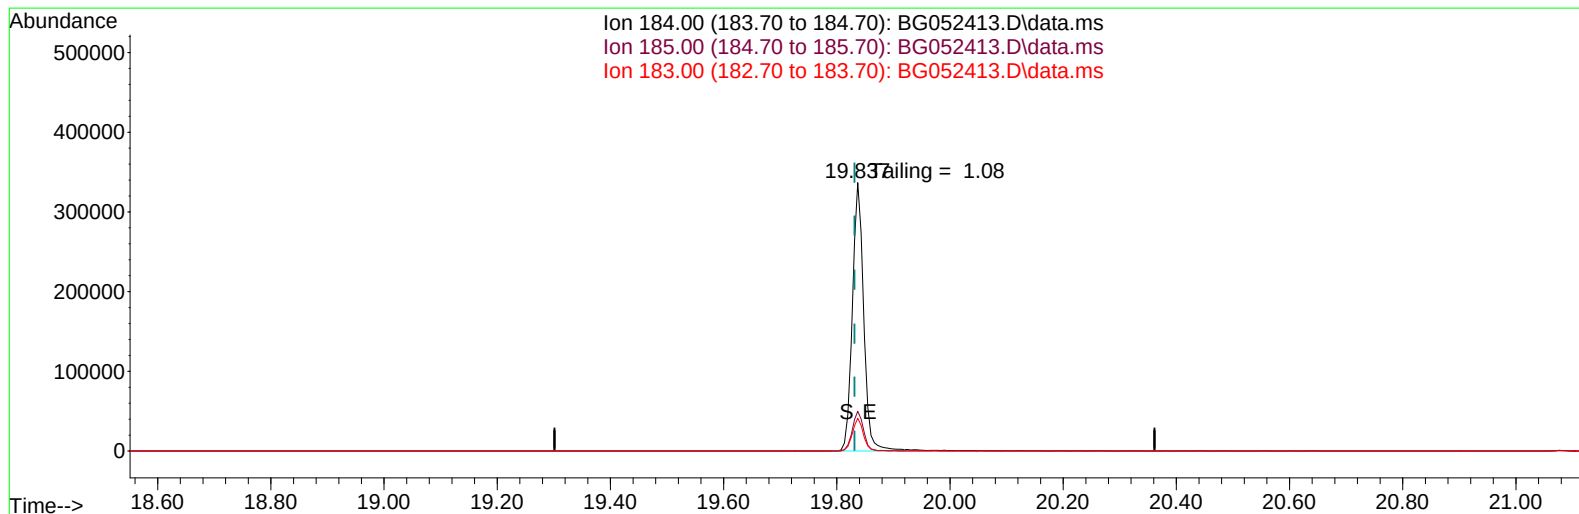

TIC: BG052413.D\data.ms

(77) Benzidine

19.837min (+ 0.006) 0.00 ng

response 470501

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.80
183.00	12.20	12.21
0.00	0.00	0.00