
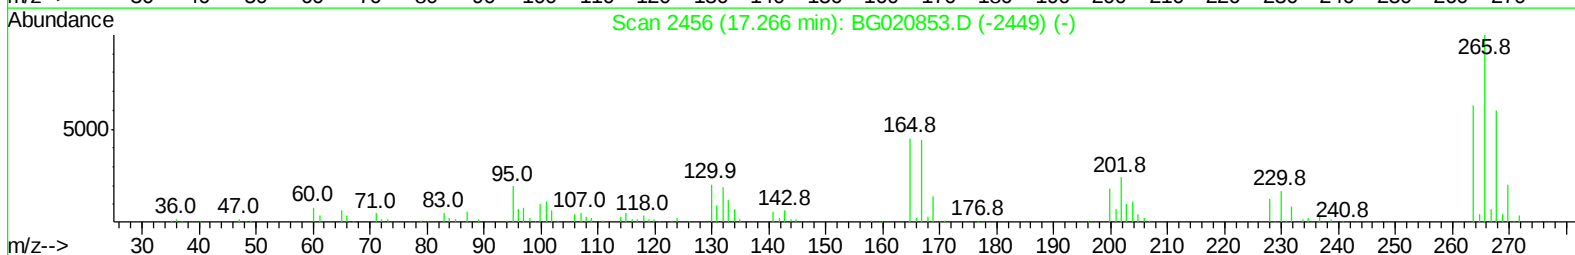
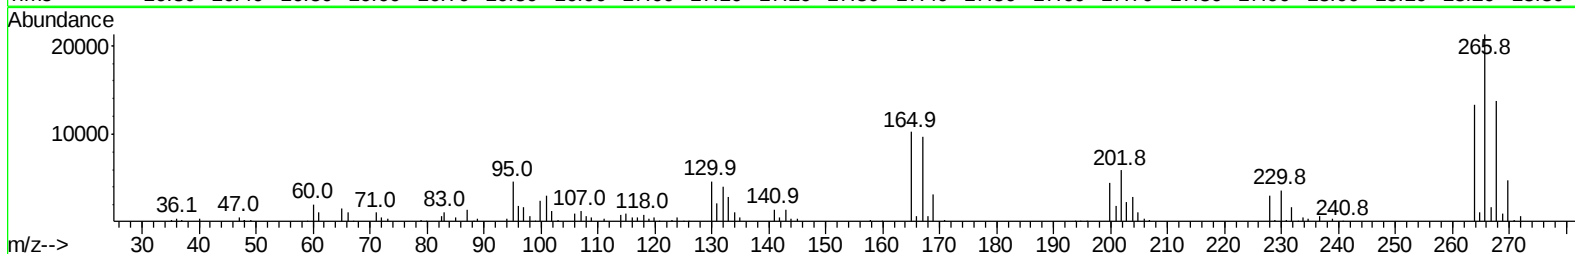


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020935.D
Acq On : 18 Feb 2016 13:53
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 07:59:50 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

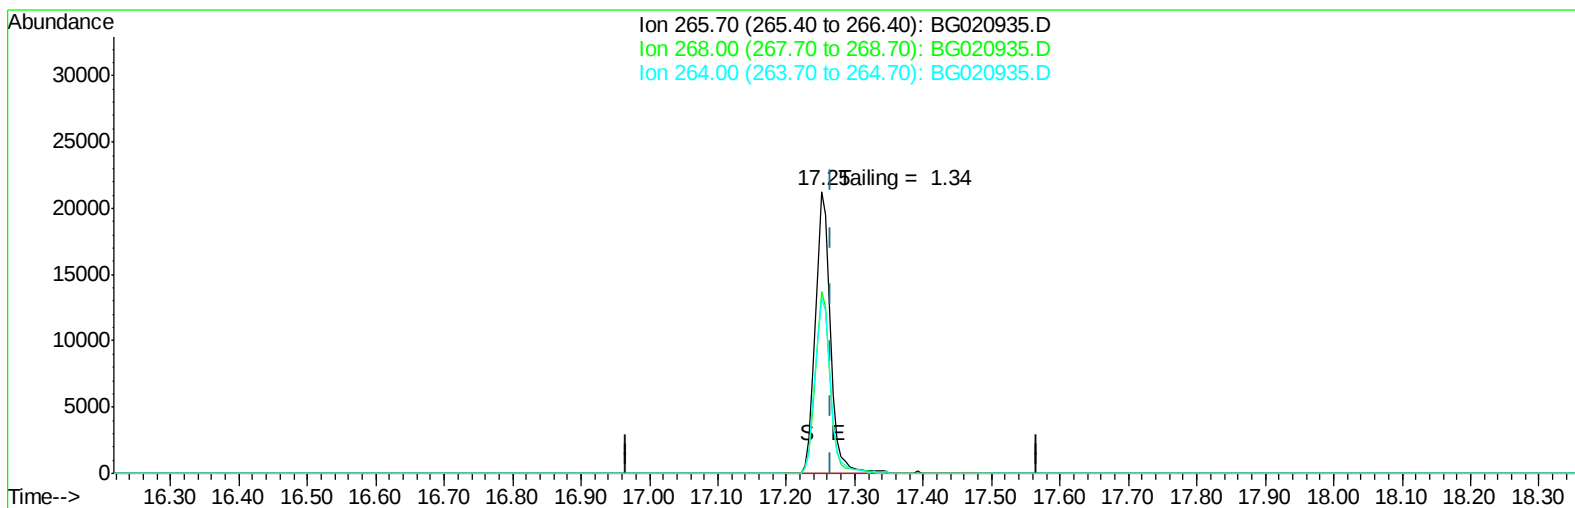

TIC: BG020935.D

(69) Pentachlorophenol (C)




17.251min (-0.015) 0.00ng

response 32679

Ion	Exp%	Act%
265.70	100	100
268.00	59.70	64.58
264.00	62.80	62.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020935.D
Acq On : 18 Feb 2016 13:53
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 07:59:50 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

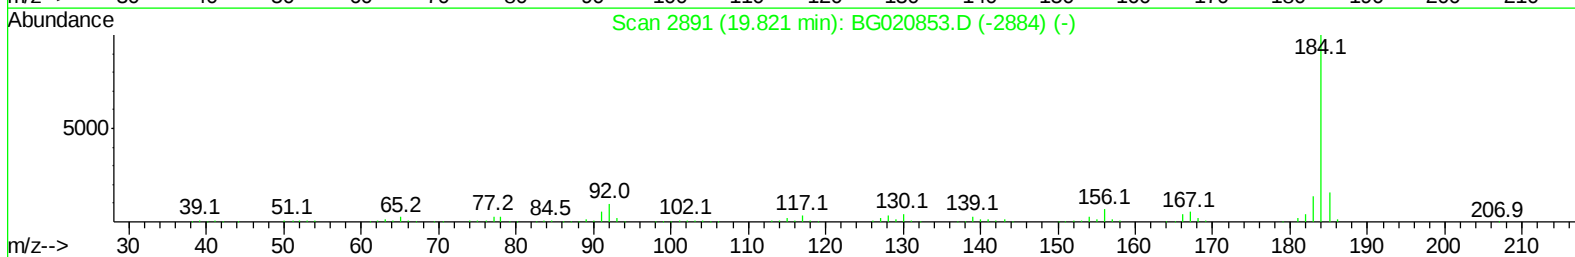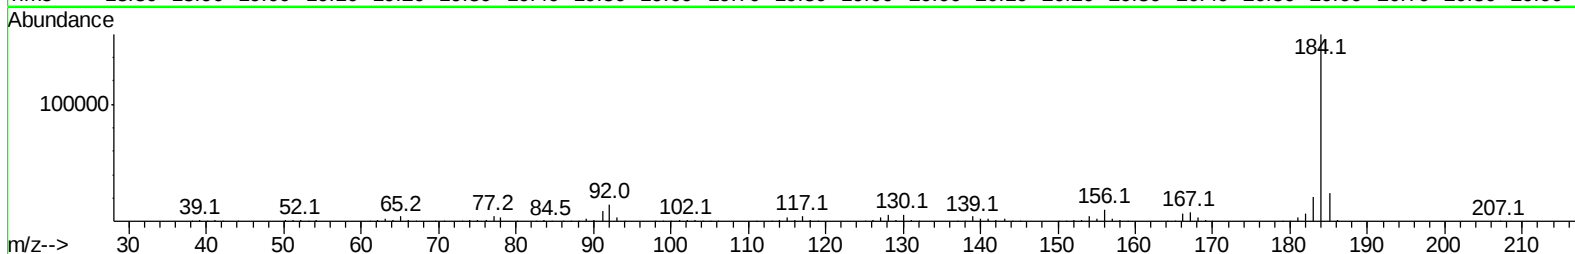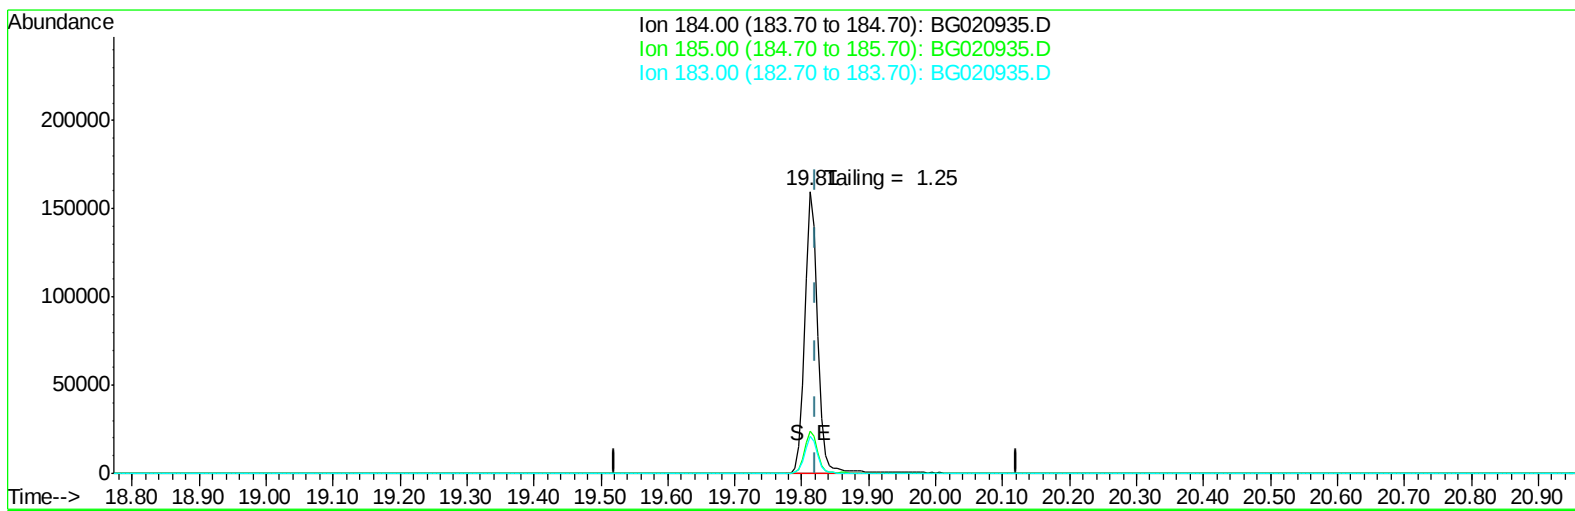

TIC: BG020935.D

(76) Benzidine

19.812min (-0.009) 61911.14ng

response 220222

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.00
183.00	13.70	13.25
0.00	0.00	0.00