

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
 Data File : BG020962.D
 Acq On : 19 Feb 2016 8:14
 Operator : SJ/UM
 Sample : H1453-07 20X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EGR-A-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.090	39	43	54	rVB	54203	72878	18.73%	2.227%
2	3.243	64	69	75	rBV	9219	15229	3.91%	0.465%
3	5.787	497	502	508	rVB2	11161	18232	4.68%	0.557%
4	7.396	769	776	787	rVB2	14064	23737	6.10%	0.725%
5	7.784	836	842	850	rVB	13112	21421	5.50%	0.655%
6	8.260	910	923	930	rBV	85196	145152	37.30%	4.435%
7	8.583	973	978	984	rVB	10296	17294	4.44%	0.528%
8	9.364	1107	1111	1115	rVB3	3030	4453	1.14%	0.136%
9	9.429	1115	1122	1130	rBV	8274	16055	4.13%	0.491%
10	9.893	1197	1201	1207	rBV4	2816	4680	1.20%	0.143%
11	10.468	1295	1299	1305	rBV2	3705	6816	1.75%	0.208%
12	11.085	1394	1404	1411	rBV	144856	256912	66.01%	7.851%
13	11.215	1422	1426	1433	rVB	9472	14856	3.82%	0.454%
14	11.285	1433	1438	1444	rBV3	2950	5240	1.35%	0.160%
15	11.555	1478	1484	1491	rVB4	2798	7283	1.87%	0.223%
16	11.767	1516	1520	1526	rVB5	5669	9563	2.46%	0.292%
17	11.984	1550	1557	1563	rVV7	3292	7077	1.82%	0.216%
18	12.072	1567	1572	1576	rVV2	10910	18670	4.80%	0.571%
19	12.113	1576	1579	1584	rVV4	4366	6962	1.79%	0.213%
20	12.166	1584	1588	1593	rVB3	3890	6967	1.79%	0.213%
21	12.260	1599	1604	1610	rVB5	6698	10639	2.73%	0.325%
22	12.448	1630	1636	1640	rBV4	3364	7487	1.92%	0.229%
23	12.601	1658	1662	1667	rVB5	3477	6892	1.77%	0.211%
24	12.677	1667	1675	1678	rBV4	5138	9645	2.48%	0.295%
25	12.718	1678	1682	1687	rVB	9288	14850	3.82%	0.454%
26	12.801	1691	1696	1701	rVB6	1953	4318	1.11%	0.132%
27	12.936	1714	1719	1722	rBV	6937	11717	3.01%	0.358%
28	13.147	1750	1755	1763	rVB8	4912	9353	2.40%	0.286%
29	13.394	1791	1797	1807	rBV4	19899	31188	8.01%	0.953%
30	13.500	1809	1815	1821	rVV	27590	41532	10.67%	1.269%
31	13.664	1838	1843	1845	rVV4	5139	8755	2.25%	0.268%
32	13.688	1845	1847	1853	rVV6	5488	9813	2.52%	0.300%
33	13.764	1856	1860	1863	rVV6	4422	8027	2.06%	0.245%
34	13.811	1866	1868	1876	rVV8	6501	13605	3.50%	0.416%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
 Data File : BG020962.D
 Acq On : 19 Feb 2016 8:14
 Operator : SJ/UM
 Sample : H1453-07 20X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EGR-A-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.911	1880	1885	1893	rVB5	5830	13404	3.44%	0.410%
36	14.034	1901	1906	1907	rBV	11209	14047	3.61%	0.429%
37	14.052	1907	1909	1915	rVB6	10670	16546	4.25%	0.506%
38	14.146	1920	1925	1928	rBV6	3918	6428	1.65%	0.196%
39	14.193	1928	1933	1937	rVV3	18959	32903	8.45%	1.005%
40	14.246	1937	1942	1946	rVB4	16375	25504	6.55%	0.779%
41	14.293	1946	1950	1953	rBV4	10363	17226	4.43%	0.526%
42	14.328	1953	1956	1961	rVB2	31282	40453	10.39%	1.236%
43	14.375	1961	1964	1968	rBV5	5756	8444	2.17%	0.258%
44	14.428	1968	1973	1982	rVB6	7114	14396	3.70%	0.440%
45	14.598	1998	2002	2003	rBV3	4769	5488	1.41%	0.168%
46	14.698	2012	2019	2025	rBV7	8673	15581	4.00%	0.476%
47	14.821	2035	2040	2042	rBV4	5350	10007	2.57%	0.306%
48	14.874	2042	2049	2057	rVV2	219222	364968	93.78%	11.152%
49	14.945	2058	2061	2064	rVB4	5898	5911	1.52%	0.181%
50	15.074	2077	2083	2089	rVB5	10590	21348	5.49%	0.652%
51	15.150	2093	2096	2100	rBV6	3261	5819	1.50%	0.178%
52	15.256	2107	2114	2121	rVB3	14342	30934	7.95%	0.945%
53	15.338	2123	2128	2132	rBV2	10579	20321	5.22%	0.621%
54	15.473	2146	2151	2156	rBV4	11503	21468	5.52%	0.656%
55	15.526	2156	2160	2164	rVV2	9783	13987	3.59%	0.427%
56	15.579	2165	2169	2173	rVB7	6365	10126	2.60%	0.309%
57	15.650	2173	2181	2184	rBV8	9264	21560	5.54%	0.659%
58	15.679	2184	2186	2189	rVB3	7088	7278	1.87%	0.222%
59	15.738	2192	2196	2200	rBV4	4737	8129	2.09%	0.248%
60	15.797	2203	2206	2215	rVB7	5113	11801	3.03%	0.361%
61	15.873	2215	2219	2220	rBV3	3045	4217	1.08%	0.129%
62	15.896	2220	2223	2225	rBV3	4507	4897	1.26%	0.150%
63	16.037	2243	2247	2249	rBV3	3772	4300	1.10%	0.131%
64	16.084	2249	2255	2266	rVB2	28665	59803	15.37%	1.827%
65	16.173	2267	2270	2274	rBV6	4157	6668	1.71%	0.204%
66	16.308	2289	2293	2296	rBV3	4407	5547	1.43%	0.170%
67	16.349	2296	2300	2305	rVV3	13987	18195	4.68%	0.556%
68	16.490	2319	2324	2328	rVB6	3326	5997	1.54%	0.183%
69	16.566	2328	2337	2342	rBV	54937	87161	22.40%	2.663%
70	16.666	2351	2354	2357	rBV4	2881	4361	1.12%	0.133%
71	16.713	2357	2362	2366	rVV5	5264	9261	2.38%	0.283%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
 Data File : BG020962.D
 Acq On : 19 Feb 2016 8:14
 Operator : SJ/UM
 Sample : H1453-07 20X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EGR-A-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	16.889	2387	2392	2396	rBV7	3898	6863	1.76%	0.210%
73	16.942	2398	2401	2402	rBV3	4574	4532	1.16%	0.138%
74	17.118	2426	2431	2433	rBV5	3981	5833	1.50%	0.178%
75	17.154	2435	2437	2440	rVV3	5705	6919	1.78%	0.211%
76	17.183	2440	2442	2448	rVB6	3940	7108	1.83%	0.217%
77	17.389	2471	2477	2481	rBV	30611	45999	11.82%	1.406%
78	17.606	2506	2514	2520	rBV2	240664	365542	93.92%	11.170%
79	17.794	2541	2546	2550	rBV6	5013	10782	2.77%	0.329%
80	17.994	2576	2580	2584	rBV4	7967	10494	2.70%	0.321%
81	18.328	2633	2637	2641	rBV4	3050	4351	1.12%	0.133%
82	18.475	2657	2662	2665	rBV2	5716	8657	2.22%	0.265%
83	18.516	2667	2669	2676	rVV4	7382	11158	2.87%	0.341%
84	18.616	2680	2686	2689	rVV6	5482	12546	3.22%	0.383%
85	18.646	2689	2691	2695	rVV4	5227	8735	2.24%	0.267%
86	18.704	2698	2701	2709	rVB8	6655	10300	2.65%	0.315%
87	19.204	2783	2786	2790	rVB3	6281	7863	2.02%	0.240%
88	19.257	2792	2795	2797	rBV4	4468	4057	1.04%	0.124%
89	19.374	2811	2815	2819	rVB2	7857	10819	2.78%	0.331%
90	19.633	2855	2859	2862	rBV4	3911	6255	1.61%	0.191%
91	19.685	2866	2868	2872	rVB4	5592	5527	1.42%	0.169%
92	19.738	2872	2877	2880	rBV6	2692	4790	1.23%	0.146%
93	20.003	2919	2922	2927	rVB5	6814	9755	2.51%	0.298%
94	20.067	2929	2933	2936	rVB3	5024	6743	1.73%	0.206%
95	20.120	2938	2942	2945	rBV6	3639	5286	1.36%	0.162%
96	20.179	2949	2952	2956	rVB	37586	47368	12.17%	1.447%
97	20.396	2985	2989	2992	rBV5	5633	8633	2.22%	0.264%
98	21.741	3214	3218	3224	rVB2	12345	20694	5.32%	0.632%
99	21.882	3235	3242	3249	rVB	228532	389194	100.00%	11.893%
100	25.248	3805	3815	3832	rVB2	132984	383940	98.65%	11.732%


Sum of corrected areas: 3272525

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020962.D
Acq On : 19 Feb 2016 8:14
Operator : SJ/UM
Sample : H1453-07 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
EGR-A-4

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

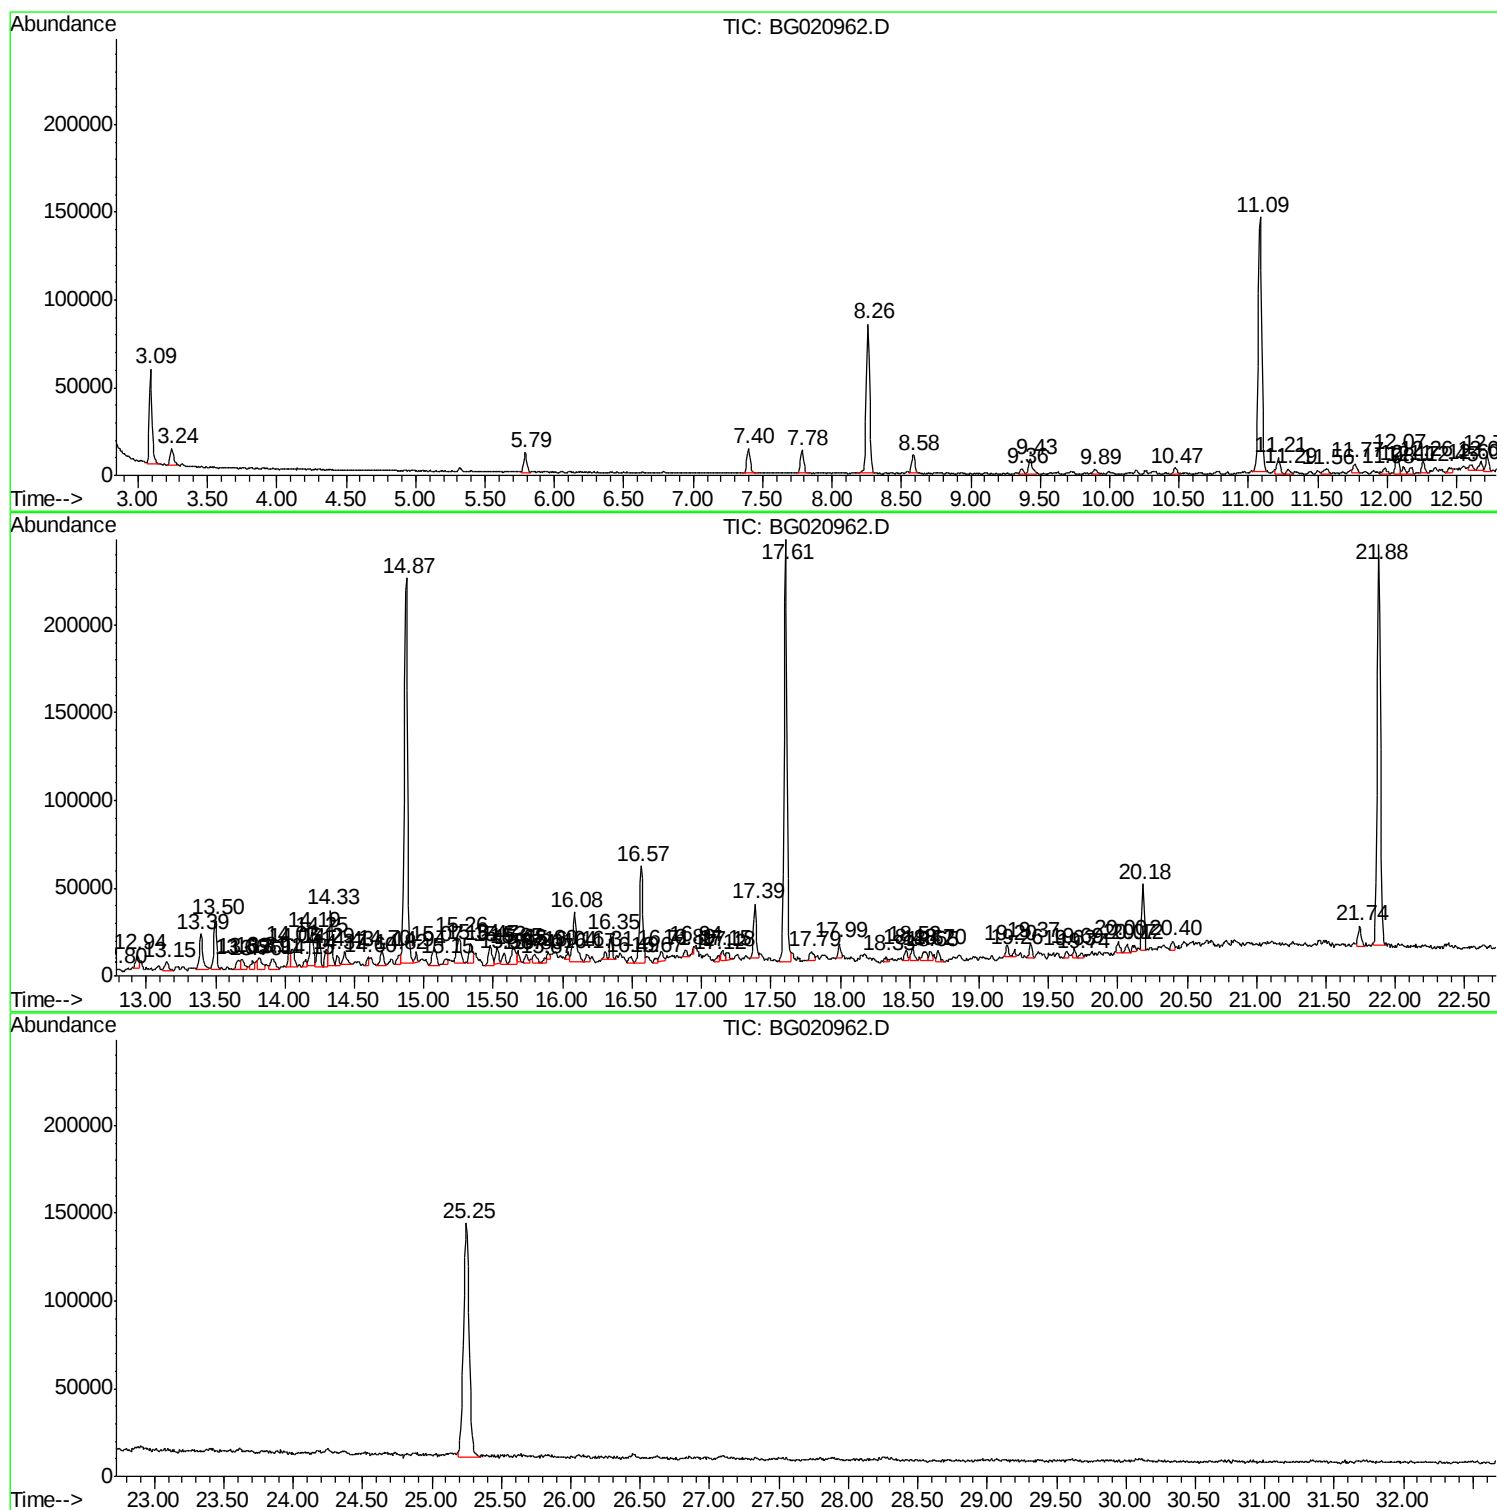

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020962.D
Acq On : 19 Feb 2016 8:14
Operator : SJ/UM
Sample : H1453-07 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EGR-A-4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown3.09 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.09	10.04 ng	72878	1,4-Dichlorobenzene-d4	8.26

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Hydroxy-2-methylbutyric acid	118	C5H10O3	003739-30-8	25
2		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	25
3		Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	9
4		Methane, isothiocyanato-	73	C2H3NS	000556-61-6	7
5		N-Ethylformamide	73	C3H7NO	000627-45-2	5

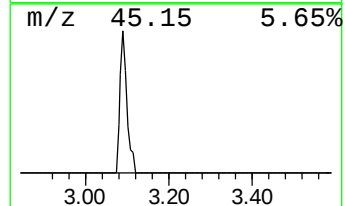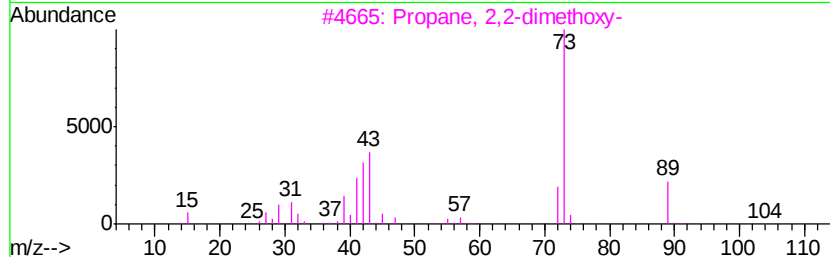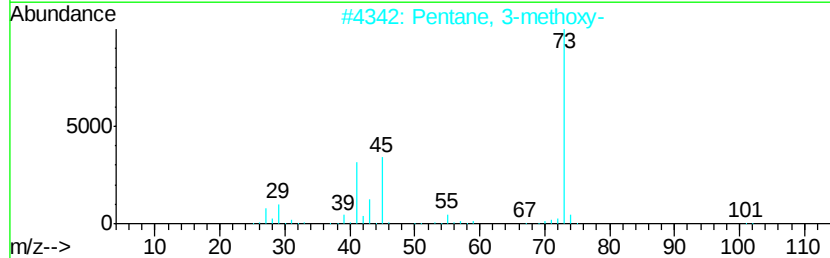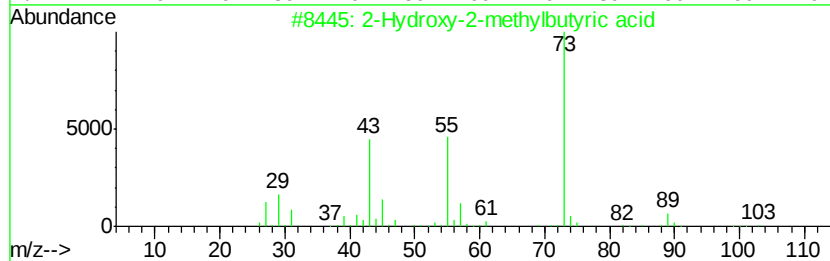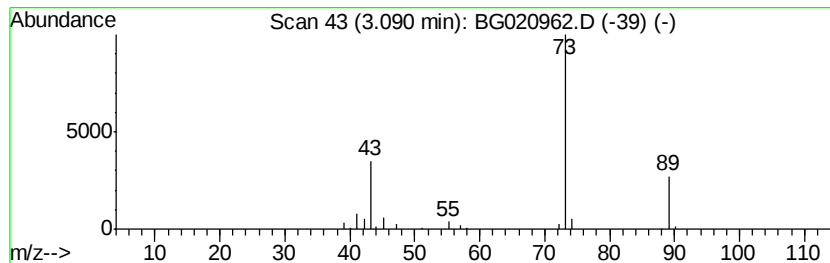

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020962.D
Acq On : 19 Feb 2016 8:14
Operator : SJ/UM
Sample : H1453-07 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EGR-A-4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown3.24 Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.24	2.10 ng	15229	1,4-Dichlorobenzene-d4	8.26

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclohexane	84	C6H12	000110-82-7	90
2		Cyclobutanone, 2-methyl-	84	C5H8O	001517-15-3	50
3		1-Hexene, 3,4-dimethyl-	112	C8H16	016745-94-1	39
4		2-Amino-oxazole	84	C3H4N2O	004570-45-0	32
5		Furan, 2,3-dihydro-4-methyl-	84	C5H8O	034314-83-5	9

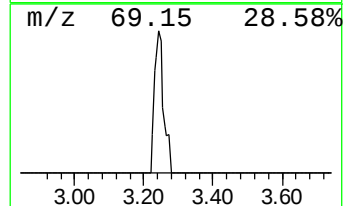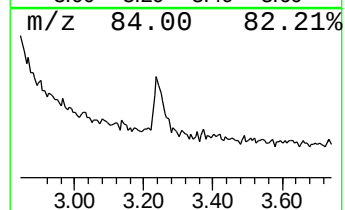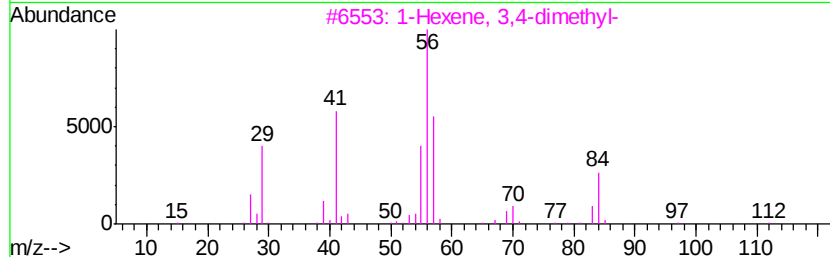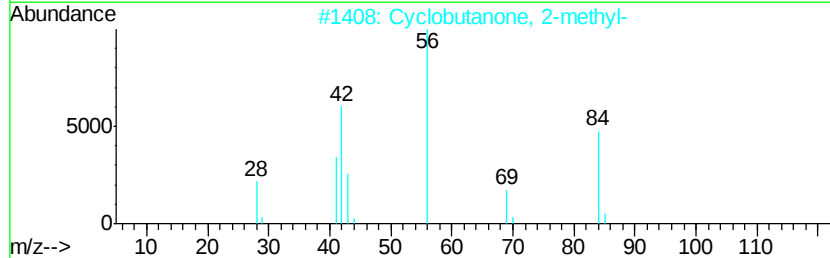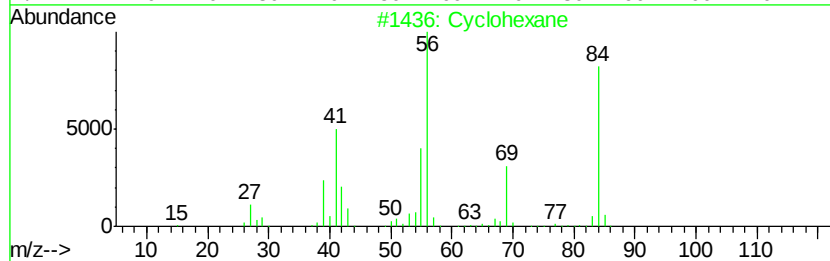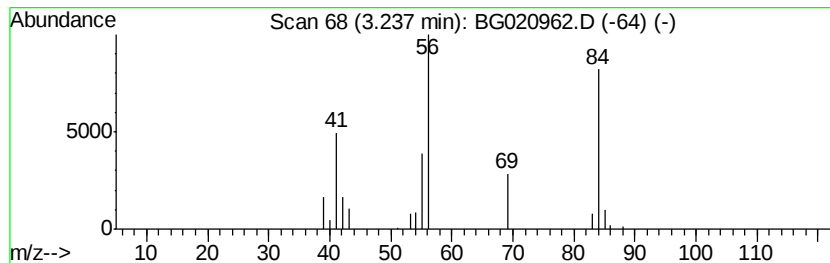

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020962.D
Acq On : 19 Feb 2016 8:14
Operator : SJ/UM
Sample : H1453-07 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EGR-A-4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown7.78 Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.78	2.95 ng	21421	1,4-Dichlorobenzene-d4	8.26

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	12
4			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	9
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

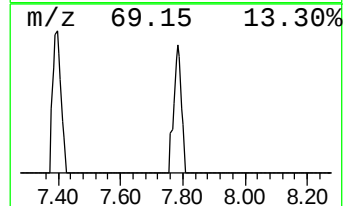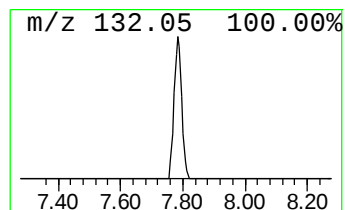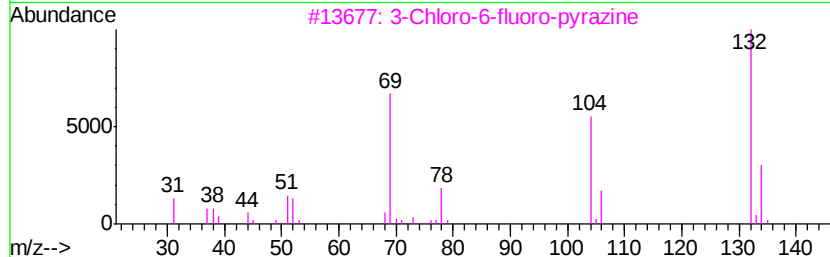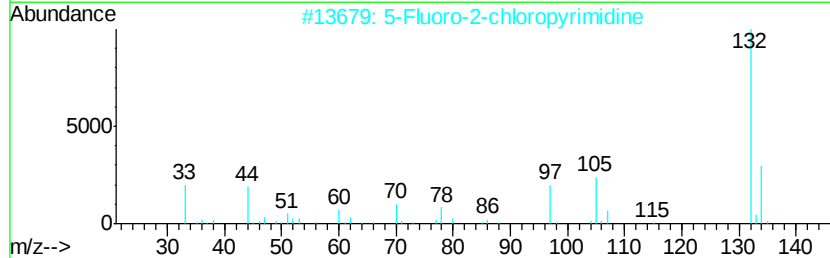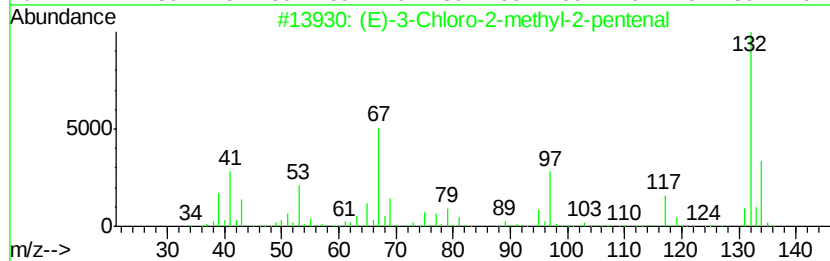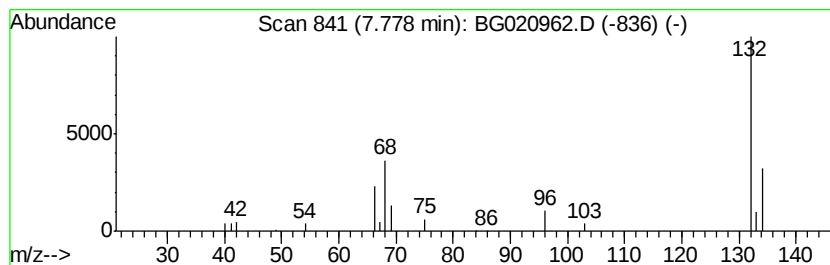

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020962.D
Acq On : 19 Feb 2016 8:14
Operator : SJ/UM
Sample : H1453-07 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EGR-A-4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 Dodecane, 2,6,11-trimethyl- Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.33	2.22 ng	40453	Acenaphthene-d10	14.87

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Dodecane, 2,6,11-trimethyl-	212	C15H32	031295-56-4	72	
2	Nonane, 3-methyl-5-propyl-	184	C13H28	031081-18-2	59	
3	Tetradecane, 1-iodo-	324	C14H29I	019218-94-1	53	
4	Nonane	128	C9H20	000111-84-2	50	
5	Octadecane	254	C18H38	000593-45-3	47	

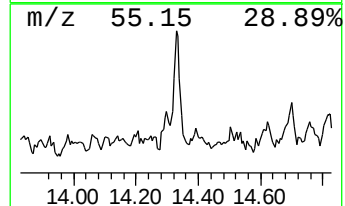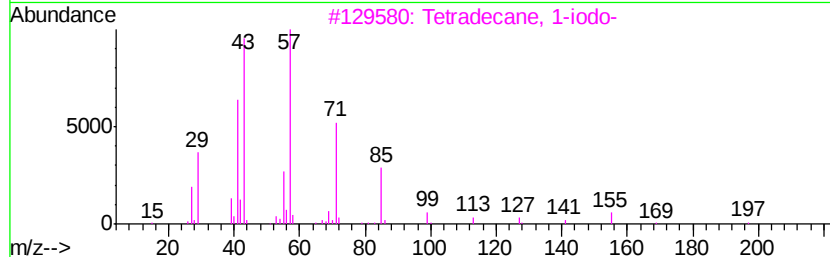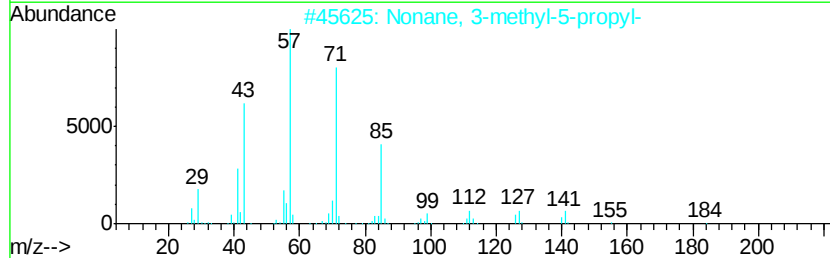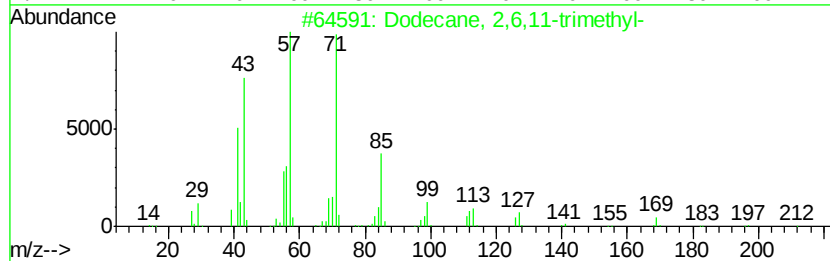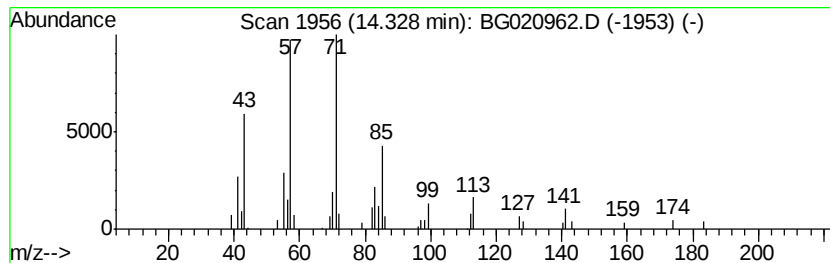

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020962.D
Acq On : 19 Feb 2016 8:14
Operator : SJ/UM
Sample : H1453-07 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EGR-A-4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 Pentadecane, 2,6,10-trimethyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.08	3.28 ng	59803	Acenaphthene-d10	14.87

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Pentadecane, 2,6,10-trimethyl-	254	C18H38	003892-00-0	90
2		Tridecane	184	C13H28	000629-50-5	83
3		Tridecane, 1-iodo-	310	C13H27I	035599-77-0	80
4		Hexacosane	366	C26H54	000630-01-3	80
5		Decane, 2,6,8-trimethyl-	184	C13H28	062108-26-3	76

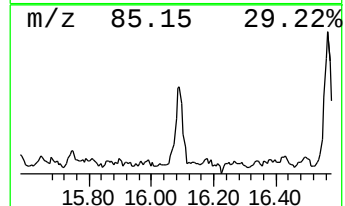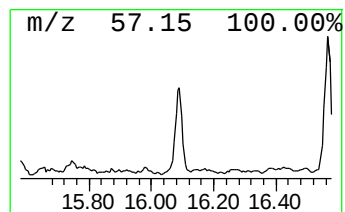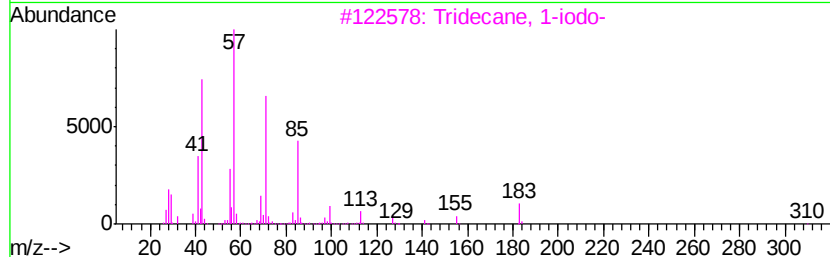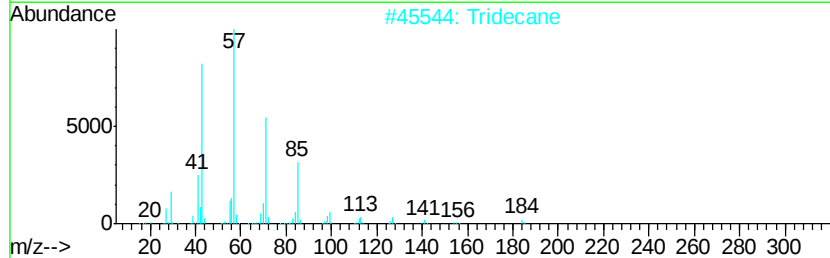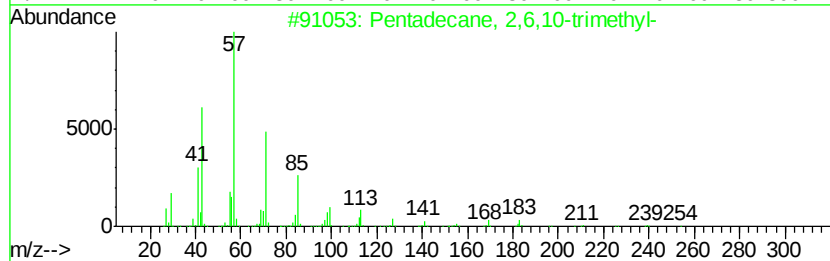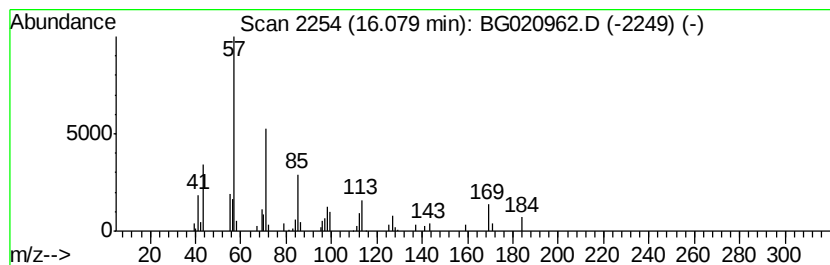

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020962.D
Acq On : 19 Feb 2016 8:14
Operator : SJ/UM
Sample : H1453-07 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EGR-A-4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Dodecane, 2,6,10-trimethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.57	4.77 ng	87161	Phenanthrene-d10	17.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Dodecane, 2,6,10-trimethyl-	212	C15H32	003891-98-3	86
2		Hexadecane, 2,6,11,15-tetramethyl-	282	C20H42	000504-44-9	72
3		Dodecane, 2,7,10-trimethyl-	212	C15H32	074645-98-0	72
4		Tridecane	184	C13H28	000629-50-5	72
5		5,5-Dibutylnonane	240	C17H36	006008-17-9	72

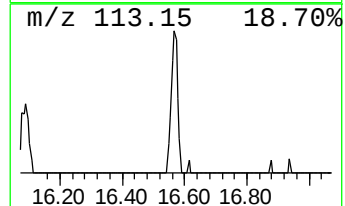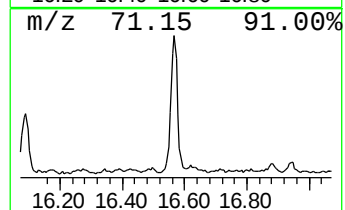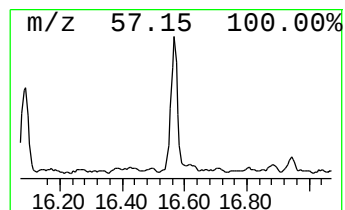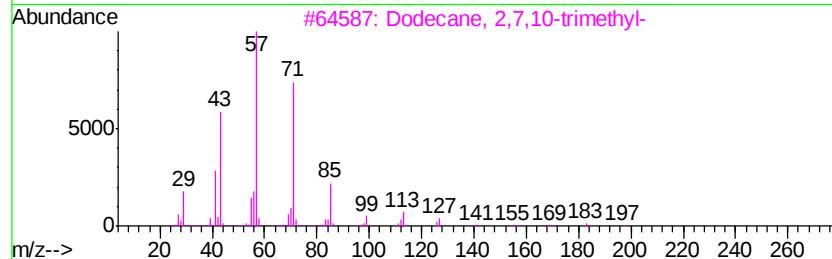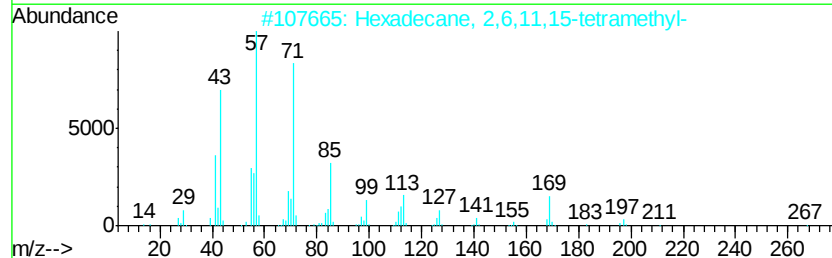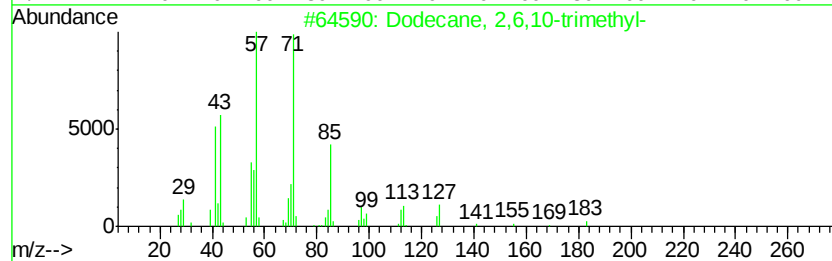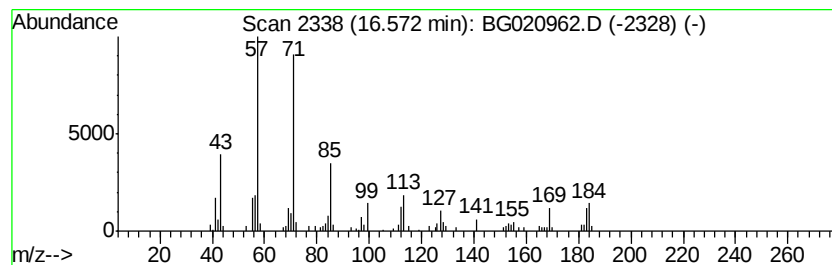

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
Data File : BG020962.D
Acq On : 19 Feb 2016 8:14
Operator : SJ/UM
Sample : H1453-07 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EGR-A-4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 8 Hexadecane, 2,6,10,14-tetra... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.39	2.52 ng	45999	Phenanthrene-d10	17.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Hexadecane, 2,6,10,14-tetramethyl-	282	C20H42	000638-36-8	83
2		Nonacosane	408	C29H60	000630-03-5	80
3		Silane, trichlorooctadecyl-	386	C18H37Cl3Si	000112-04-9	78
4		triacontane	422	C30H62	000638-68-6	72
5		Hexacosane	366	C26H54	000630-01-3	64

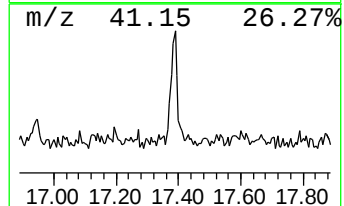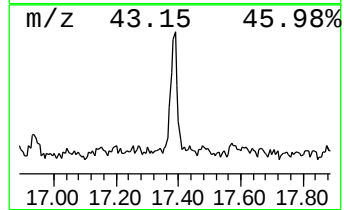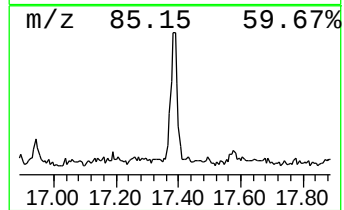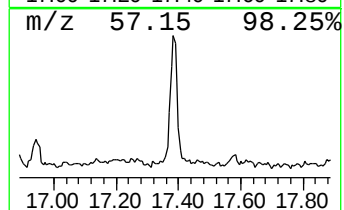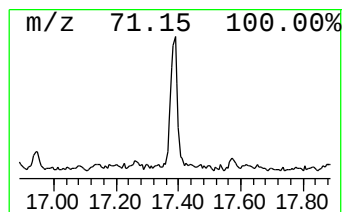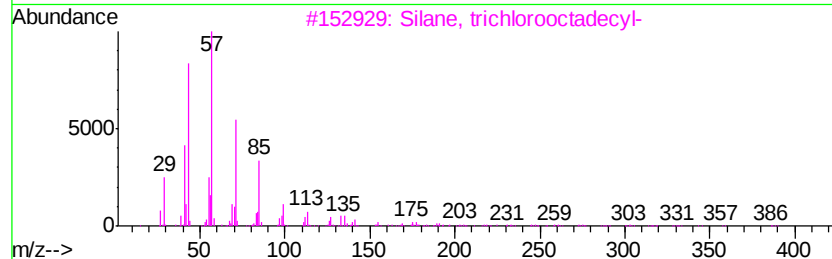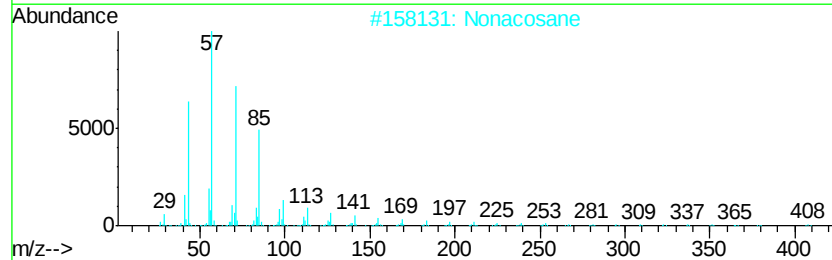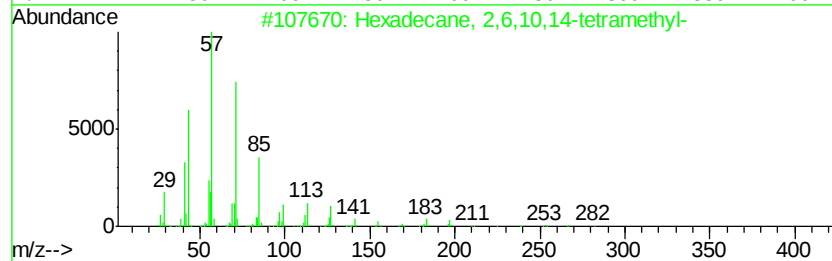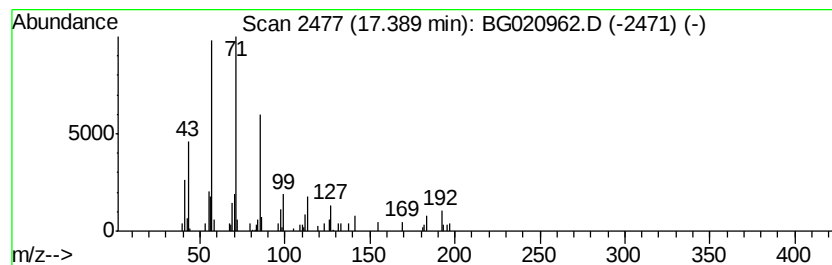

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021816\
Data File : BG020962.D
Acq On : 19 Feb 2016 8:14
Operator : SJ/UM
Sample : H1453-07 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EGR-A-4

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.09	3.09	10.0	ng	72878	1	8.26	145152	20.0
unknown3.24	3.24	2.1	ng	15229	1	8.26	145152	20.0
unknown7.78	7.78	3.0	ng	21421	1	8.26	145152	20.0
Dodecane, 2,6,11-...	14.33	2.2	ng	40453	3	14.87	364968	20.0
Pentadecane, 2,6,...	16.08	3.3	ng	59803	3	14.87	364968	20.0
Dodecane, 2,6,10-...	16.57	4.8	ng	87161	4	17.61	365542	20.0
Hexadecane, 2,6,1...	17.39	2.5	ng	45999	4	17.61	365542	20.0