


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
 Data File : BG020935.D
 Acq On : 18 Feb 2016 13:53
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 11 15:26:53 2016

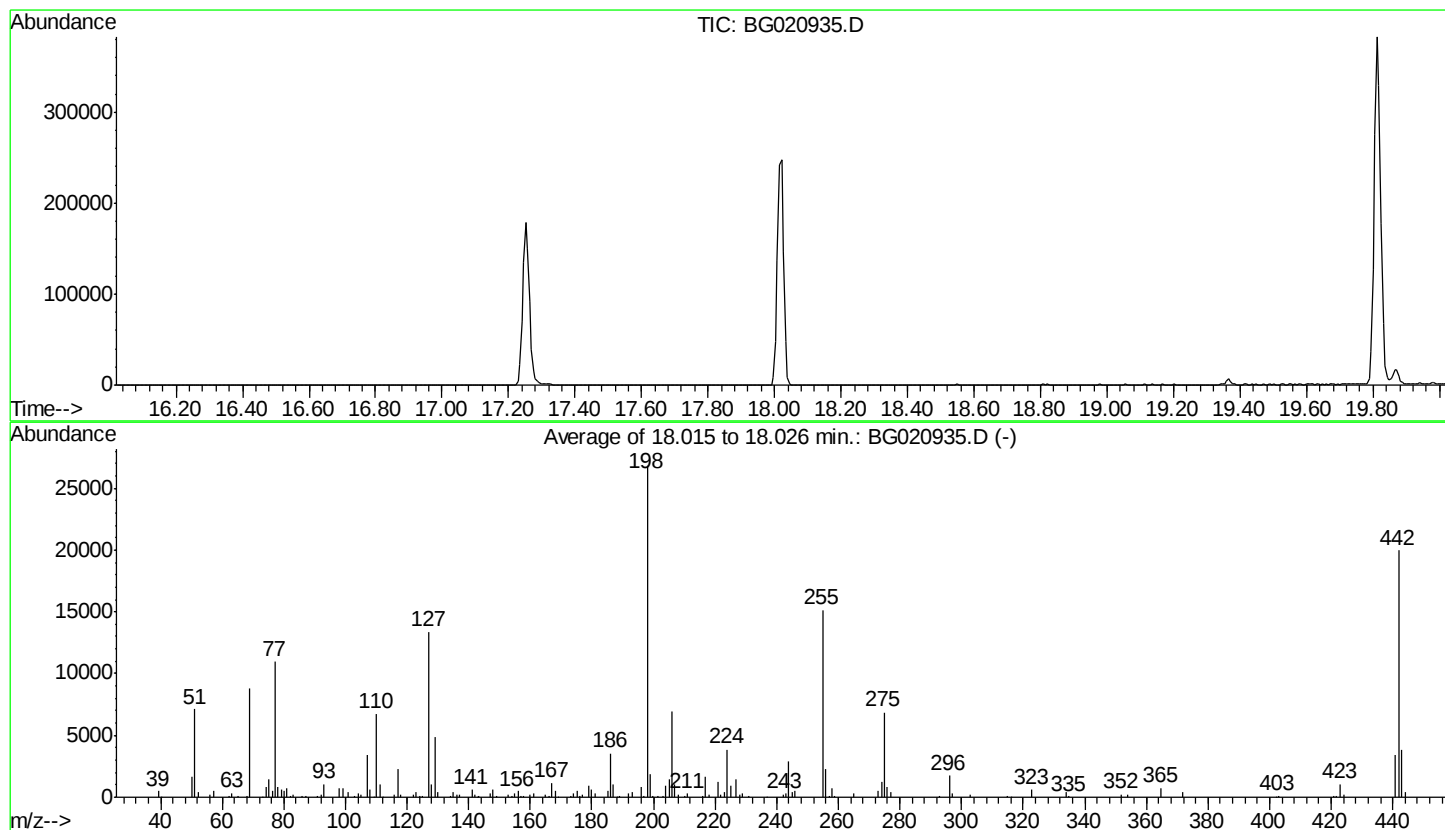

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	7129	PASS
68	69	0.00	2	0.8	67	PASS
69	198	0.00	100	32.7	8759	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	13388	PASS
197	198	0.00	2	0.3	74	PASS
198	198	100	100	100.0	26824	PASS
199	198	5	9	7.0	1871	PASS
275	198	10	60	25.6	6871	PASS
365	198	1	100	2.9	777	PASS
441	442	0.01	24	17.1	3418	PASS
442	198	50	100	74.4	19968	PASS
443	442	15	24	19.5	3885	PASS