


Data Path : Z:\HPCHEM1\BNA G\DATA\BG021816\
 Data File : BG020951.D
 Acq On : 19 Feb 2016 1:04
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 11 15:26:53 2016

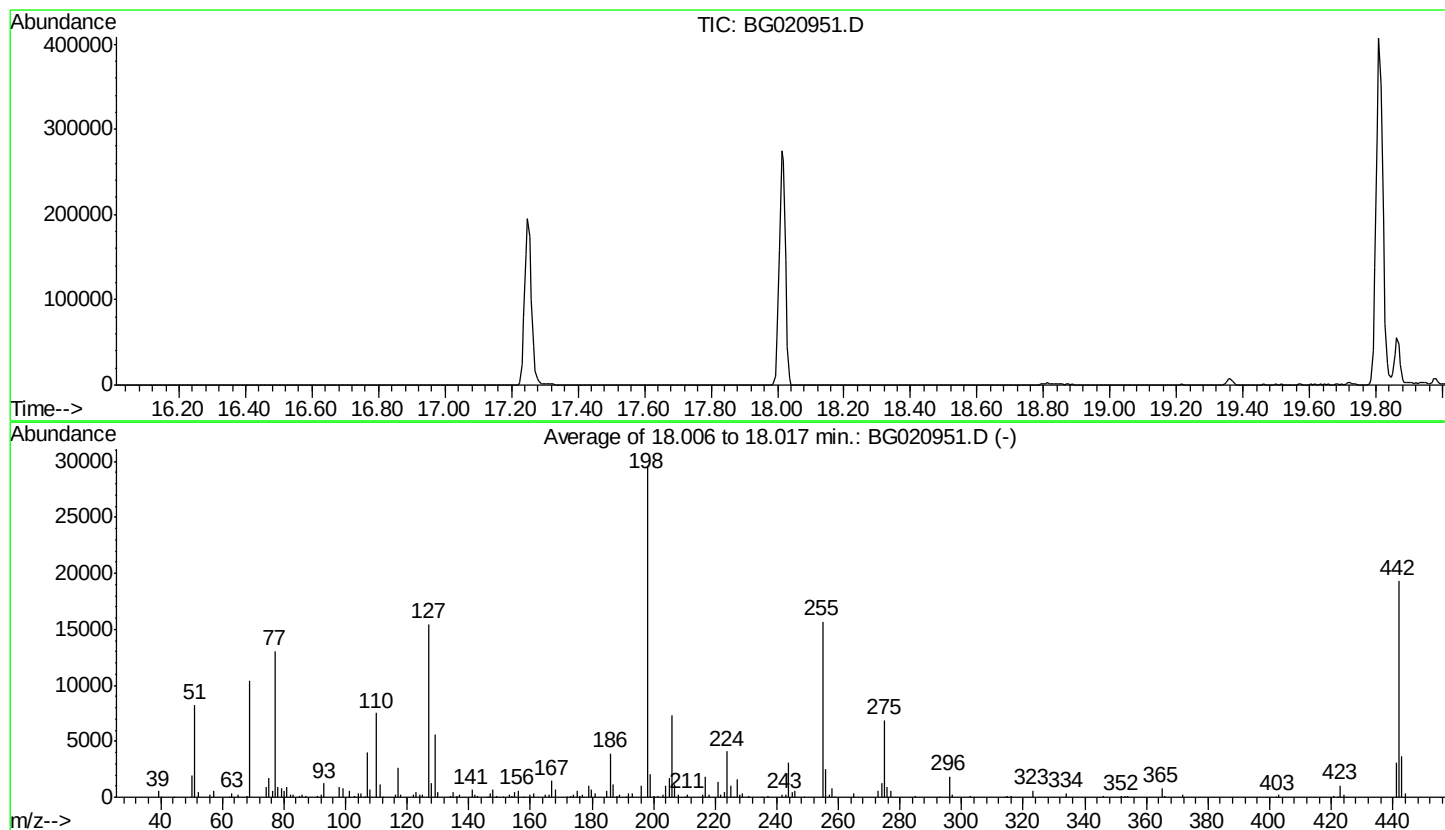

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	8252	PASS
68	69	0.00	2	0.6	66	PASS
69	198	0.00	100	35.2	10437	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	15472	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29616	PASS
199	198	5	9	6.8	2023	PASS
275	198	10	60	23.2	6874	PASS
365	198	1	100	2.7	801	PASS
441	442	0.01	24	16.0	3107	PASS
442	198	50	100	65.4	19363	PASS
443	442	15	24	19.1	3704	PASS