
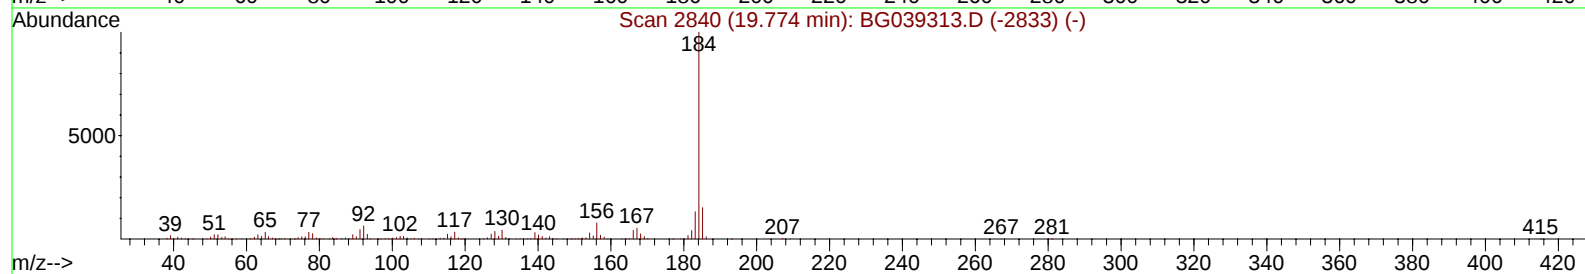
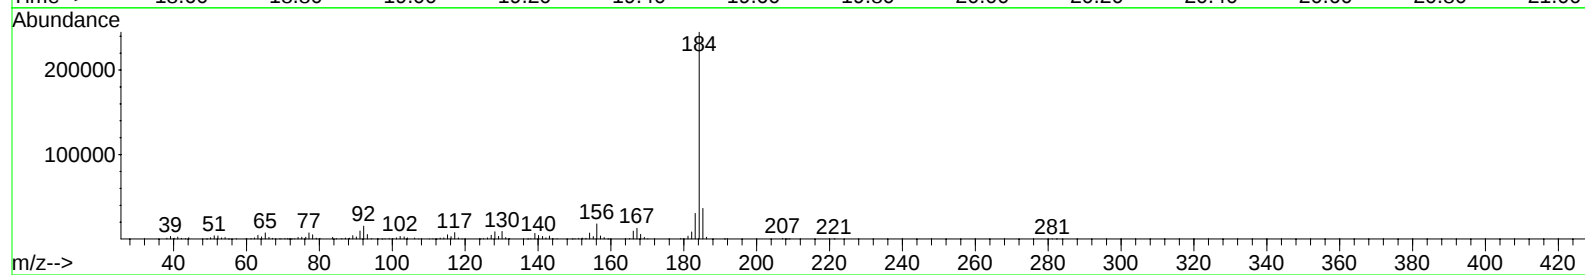


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021819\
Data File : BG039537.D
Acq On : 18 Feb 2019 12:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 17:24:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

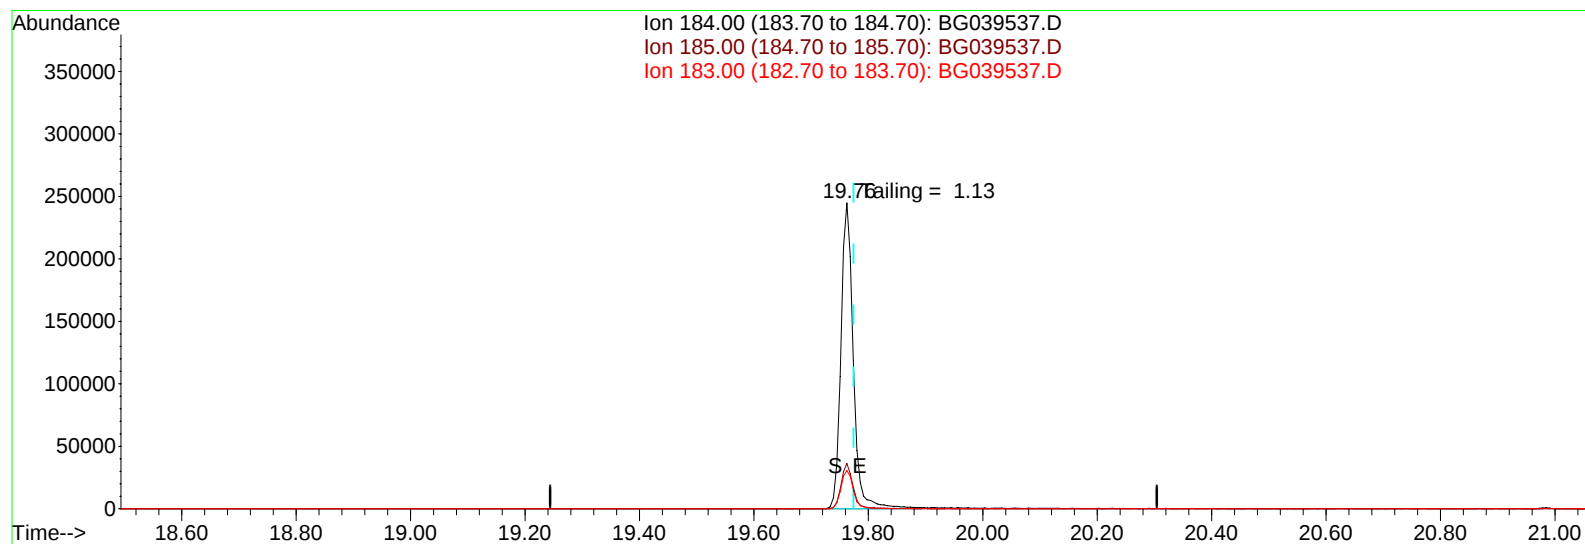

TIC: BG039537.D

(77) Benzidine




19.763min (-0.012) 0.00ng

response 367679

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.83
183.00	13.20	12.48
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021819\
Data File : BG039537.D
Acq On : 18 Feb 2019 12:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 17:24:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

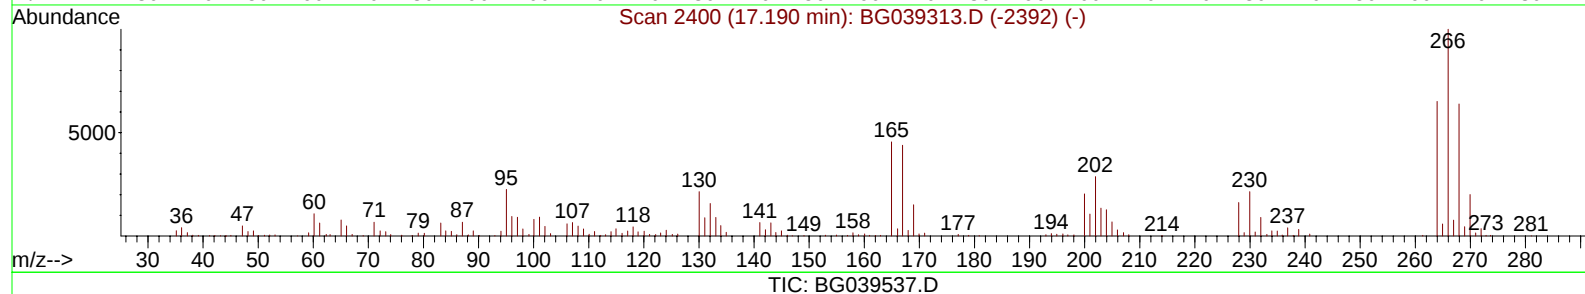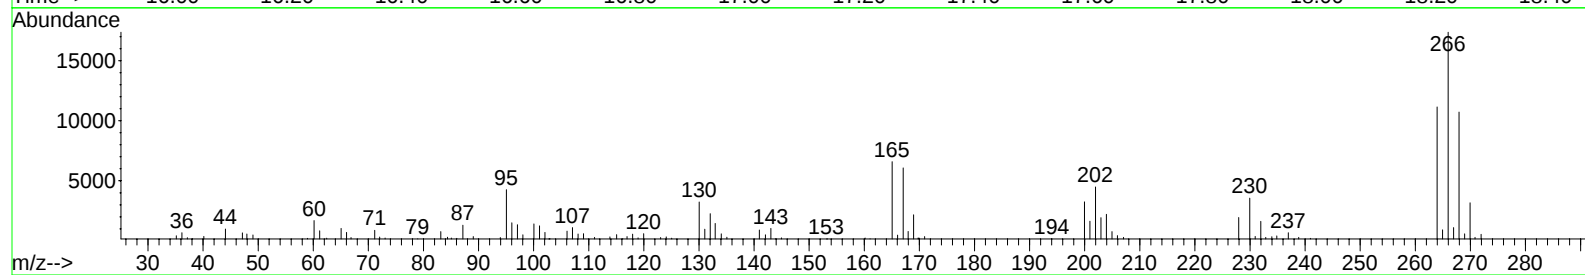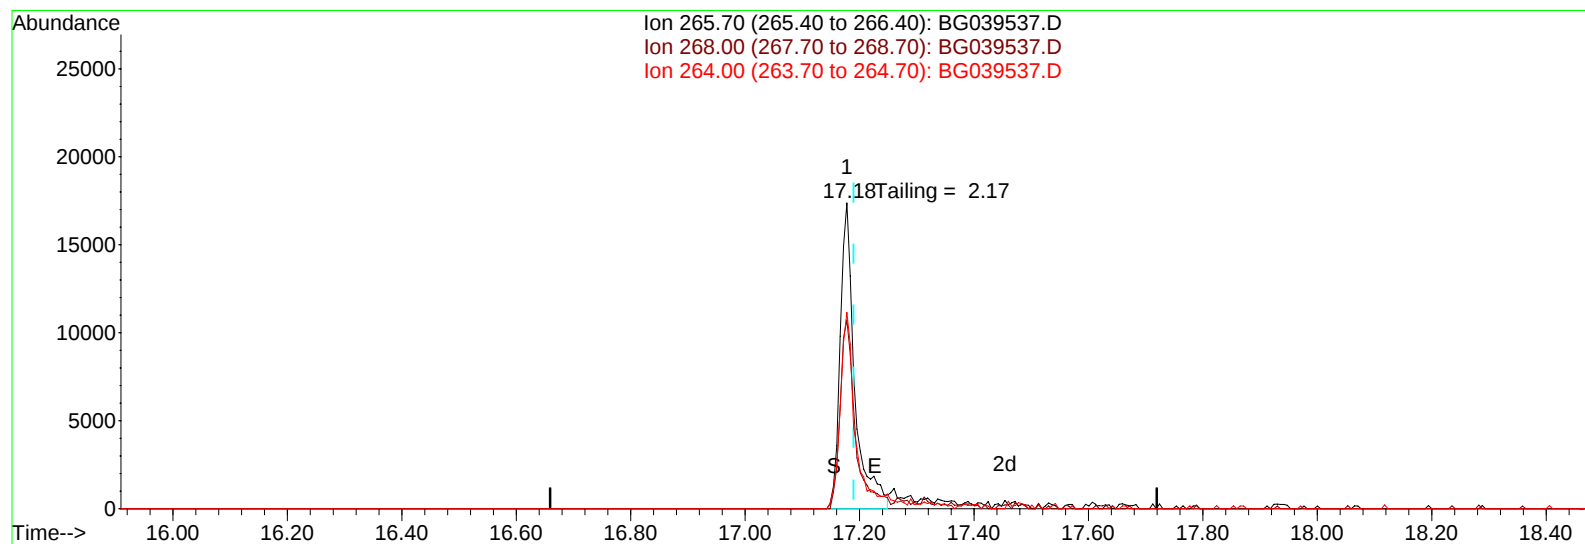

(70) Pentachlorophenol (C)

17.178min (-0.012) 72751.75ng

response 30954

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.75
264.00	65.10	64.21
0.00	0.00	0.00