

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
 Data File : BG052421.D
 Acq On : 18 Feb 2022 10:19
 Operator : CG/JU
 Sample : PB142721BL
 Misc : LOQ-WATER 10ppm
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.548	6	10	19	rVB2	7490	12206	1.36%	0.149%
2	3.977	79	83	99	rBV	88523	154210	17.22%	1.882%
3	4.329	141	143	146	rBV2	1336	1623	0.18%	0.020%
4	6.403	492	496	500	rVB2	711	1191	0.13%	0.015%
5	7.372	655	661	669	rBV	105889	183451	20.49%	2.239%
6	7.537	682	689	697	rVB	84915	140117	15.65%	1.710%
7	7.760	721	727	735	rVB	104044	176904	19.76%	2.159%
8	8.230	800	807	816	rVB	84133	139159	15.54%	1.698%
9	8.935	920	927	938	rBV	134007	225789	25.22%	2.755%
10	9.399	999	1006	1015	rVB	108695	191761	21.42%	2.340%
11	10.133	1124	1131	1139	rBV	93848	159023	17.76%	1.941%
12	10.685	1218	1225	1237	rBV	121232	228558	25.53%	2.789%
13	11.067	1281	1290	1300	rBV	118093	212103	23.69%	2.588%
14	11.191	1304	1311	1323	rBV	123538	241009	26.92%	2.941%
15	12.653	1555	1560	1563	rBV3	2052	3321	0.37%	0.041%
16	14.263	1827	1834	1843	rBV	271138	404334	45.16%	4.934%
17	14.568	1879	1886	1896	rBV	307071	482098	53.84%	5.883%
18	14.874	1932	1938	1947	rVB	207373	327916	36.62%	4.002%
19	15.062	1964	1970	1987	rBV	81855	174504	19.49%	2.130%
20	15.861	2097	2106	2115	rBV	391917	605844	67.66%	7.393%
21	15.972	2119	2125	2139	rVV	98940	154745	17.28%	1.888%
22	16.102	2144	2147	2152	rVB	1695	2126	0.24%	0.026%
23	17.623	2398	2406	2416	rBV	287420	445612	49.77%	5.438%
24	17.717	2416	2422	2434	rVB	449925	714243	79.77%	8.716%
25	19.567	2731	2737	2741	rBV4	7206	10183	1.14%	0.124%
26	19.632	2745	2748	2753	rVV2	5312	7171	0.80%	0.088%
27	20.002	2804	2811	2818	rBV	611382	895412	100.00%	10.927%
28	20.219	2845	2848	2849	rVB2	1676	1383	0.15%	0.017%
29	20.255	2849	2854	2855	rBV3	1375	2362	0.26%	0.029%
30	21.071	2990	2993	2994	rBV2	1754	1841	0.21%	0.022%
31	21.118	2999	3001	3002	rBV2	1904	1374	0.15%	0.017%
32	21.723	3102	3104	3105	rBV	2107	1432	0.16%	0.017%
33	21.935	3133	3140	3150	rBV	286989	512031	57.18%	6.248%
34	24.690	3607	3609	3612	rVB3	2735	2307	0.26%	0.028%
35	25.166	3679	3690	3703	rBV2	289324	845706	94.45%	10.320%
36	25.407	3721	3731	3745	rVB2	167712	523224	58.43%	6.385%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
Data File : BG052421.D
Acq On : 18 Feb 2022 10:19
Operator : CG/JU
Sample : PB142721BL
Misc : LOQ-WATER 10ppm
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Title : SVOA CALIBRATION

37	27.891	4152	4154	4156	rBV3	2515	2205	0.25%	0.027%
38	28.079	4184	4186	4187	rBV2	2557	2056	0.23%	0.025%
39	29.918	4497	4499	4502	rBV4	3180	4019	0.45%	0.049%




Sum of corrected areas: 8194553

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
Data File : BG052421.D
Acq On : 18 Feb 2022 10:19
Operator : CG/JU
Sample : PB142721BL
Misc : LOQ-WATER 10ppm
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

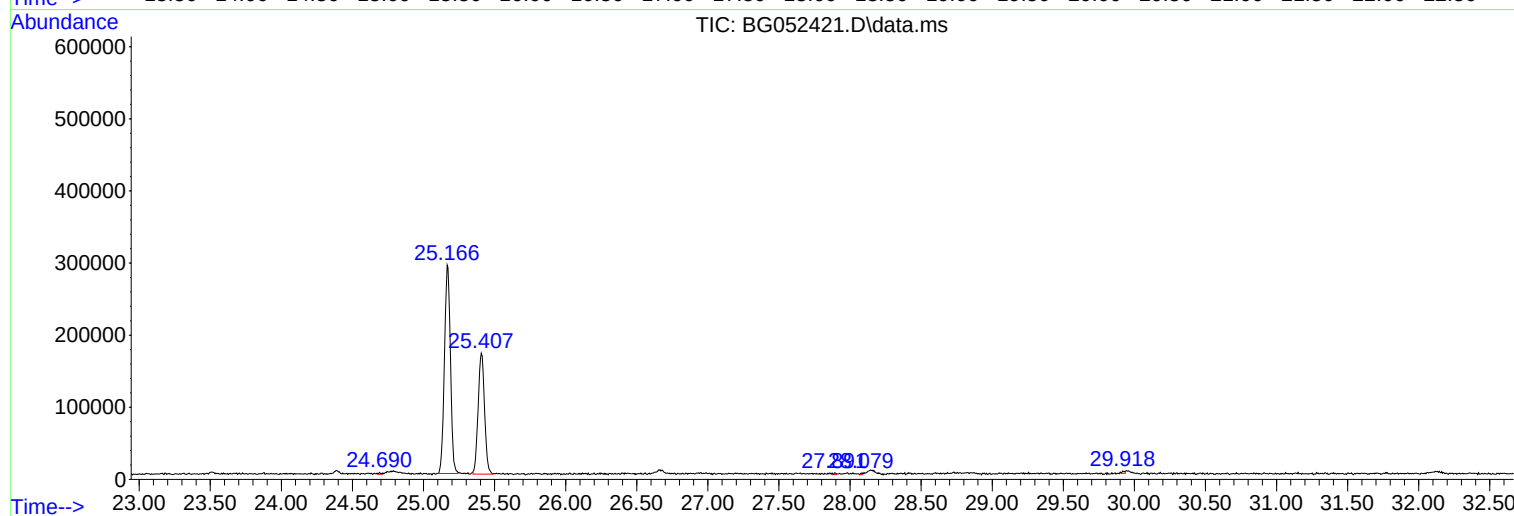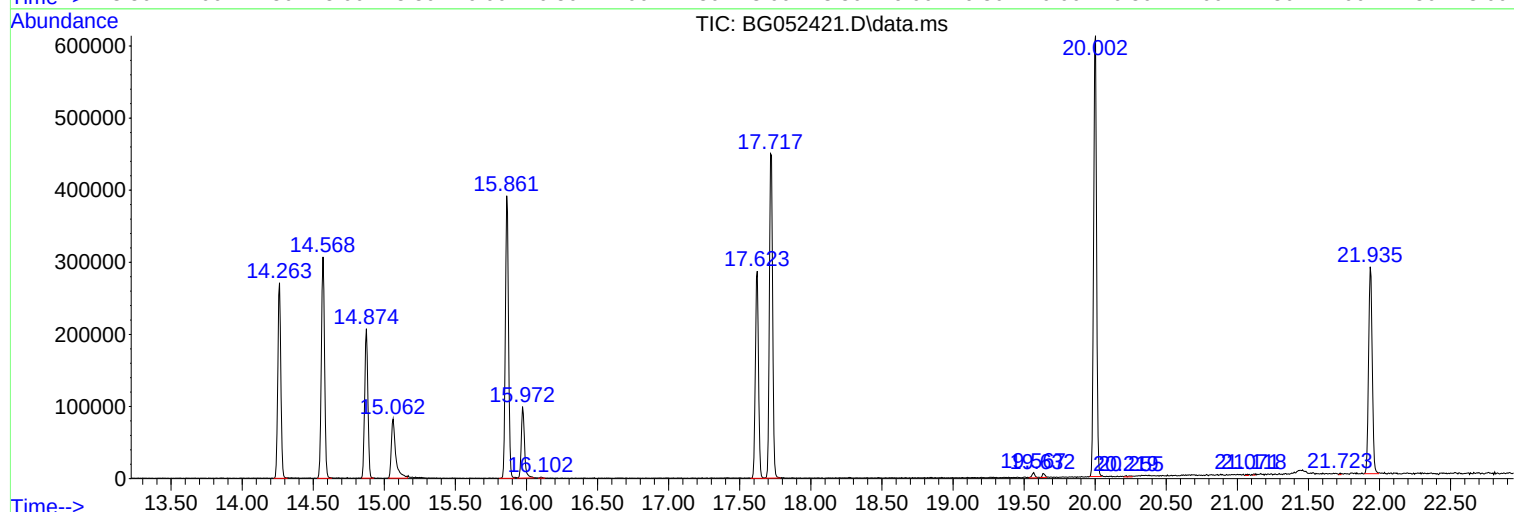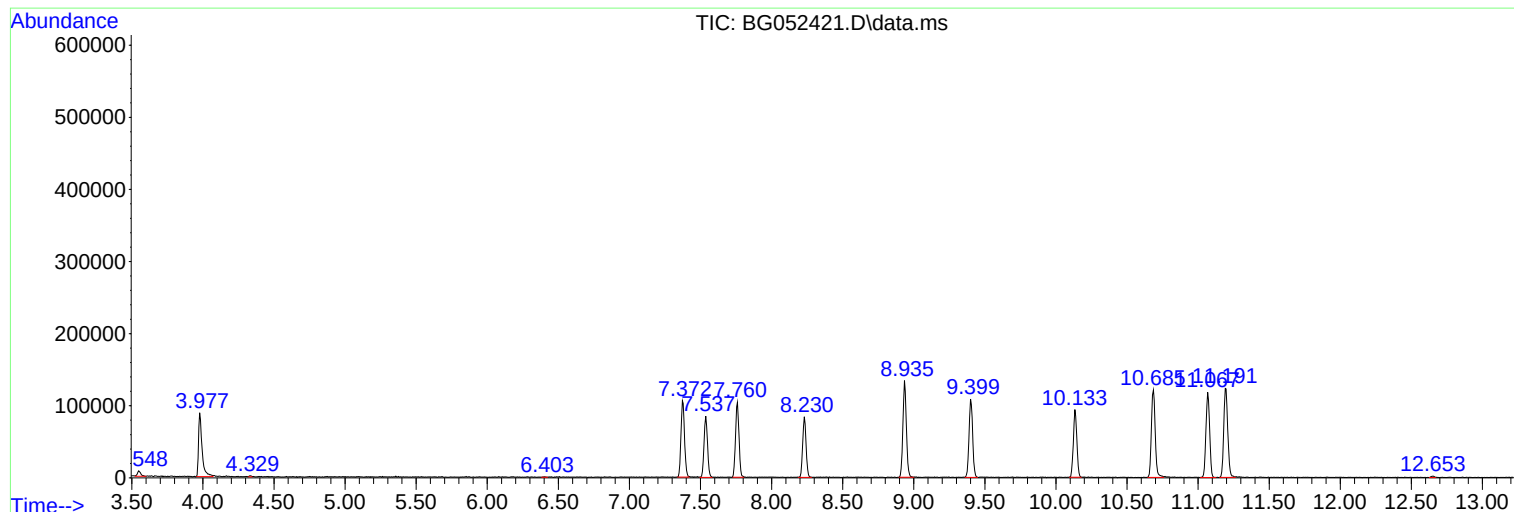

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
Data File : BG052421.D
Acq On : 18 Feb 2022 10:19
Operator : CG/JU
Sample : PB142721BL
Misc : LOQ-WATER 10ppm
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
Data File : BG052421.D
Acq On : 18 Feb 2022 10:19
Operator : CG/JU
Sample : PB142721BL
Misc : LOQ-WATER 10ppm
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
