

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
 Data File : BG052425.D
 Acq On : 18 Feb 2022 16:53
 Operator : CG/JU
 Sample : PB142721BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.548	6	10	13	rBV3	7605	11208	1.19%	0.128%
2	3.977	78	83	96	rBV	92389	162006	17.15%	1.845%
3	4.329	140	143	146	rBV3	2000	2095	0.22%	0.024%
4	5.962	415	421	424	rVB	909	1588	0.17%	0.018%
5	6.532	515	518	521	rBV2	1572	1691	0.18%	0.019%
6	7.366	654	660	667	rVV	112203	194052	20.54%	2.210%
7	7.531	680	688	696	rBV	83641	144058	15.25%	1.641%
8	7.754	719	726	735	rBV	107075	181963	19.26%	2.072%
9	8.224	799	806	812	rBV	85565	147507	15.61%	1.680%
10	8.929	917	926	935	rBV	136154	234549	24.83%	2.671%
11	9.399	998	1006	1013	rBV	107591	198212	20.98%	2.257%
12	10.127	1121	1130	1140	rBV2	92000	169016	17.89%	1.925%
13	10.679	1216	1224	1233	rBV	127005	235793	24.96%	2.685%
14	10.773	1238	1240	1244	rVV3	1410	1861	0.20%	0.021%
15	11.061	1281	1289	1297	rBV	122050	218857	23.17%	2.492%
16	11.190	1304	1311	1325	rBV	128477	244602	25.89%	2.785%
17	12.647	1554	1559	1565	rVB	1636	2855	0.30%	0.033%
18	14.257	1827	1833	1841	rBV	279756	416108	44.05%	4.739%
19	14.562	1878	1885	1895	rBV	309384	498012	52.72%	5.671%
20	14.868	1930	1937	1948	rVB	218295	339803	35.97%	3.870%
21	15.056	1963	1969	1982	rBV	91202	177612	18.80%	2.023%
22	15.144	1982	1984	1988	rVV2	2853	4202	0.44%	0.048%
23	15.860	2099	2106	2116	rBV	402255	626586	66.33%	7.135%
24	15.972	2119	2125	2138	rVB	101545	164522	17.42%	1.874%
25	16.095	2143	2146	2151	rVB2	1585	1872	0.20%	0.021%
26	17.405	2363	2369	2374	rBV3	1146	2173	0.23%	0.025%
27	17.617	2399	2405	2414	rBV	310109	457269	48.40%	5.207%
28	17.717	2415	2422	2435	rVB2	489748	737772	78.10%	8.402%
29	19.561	2731	2736	2742	rBV3	6940	9738	1.03%	0.111%
30	19.632	2744	2748	2756	rVB2	6132	8166	0.86%	0.093%
31	19.996	2803	2810	2820	rVV	673391	944679	100.00%	10.758%
32	20.319	2863	2865	2868	rBV5	1157	1559	0.17%	0.018%
33	20.366	2871	2873	2876	rVV3	1191	1483	0.16%	0.017%
34	20.419	2879	2882	2887	rBV3	1957	2957	0.31%	0.034%
35	20.478	2887	2892	2894	rBV5	1796	2298	0.24%	0.026%
36	20.660	2920	2923	2927	rBV4	1083	1752	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
 Data File : BG052425.D
 Acq On : 18 Feb 2022 16:53
 Operator : CG/JU
 Sample : PB142721BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	21.283	3028	3029	3032	rBV3	2299	2406	0.25%	0.027%
38	21.335	3036	3038	3039	rVB2	2176	1403	0.15%	0.016%
39	21.535	3070	3072	3074	rVB2	2147	1641	0.17%	0.019%
40	21.653	3090	3092	3095	rBV3	1316	1537	0.16%	0.018%
41	21.935	3133	3140	3148	rBV	315078	534053	56.53%	6.082%
42	22.105	3167	3169	3173	rBV2	1684	1884	0.20%	0.021%
43	22.316	3203	3205	3208	rBV4	1774	1627	0.17%	0.019%
44	22.340	3208	3209	3214	rBV4	1497	1577	0.17%	0.018%
45	22.469	3230	3231	3234	rBV3	2421	2645	0.28%	0.030%
46	22.769	3278	3282	3285	rBV4	2743	3983	0.42%	0.045%
47	22.963	3313	3315	3318	rBV4	1856	2019	0.21%	0.023%
48	23.115	3340	3341	3345	rBV4	1288	1654	0.18%	0.019%
49	23.309	3372	3374	3376	rVB3	2256	1729	0.18%	0.020%
50	23.509	3401	3408	3414	rVB7	7527	15553	1.65%	0.177%
51	23.568	3414	3418	3420	rBV4	2417	2353	0.25%	0.027%
52	23.715	3441	3443	3447	rBV4	1850	2717	0.29%	0.031%
53	23.762	3449	3451	3452	rVV2	1908	1334	0.14%	0.015%
54	23.779	3452	3454	3457	rVB2	1526	1909	0.20%	0.022%
55	23.985	3487	3489	3492	rVB4	2124	1376	0.15%	0.016%
56	24.384	3550	3557	3560	rBV4	11118	19665	2.08%	0.224%
57	24.513	3575	3579	3582	rVV5	1519	2098	0.22%	0.024%
58	24.731	3614	3616	3619	rBV4	1402	1520	0.16%	0.017%
59	24.972	3655	3657	3658	rBV2	1905	1360	0.14%	0.015%
60	25.166	3677	3690	3702	rBV2	305096	899061	95.17%	10.238%
61	25.406	3719	3731	3744	rVB2	179454	561637	59.45%	6.396%
62	25.530	3750	3752	3754	rBV3	2131	2240	0.24%	0.026%
63	26.658	3932	3944	3949	rBV7	12075	37799	4.00%	0.430%
64	26.816	3969	3971	3975	rVB4	1980	2618	0.28%	0.030%
65	26.846	3975	3976	3980	rBV4	2171	2887	0.31%	0.033%
66	26.981	3997	3999	4003	rVB3	2858	3352	0.35%	0.038%
67	27.016	4003	4005	4006	rBV2	2100	1547	0.16%	0.018%
68	27.104	4017	4020	4022	rVB4	1508	1609	0.17%	0.018%
69	27.163	4027	4030	4032	rBV3	1675	2013	0.21%	0.023%
70	27.457	4078	4080	4083	rVB4	1481	1486	0.16%	0.017%
71	27.480	4083	4084	4087	rBV3	1328	1564	0.17%	0.018%
72	27.574	4097	4100	4101	rVB3	1827	1570	0.17%	0.018%
73	27.844	4144	4146	4150	rVB5	2111	2661	0.28%	0.030%
74	27.979	4167	4169	4172	rVB3	1485	1409	0.15%	0.016%
75	28.015	4172	4175	4176	rBV3	1907	1652	0.17%	0.019%
76	28.032	4176	4178	4180	rBV3	2050	2000	0.21%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
 Data File : BG052425.D
 Acq On : 18 Feb 2022 16:53
 Operator : CG/JU
 Sample : PB142721BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	28.056	4180	4182	4184	rBV3	1787	1363	0.14%	0.016%
78	28.138	4187	4196	4205	rBV8	12523	41195	4.36%	0.469%
79	28.355	4231	4233	4234	rVB2	2882	1467	0.16%	0.017%
80	28.367	4234	4235	4237	rBV	1839	1479	0.16%	0.017%
81	29.013	4343	4345	4350	rBV6	1331	1983	0.21%	0.023%
82	29.871	4489	4491	4492	rBV2	2865	2306	0.24%	0.026%
83	29.918	4495	4499	4500	rBV5	4636	5634	0.60%	0.064%
84	30.171	4540	4542	4545	rVB4	1857	1499	0.16%	0.017%
85	30.200	4545	4547	4550	rBV4	1993	1437	0.15%	0.016%
86	30.388	4577	4579	4581	rVB3	1988	1431	0.15%	0.016%
87	30.447	4586	4589	4590	rBV	1630	1650	0.17%	0.019%
88	30.535	4601	4604	4607	rBV4	1693	3117	0.33%	0.035%
89	30.582	4610	4612	4615	rVB2	2515	2238	0.24%	0.025%
90	30.629	4618	4620	4623	rVB4	1551	1448	0.15%	0.016%
91	30.658	4623	4625	4627	rBV3	1691	1760	0.19%	0.020%
92	30.740	4638	4639	4642	rVB2	2189	1859	0.20%	0.021%
93	30.917	4668	4669	4674	rBV4	2263	3118	0.33%	0.036%
94	30.975	4676	4679	4680	rBV2	2148	1940	0.21%	0.022%
95	31.046	4689	4691	4696	rBV5	2093	3127	0.33%	0.036%
96	31.281	4729	4731	4733	rVB3	2782	1932	0.20%	0.022%
97	31.633	4790	4791	4793	rBV2	2270	1504	0.16%	0.017%
98	32.080	4862	4867	4868	rBV4	5456	7745	0.82%	0.088%
99	32.291	4900	4903	4905	rBV3	2415	2165	0.23%	0.025%
100	32.420	4922	4925	4929	rBV6	1873	2280	0.24%	0.026%


Sum of corrected areas: 8781301

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
Data File : BG052425.D
Acq On : 18 Feb 2022 16:53
Operator : CG/JU
Sample : PB142721BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

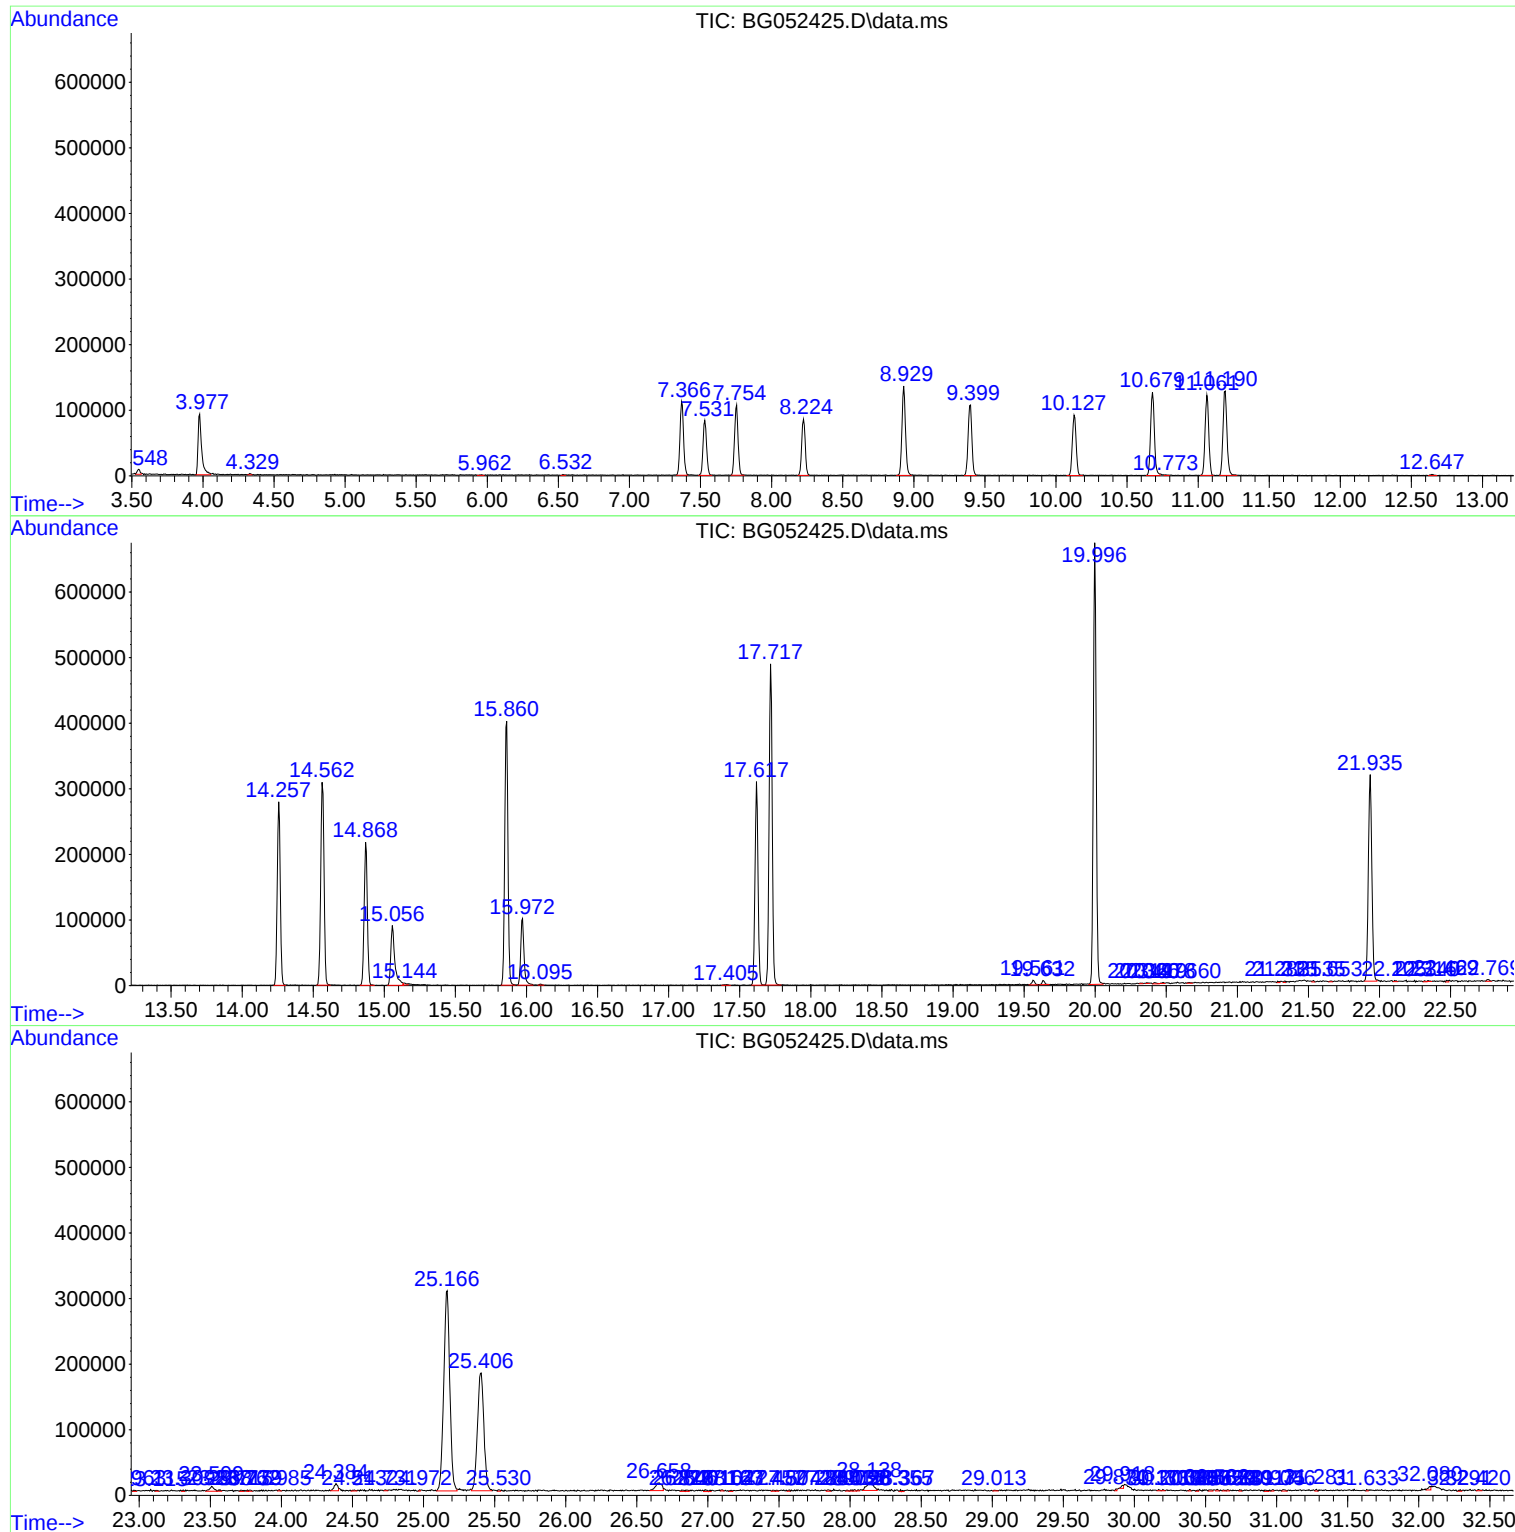

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
Data File : BG052425.D
Acq On : 18 Feb 2022 16:53
Operator : CG/JU
Sample : PB142721BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021822\
Data File : BG052425.D
Acq On : 18 Feb 2022 16:53
Operator : CG/JU
Sample : PB142721BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc