


Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG021915\  
Data File : BG016001.D  
Acq On : 19 Feb 2015 13:42  
Operator : TP/IZ  
Sample : DFTPP05  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM01.2-EPA-MA-BG021915.M  
Title : SVOA CALIBRATION  
Last Update : Fri Feb 20 05:38:39 2015

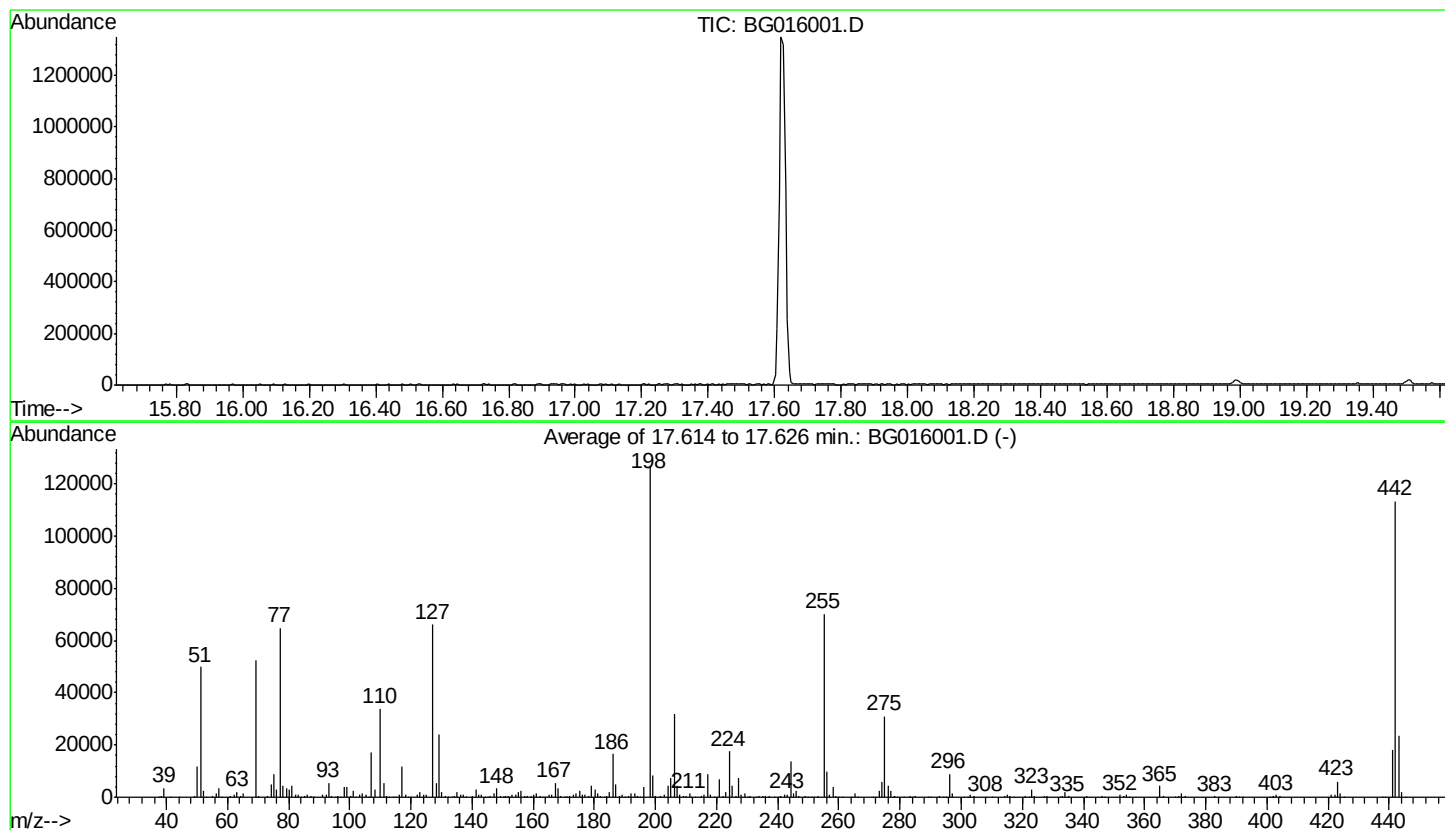

AutoFind: Scans 2541, 2542, 2543; Background Corrected with Scan 2536

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 39.3      | 49848   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 41.3      | 52386   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 329     | PASS             |
| 127         | 198          | 10           | 80           | 52.0      | 66024   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 126893  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 8372    | PASS             |
| 275         | 198          | 10           | 60           | 24.5      | 31093   | PASS             |
| 365         | 198          | 1            | 100          | 3.4       | 4306    | PASS             |
| 441         | 443          | 0.01         | 100          | 76.7      | 17998   | PASS             |
| 442         | 198          | 50           | 100          | 89.3      | 113378  | PASS             |
| 443         | 442          | 15           | 24           | 20.7      | 23477   | PASS             |