

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021915\
 Data File : BG016008.D
 Acq On : 19 Feb 2015 18:49
 Operator : TP/IZ
 Sample : MDL-01-W
 Misc : MDL-WATER-3PPM-SOM0
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Feb 20 06:23:31 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-MA-BG021915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 20 05:38:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	98460	20.00	ng/ul	0.00
16) Naphthalene-d8	10.60	136	442758	20.00	ng/ul	0.00
33) Acenaphthene-d10	14.44	164	269347	20.00	ng/ul	0.00
59) Phenanthrene-d10	17.18	188	574028	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	586598	20.00	ng/ul	0.00
83) Perylene-d12	23.65	264	582911	20.00	ng/ul	0.00


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) Phenol-d5	6.98	99	309842	33.08	ng/ul	0.00
5) Bis-(2-Chloroethyl)ether-d	7.15	67	192948	34.87	ng/ul	0.00
7) 2-Chlorophenol-d4	7.35	132	236851	34.18	ng/ul	0.00
11) 4-Methylphenol-d8	8.51	113	233537	33.69	ng/ul	0.00
17) Nitrobenzene-d5	8.97	128	118214	37.78	ng/ul	0.00
20) 2-Nitrophenol-d4	9.68	143	109426	37.91	ng/ul	0.00
24) 2,4-Dichlorophenol-d3	10.22	165	205486	32.82	ng/ul	0.00
27) 4-Chloroaniline-d4	10.73	131	365152	52.94	ng/ul	0.00
41) Dimethylphthalate-d6	13.85	166	671821	37.31	ng/ul	0.00
44) Acenaphthylene-d8	14.13	160	872310	34.23	ng/ul	0.00
49) 4-Nitrophenol-d4	14.62	143	112555	31.08	ng/ul	0.00
55) Fluorene-d10	15.43	176	632403	34.94	ng/ul	0.00
60) 4,6-Dinitro-2-methylphenol	15.54	200	46993	21.23	ng/ul	0.00
68) Anthracene-d10	17.28	188	951215	34.94	ng/ul	0.00
76) Pyrene-d10	19.57	212	1000406	36.31	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	945560	35.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
70) 1,2,3,4-Tetrachlorobenzene	13.24	216	14403	1.97	ng/uL	95
71) Pentachlorobenzene	14.75	250	30053	4.20	ng/uL	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021915\
Data File : BG016008.D
Acq On : 19 Feb 2015 18:49
Operator : TP/IZ
Sample : MDL-01-W
Misc : MDL-WATER-3PPM-SOM0
ALS Vial : 8 Sample Multiplier: 1


Quant Time: Feb 20 06:23:31 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-MA-BG021915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 20 05:38:39 2015
Response via : Initial Calibration

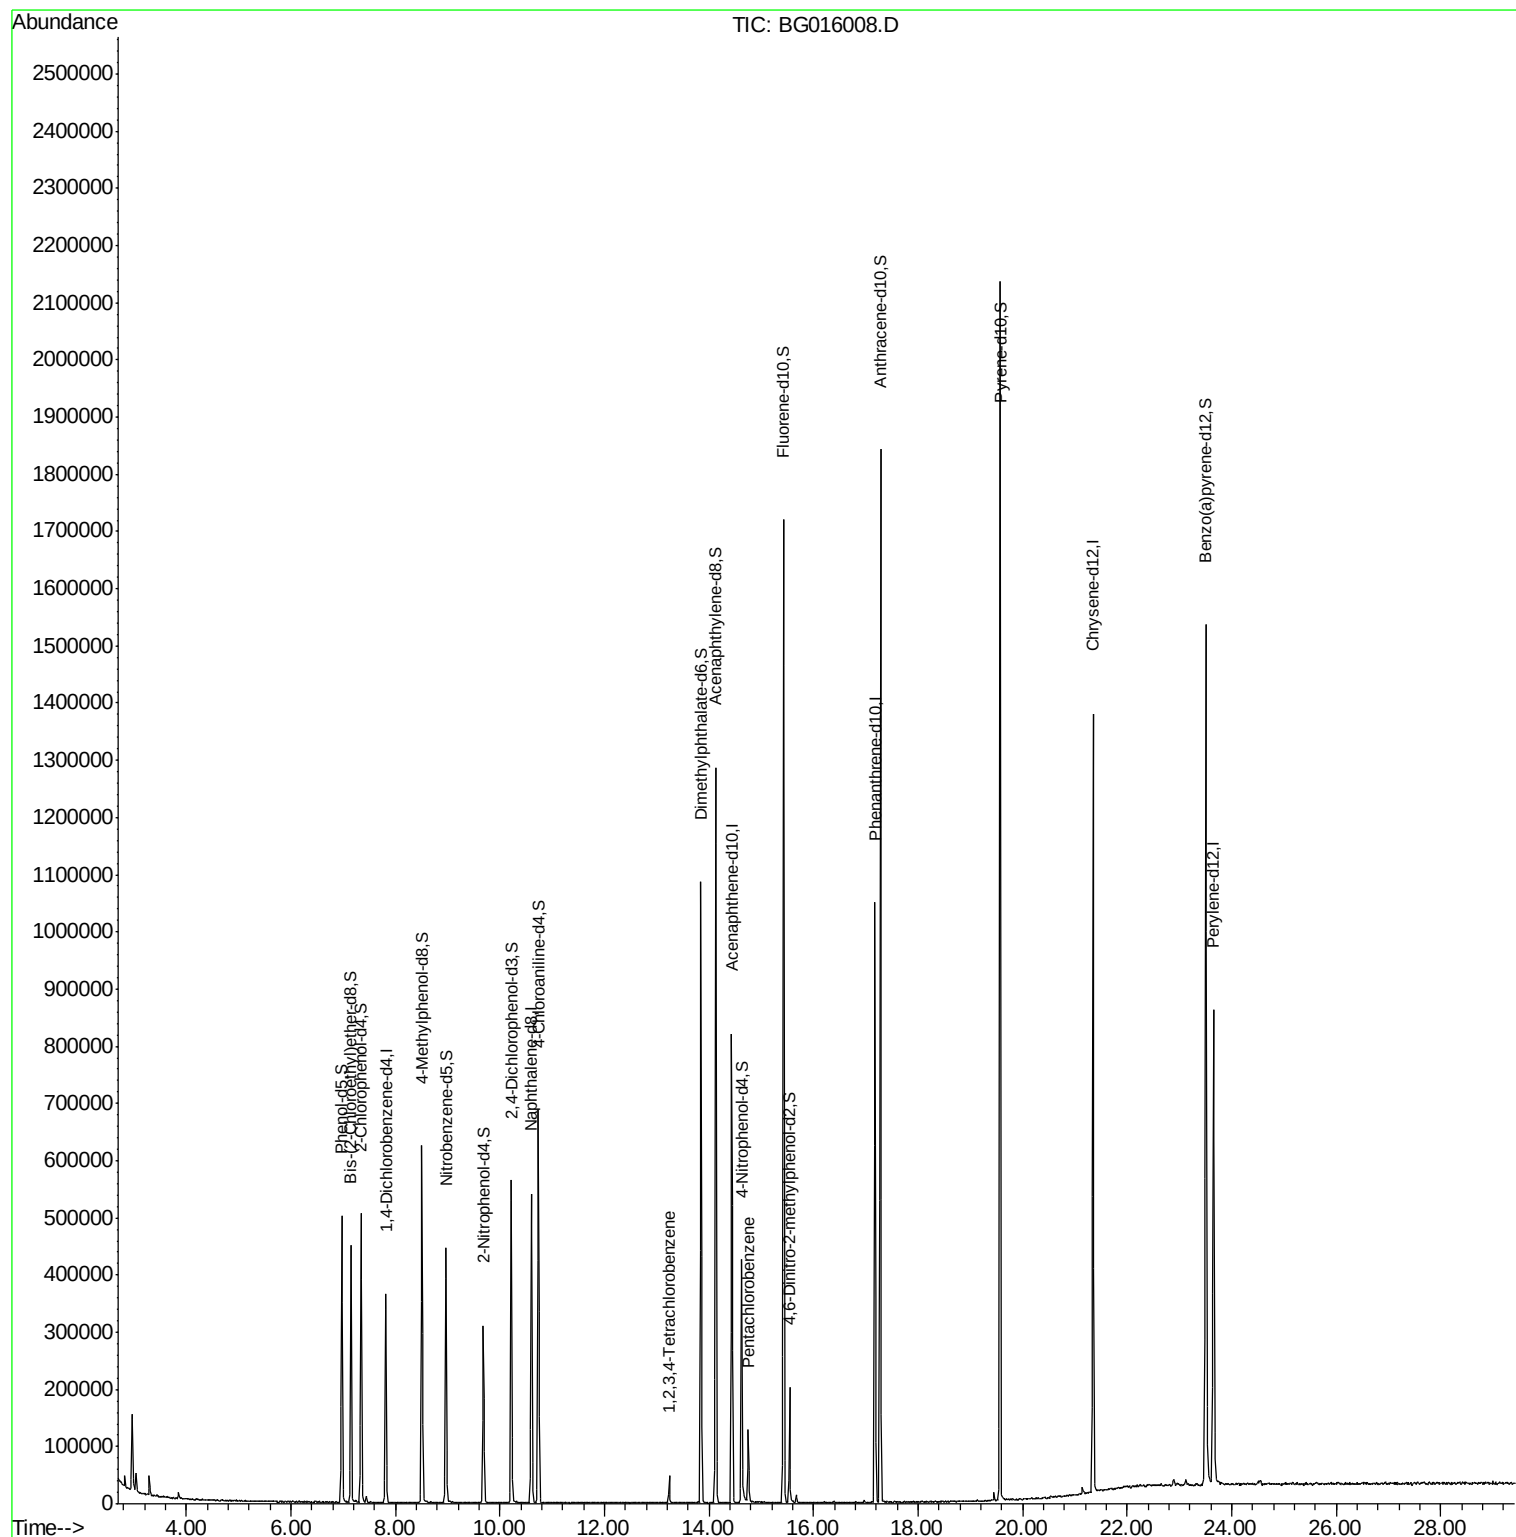



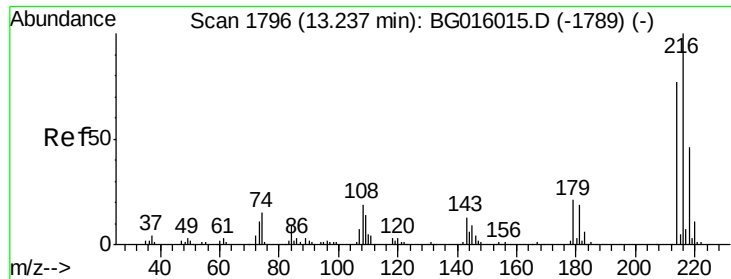


#70
 1,2,3,4-Tetrachlorobenzene
 Concen: 1.97 ng/uL
 RT: 13.24 min Scan# 1796
 Delta R.T. -0.00 min
 Lab File: BG016008.D
 Acq: 19 Feb 2015 18:49

Tgt Ion	Ratio	Lower	Upper
216	100		
214	83.1	64.5	96.7
218	52.4	37.9	56.9

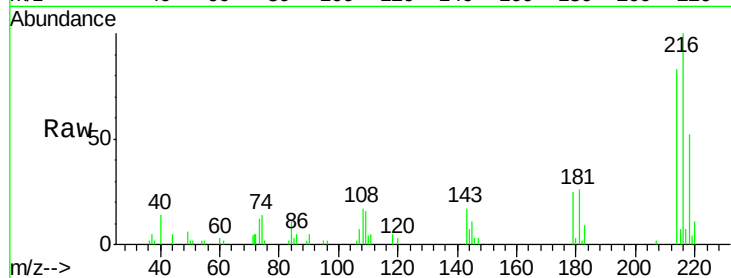


Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 218.00 (217.70 to 218.70): E

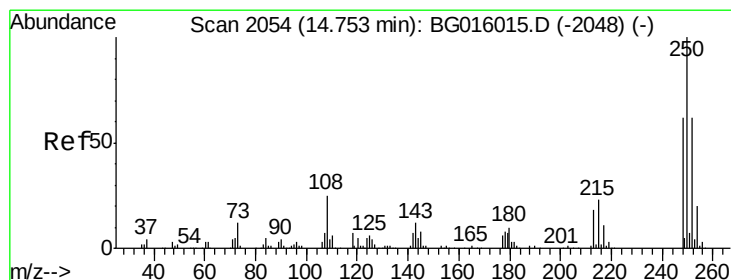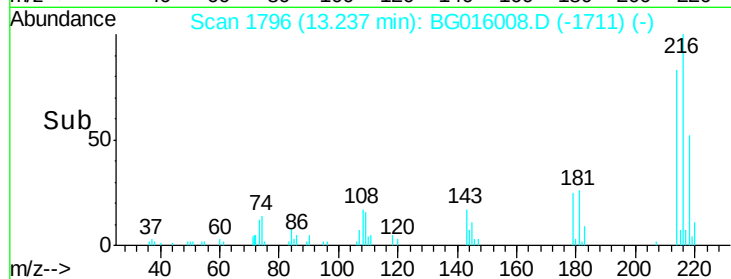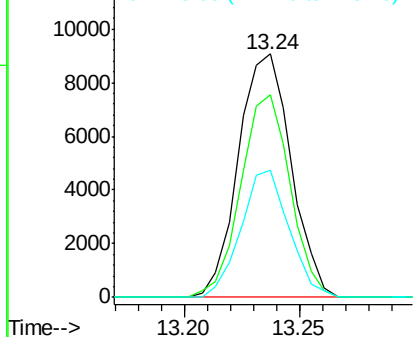

#71
 Pentachlorobenzene
 Concen: 4.20 ng/uL
 RT: 14.75 min Scan# 2054
 Delta R.T. -0.00 min
 Lab File: BG016008.D
 Acq: 19 Feb 2015 18:49

Tgt Ion	Ratio	Lower	Upper
250	100		
248	64.4	50.5	75.7
252	58.6	50.7	76.1

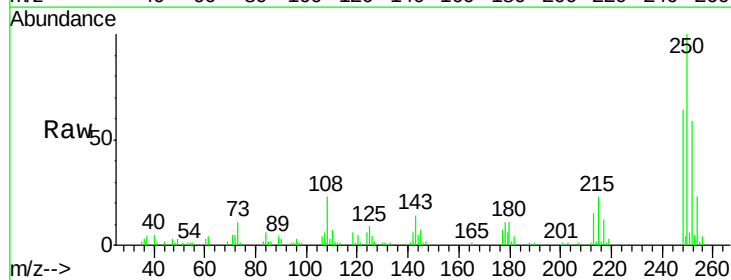

Abundance Ion 250.00 (249.70 to 250.70): E
 Ion 248.00 (247.70 to 248.70): E
 Ion 252.00 (251.70 to 252.70): E

