

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021915\
 Data File : BG016013.D
 Acq On : 19 Feb 2015 21:41
 Operator : TP/IZ
 Sample : MDL-06-W
 Misc : MDL-WATER-3PPM-SOM0
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Feb 20 06:35:39 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-MA-BG021915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 20 05:38:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	93789	20.00	ng/ul	0.00
16) Naphthalene-d8	10.60	136	409698	20.00	ng/ul	0.00
33) Acenaphthene-d10	14.44	164	246727	20.00	ng/ul	0.00
59) Phenanthrene-d10	17.18	188	532643	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	571604	20.00	ng/ul	0.00
83) Perylene-d12	23.65	264	561694	20.00	ng/ul	0.00


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) Phenol-d5	6.97	99	286627	32.12	ng/ul	0.00
5) Bis-(2-Chloroethyl)ether-d	7.14	67	177644	33.71	ng/ul	0.00
7) 2-Chlorophenol-d4	7.34	132	222068	33.64	ng/ul	0.00
11) 4-Methylphenol-d8	8.51	113	216417	32.77	ng/ul	0.00
17) Nitrobenzene-d5	8.96	128	108818	37.58	ng/ul	0.00
20) 2-Nitrophenol-d4	9.69	143	98774	36.98	ng/ul	0.00
24) 2,4-Dichlorophenol-d3	10.22	165	184196	31.79	ng/ul	0.00
27) 4-Chloroaniline-d4	10.73	131	338245	52.99	ng/ul	0.00
41) Dimethylphthalate-d6	13.85	166	620362	37.61	ng/ul	0.00
44) Acenaphthylene-d8	14.13	160	801209	34.32	ng/ul	0.00
49) 4-Nitrophenol-d4	14.62	143	101031	30.46	ng/ul	0.00
55) Fluorene-d10	15.43	176	587607	35.44	ng/ul	0.00
60) 4,6-Dinitro-2-methylphenol	15.54	200	40403	19.67	ng/ul	0.00
68) Anthracene-d10	17.28	188	900337	35.64	ng/ul	0.00
76) Pyrene-d10	19.57	212	976413	36.37	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	923339	36.25	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
70) 1,2,3,4-Tetrachlorobenzene	13.23	216	15011	2.22	ng/uL	94
71) Pentachlorobenzene	14.75	250	30718	4.63	ng/uL	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021915\
Data File : BG016013.D
Acq On : 19 Feb 2015 21:41
Operator : TP/IZ
Sample : MDL-06-W
Misc : MDL-WATER-3PPM-SOM0
ALS Vial : 13 Sample Multiplier: 1


Quant Time: Feb 20 06:35:39 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-MA-BG021915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 20 05:38:39 2015
Response via : Initial Calibration

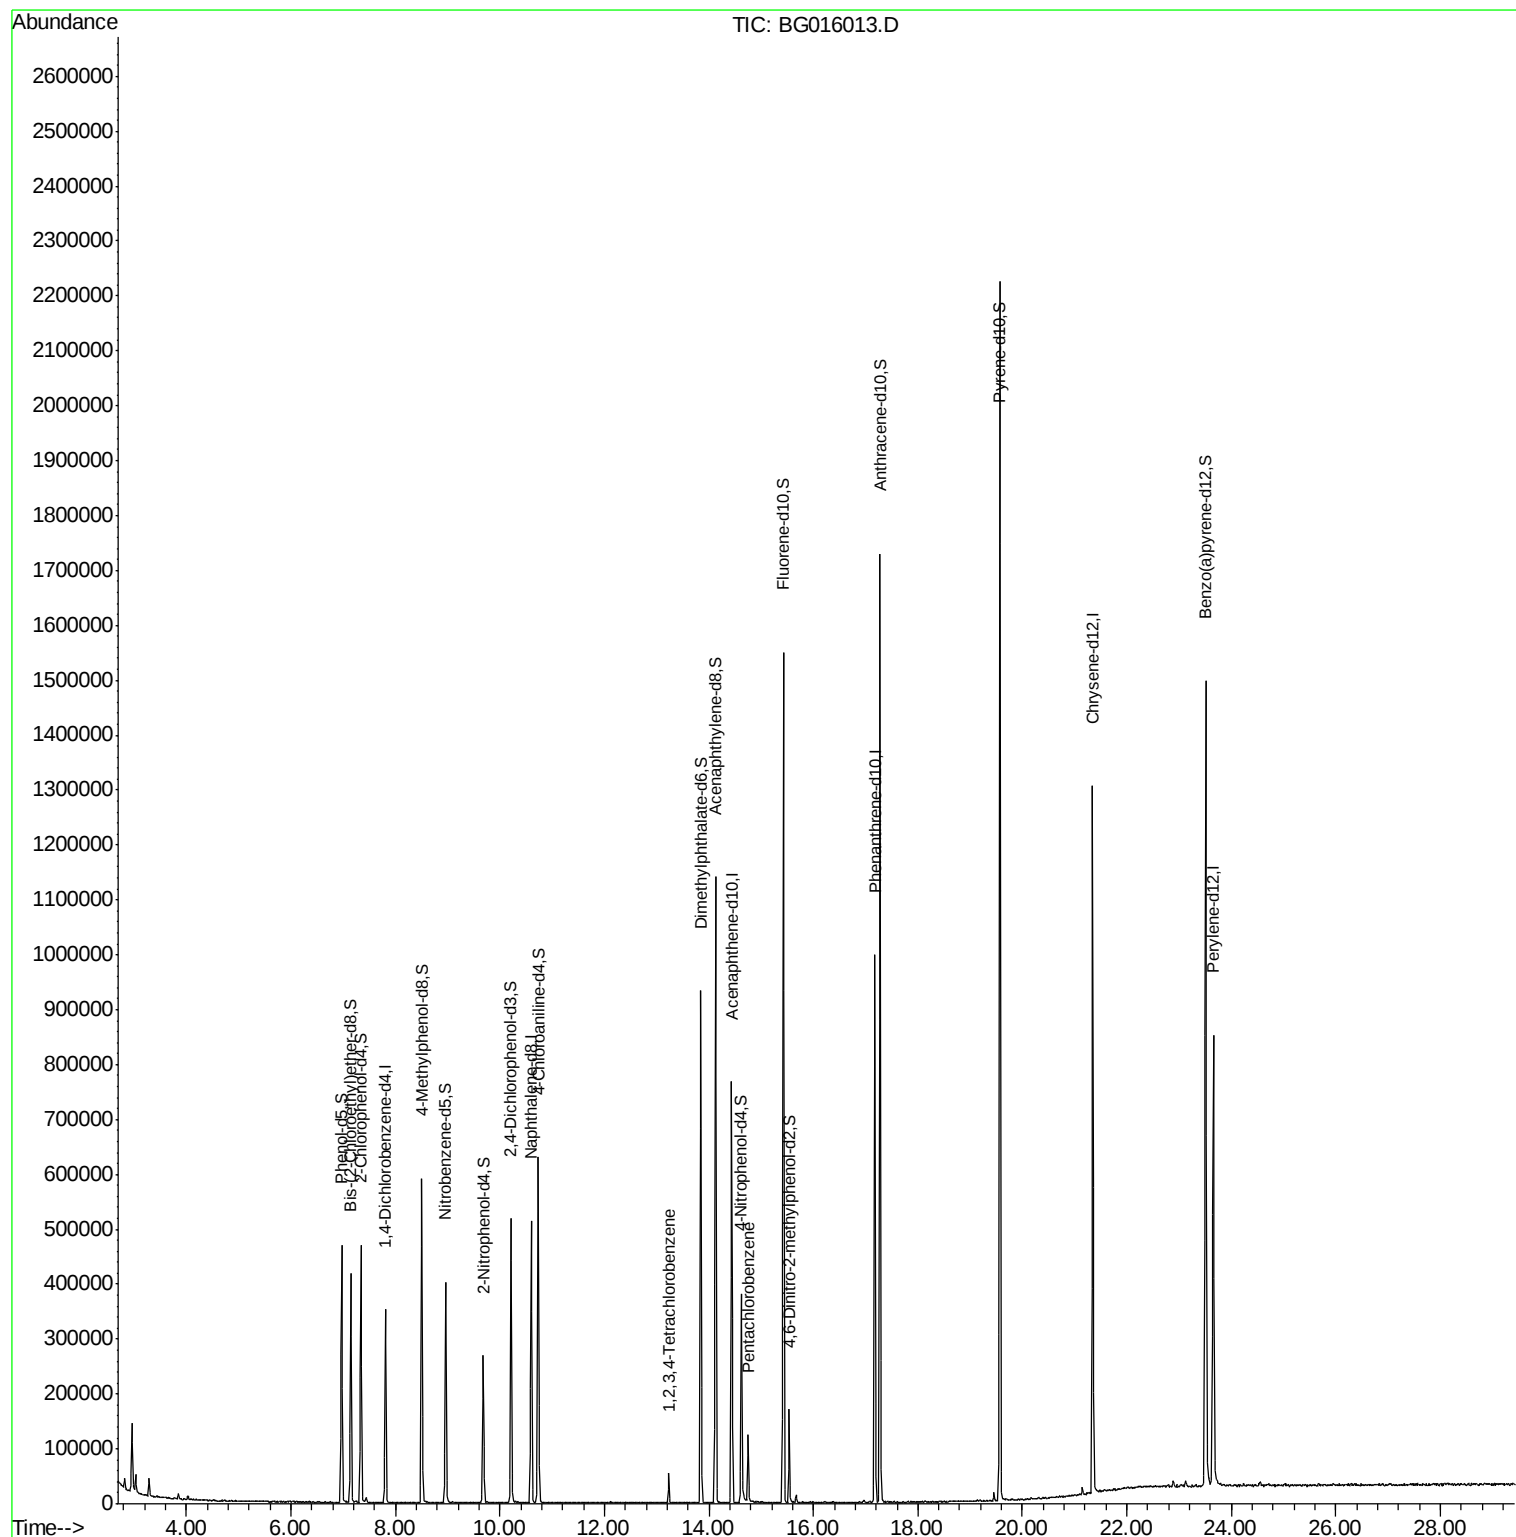



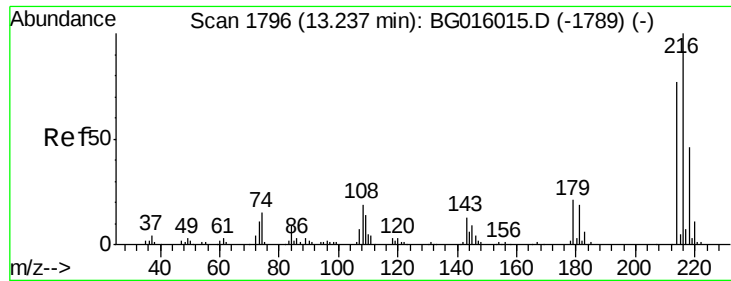


#70
 1,2,3,4-Tetrachlorobenzene
 Concen: 2.22 ng/uL
 RT: 13.23 min Scan# 1795
 Delta R.T. -0.00 min
 Lab File: BG016013.D
 Acq: 19 Feb 2015 21:41

Tgt Ion	Ratio	Lower	Upper
216	100		
214	73.7	64.5	96.7
218	49.0	37.9	56.9

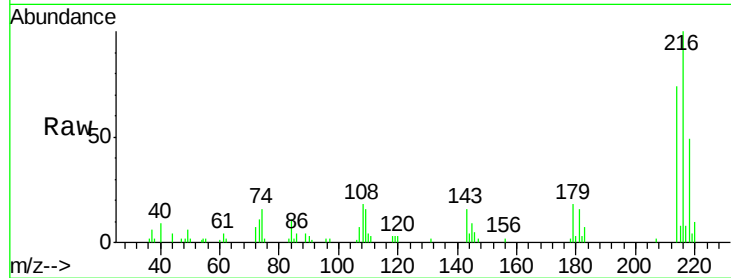


Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 218.00 (217.70 to 218.70): E

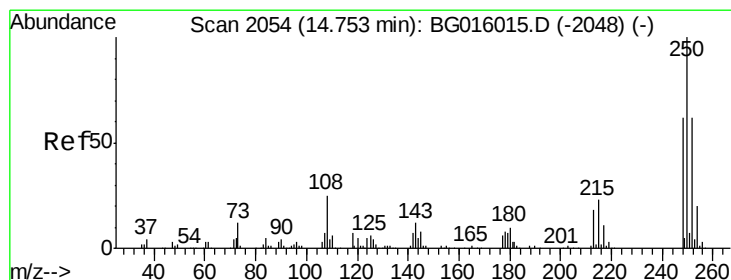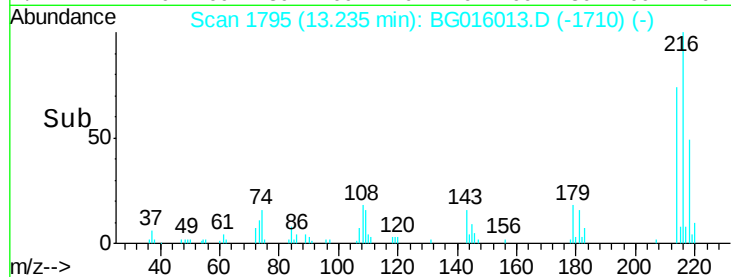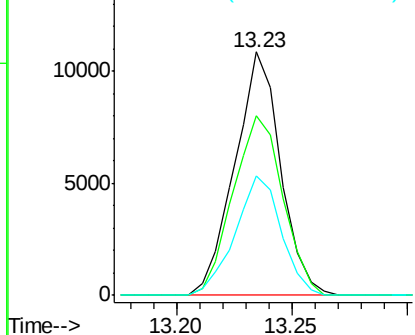

#71
 Pentachlorobenzene
 Concen: 4.63 ng/uL
 RT: 14.75 min Scan# 2053
 Delta R.T. -0.00 min
 Lab File: BG016013.D
 Acq: 19 Feb 2015 21:41

Tgt Ion	Ratio	Lower	Upper
250	100		
248	54.4	50.5	75.7
252	56.7	50.7	76.1

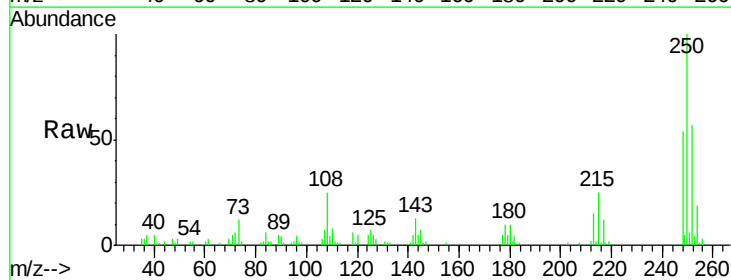

Abundance Ion 250.00 (249.70 to 250.70): E
 Ion 248.00 (247.70 to 248.70): E
 Ion 252.00 (251.70 to 252.70): E

