

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021915\
 Data File : BG016028.D
 Acq On : 20 Feb 2015 10:24
 Operator : TP/IZ
 Sample : MDL-03-S-ML
 Misc : MDL-SOIL-3PPM-SOM0-ML
 ALS Vial : 31 Sample Multiplier: 1

Quant Time: Feb 20 12:21:35 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-MA-BG021915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 20 05:38:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	87206	20.00	ng/ul	0.00
16) Naphthalene-d8	10.60	136	399895	20.00	ng/ul	0.00
33) Acenaphthene-d10	14.43	164	246074	20.00	ng/ul	0.00
59) Phenanthrene-d10	17.18	188	531795	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	550518	20.00	ng/ul	0.00
83) Perylene-d12	23.65	264	527136	20.00	ng/ul	0.00

System Monitoring Compounds

3) Phenol-d5	6.97	99	277730	33.48	ng/ul	0.00
5) Bis-(2-Chloroethyl)ether-d	7.14	67	169200	34.53	ng/ul	0.00
7) 2-Chlorophenol-d4	7.34	132	217273	35.40	ng/ul	0.00
11) 4-Methylphenol-d8	8.50	113	212217	34.56	ng/ul	0.00
17) Nitrobenzene-d5	8.96	128	108184	38.28	ng/ul	0.00
20) 2-Nitrophenol-d4	9.68	143	97763	37.50	ng/ul	0.00
24) 2,4-Dichlorophenol-d3	10.21	165	181293	32.06	ng/ul	0.00
27) 4-Chloroaniline-d4	10.73	131	339006	54.41	ng/ul	0.00
41) Dimethylphthalate-d6	13.84	166	620977	37.74	ng/ul	0.00
44) Acenaphthylene-d8	14.13	160	812400	34.89	ng/ul	0.00
49) 4-Nitrophenol-d4	14.62	143	96511	29.17	ng/ul	0.00
55) Fluorene-d10	15.42	176	587392	35.52	ng/ul	0.00
60) 4,6-Dinitro-2-methylphenol	15.54	200	43014	20.98	ng/ul	0.00
68) Anthracene-d10	17.27	188	897045	35.56	ng/ul	0.00
76) Pyrene-d10	19.56	212	955141	36.94	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	877683	36.72	ng/ul	0.00


Target Compounds


						Qvalue
70) 1,2,3,4-Tetrachlorobenzene	13.23	216	15768	2.33	ng/uL	96
71) Pentachlorobenzene	14.75	250	32469	4.90	ng/uL	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG021915\
Data File : BG016028.D
Acq On : 20 Feb 2015 10:24
Operator : TP/IZ
Sample : MDL-03-S-ML
Misc : MDL-SOIL-3PPM-SOM0-ML
ALS Vial : 31 Sample Multiplier: 1


Quant Time: Feb 20 12:21:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-MA-BG021915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 20 05:38:39 2015
Response via : Initial Calibration

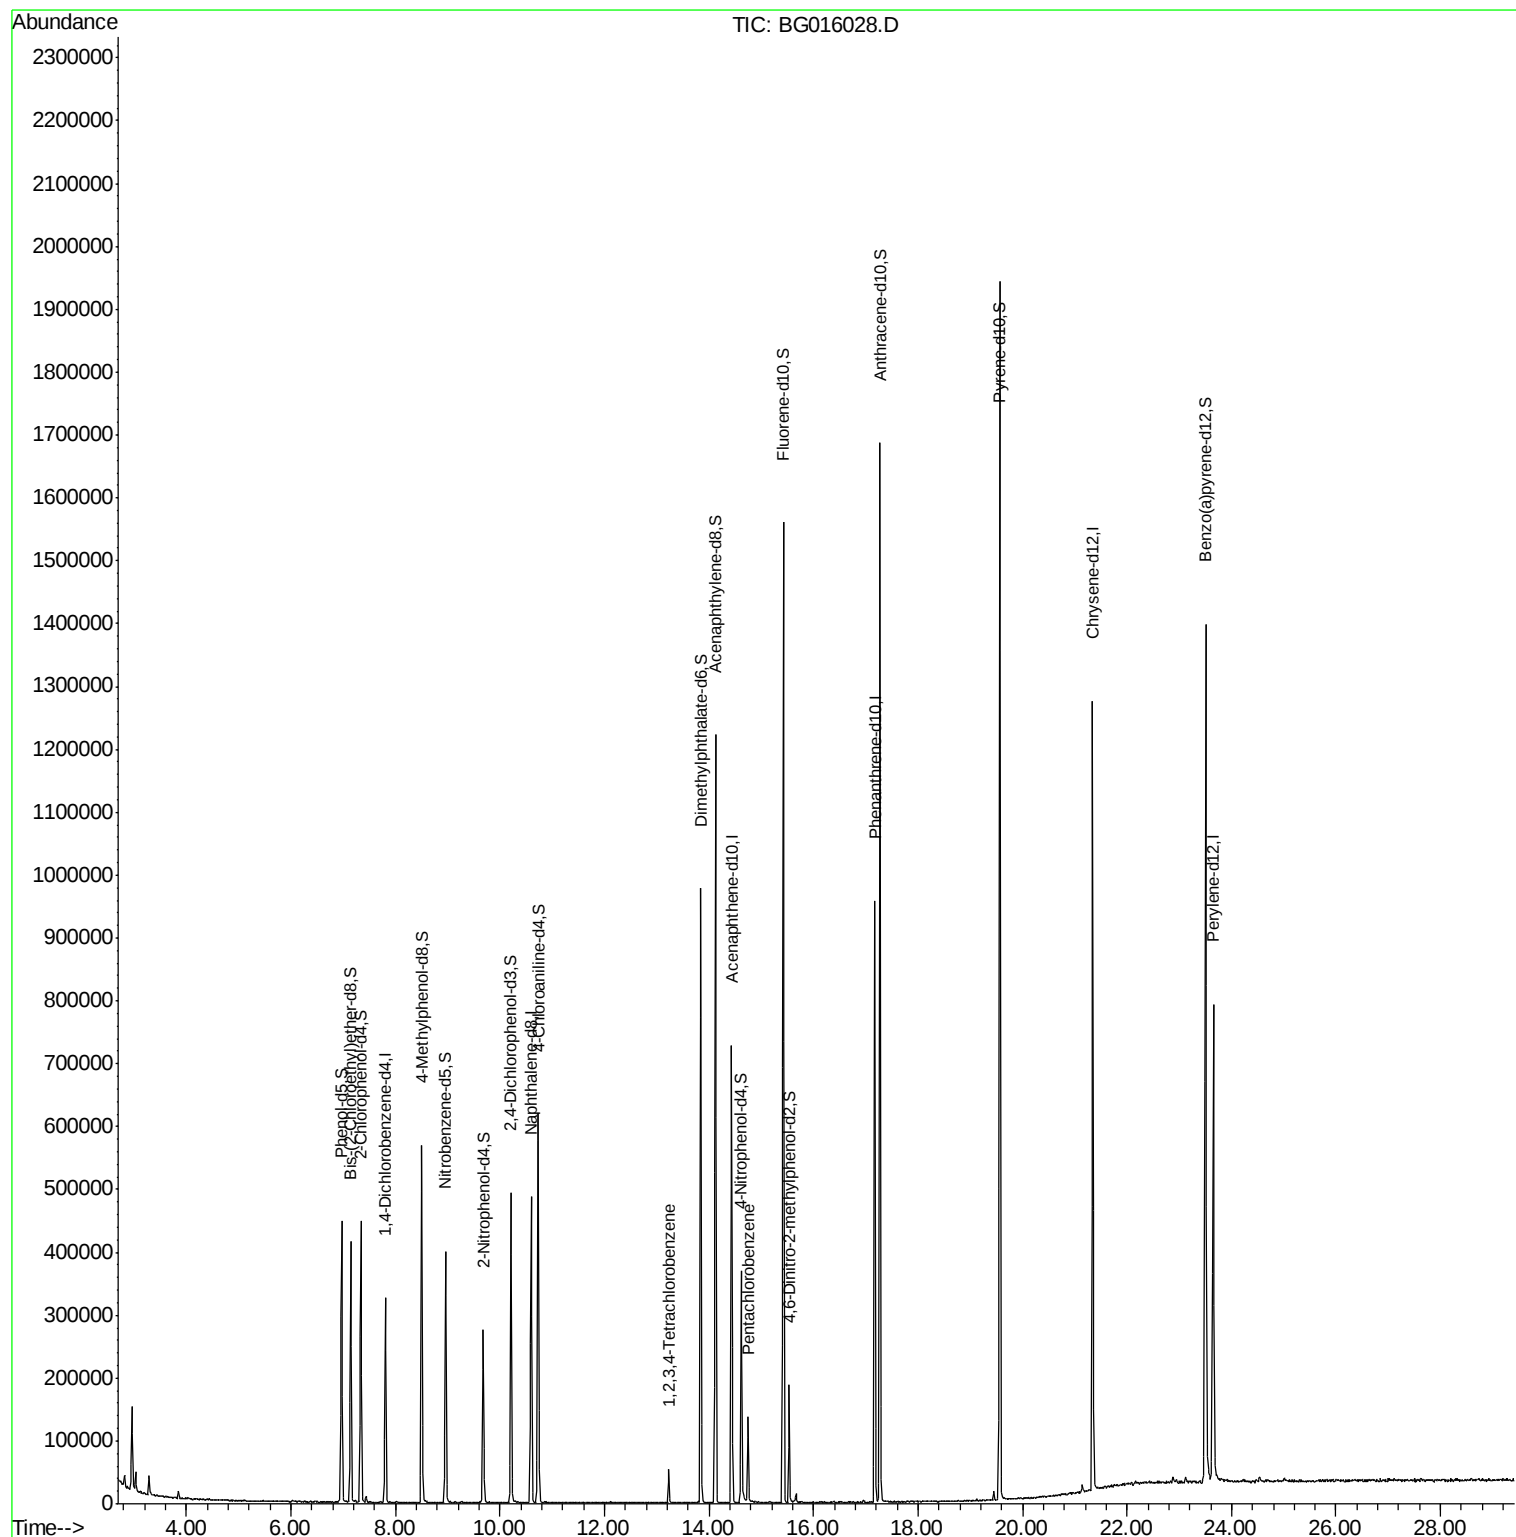



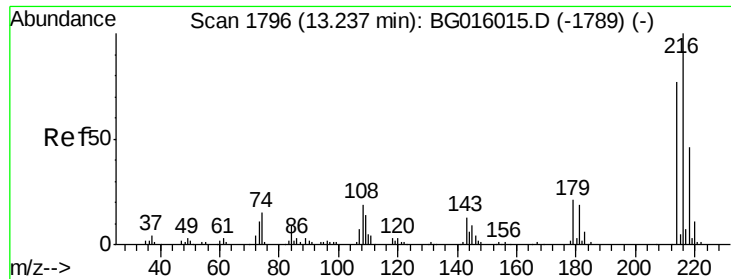


#70
 1,2,3,4-Tetrachlorobenzene
 Concen: 2.33 ng/uL
 RT: 13.23 min Scan# 1795
 Delta R.T. -0.00 min
 Lab File: BG016028.D
 Acq: 20 Feb 2015 10:24

Tgt Ion	Ratio	Lower	Upper
216	100		
214	75.8	64.5	96.7
218	45.8	37.9	56.9

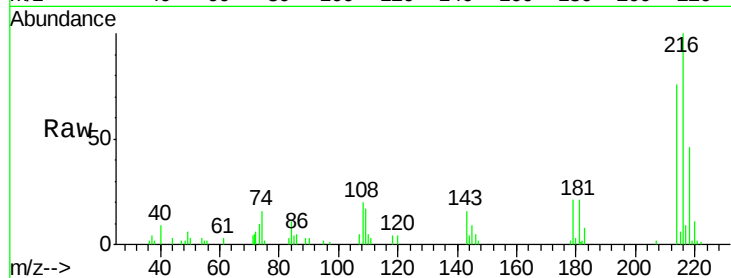


Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 218.00 (217.70 to 218.70): E

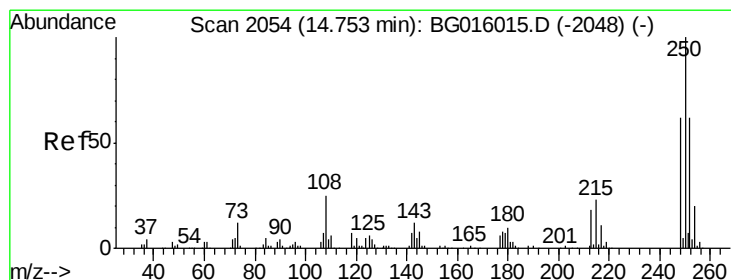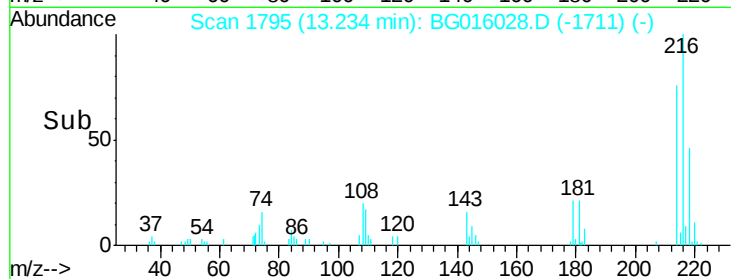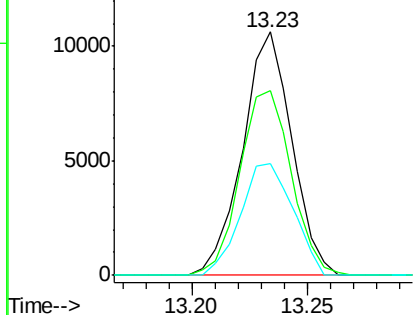

#71
 Pentachlorobenzene
 Concen: 4.90 ng/uL
 RT: 14.75 min Scan# 2053
 Delta R.T. -0.00 min
 Lab File: BG016028.D
 Acq: 20 Feb 2015 10:24

Tgt Ion	Ratio	Lower	Upper
250	100		
248	65.4	50.5	75.7
252	68.1	50.7	76.1

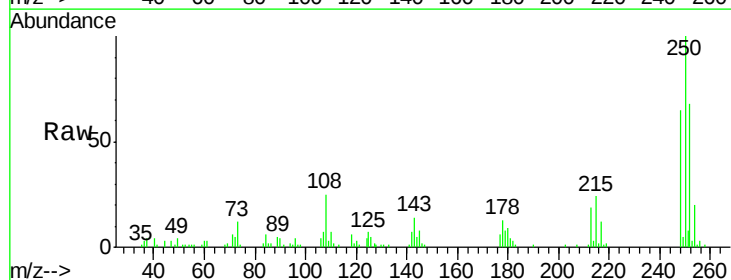

Abundance Ion 250.00 (249.70 to 250.70): E
 Ion 248.00 (247.70 to 248.70): E
 Ion 252.00 (251.70 to 252.70): E

