
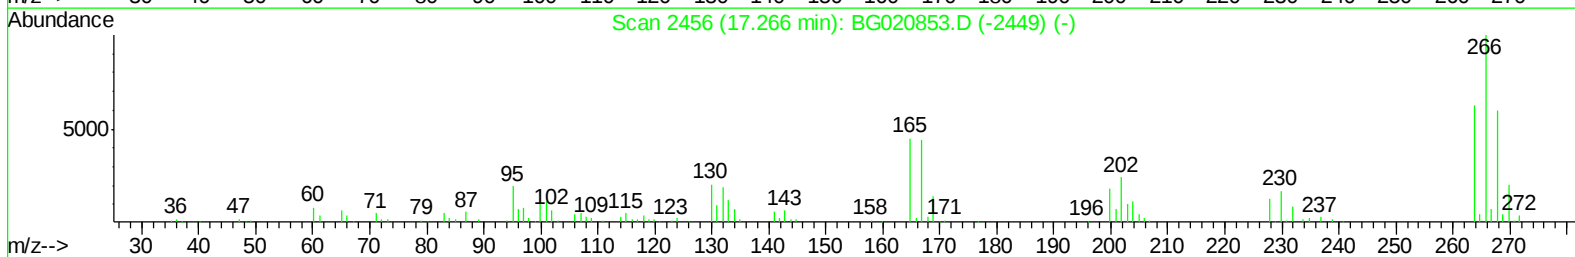
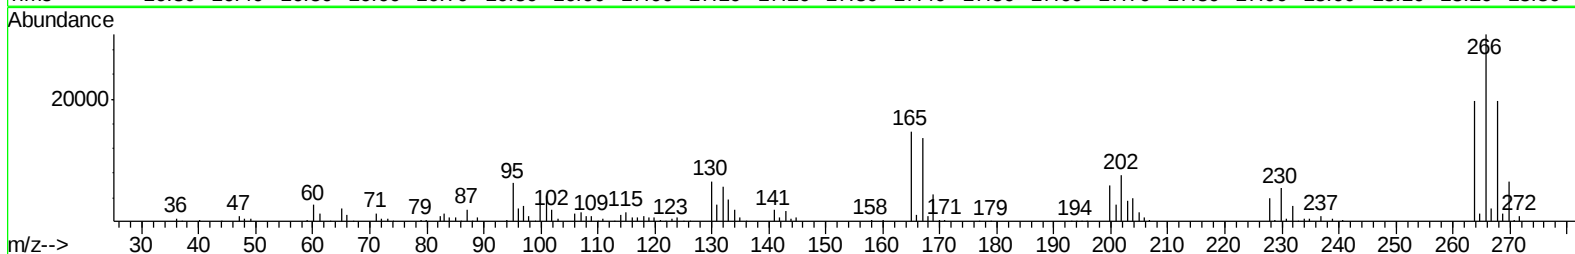


Data Path : Z:\HPCHEM1\BNA_G\Data\BG021916\
Data File : BG020968.D
Acq On : 19 Feb 2016 12:21
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:02:46 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

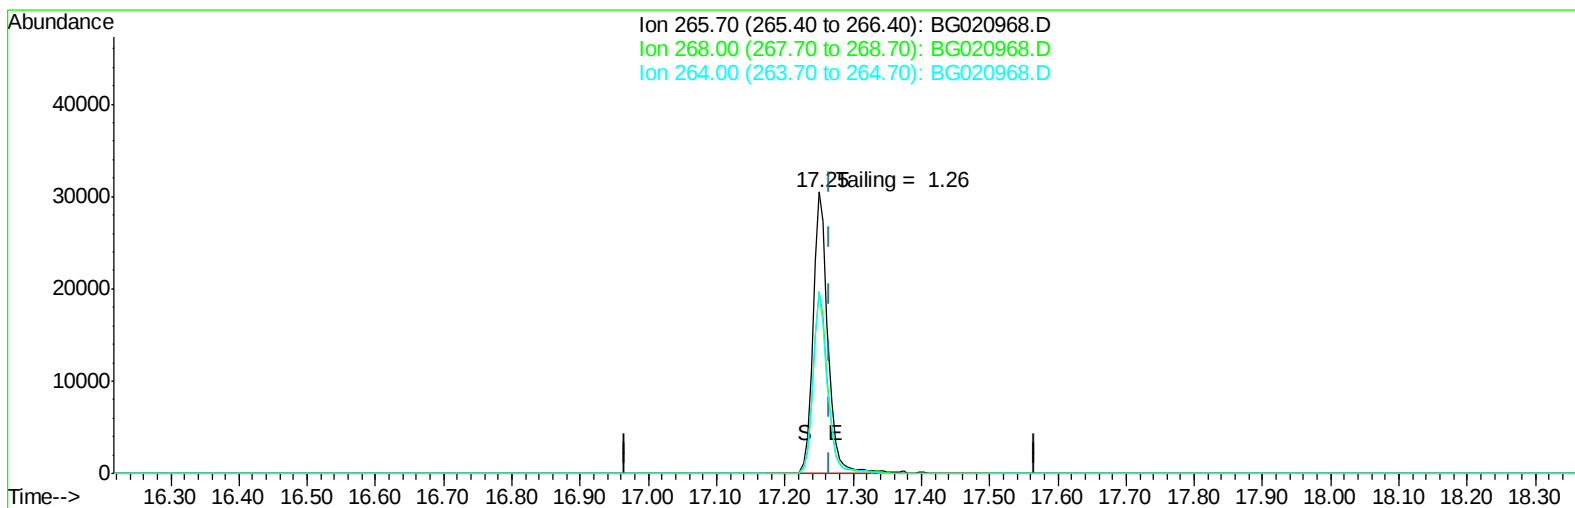

TIC: BG020968.D

(69) Pentachlorophenol (C)




17.250min (-0.016) 0.00ng

response 46120

Ion	Exp%	Act%
265.70	100	100
268.00	59.70	64.55
264.00	62.80	64.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG021916\
Data File : BG020968.D
Acq On : 19 Feb 2016 12:21
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:02:46 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

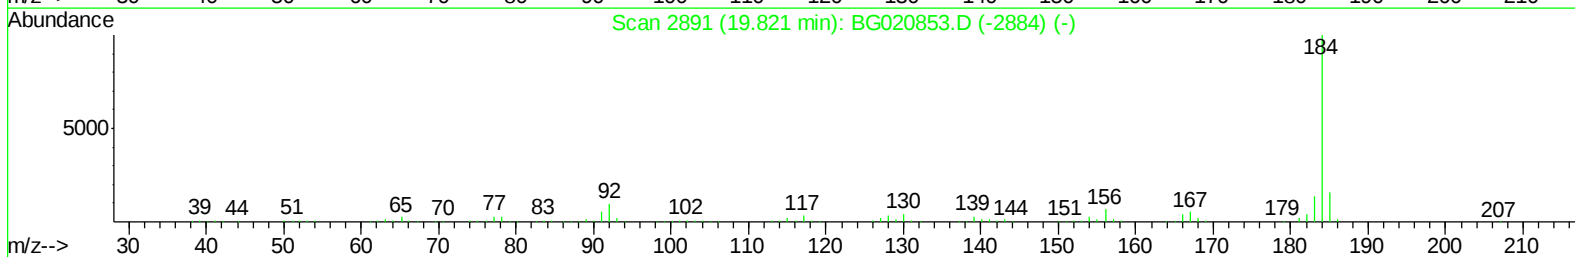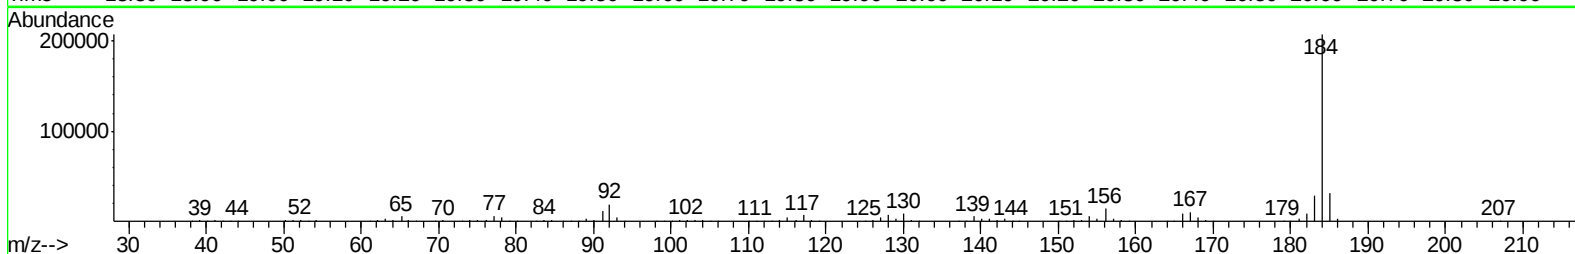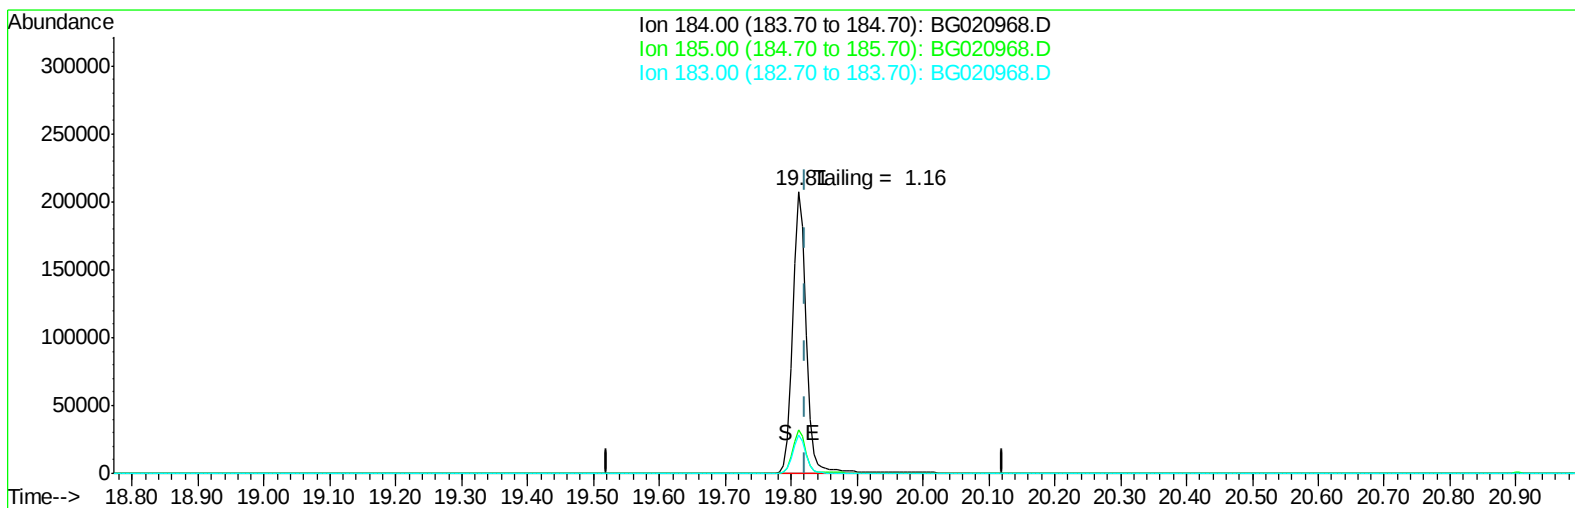

TIC: BG020968.D

(76) Benzidine

19.812min (-0.010) 78891.99ng

response 301033

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.38
183.00	13.70	13.55
0.00	0.00	0.00