
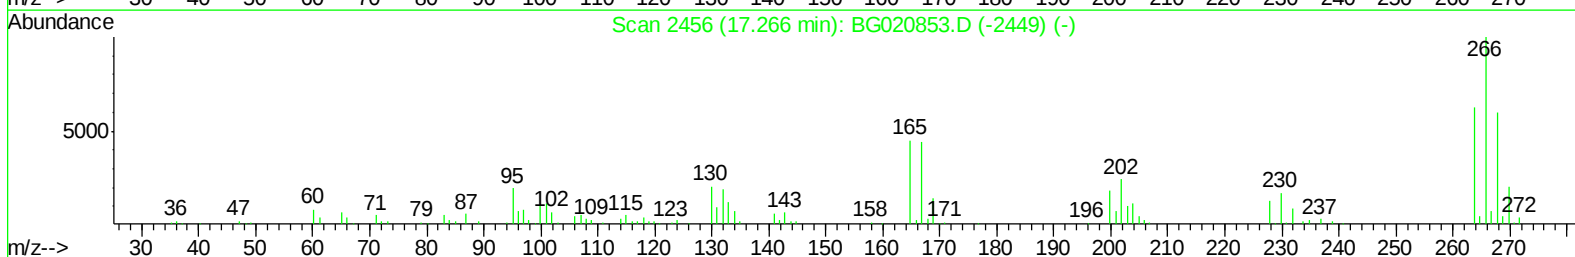
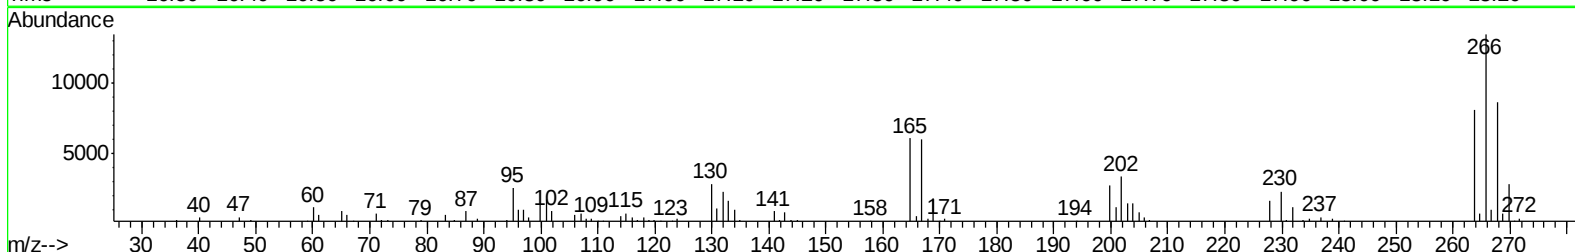


Data Path : Z:\HPCHEM1\BNA_G\Data\BG021916\
Data File : BG020987.D
Acq On : 20 Feb 2016 00:50
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:03:52 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

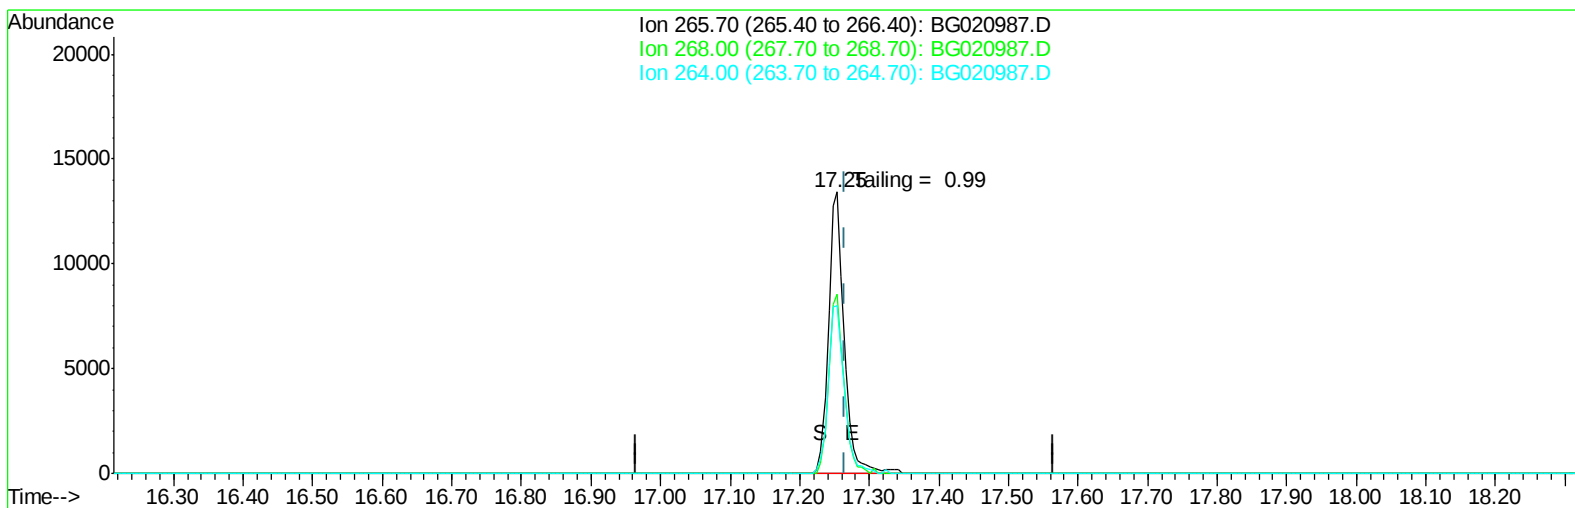

TIC: BG020987.D

(69) Pentachlorophenol (C)




17.254min (-0.012) 0.00ng

response 20867

Ion	Exp%	Act%
265.70	100	100
268.00	59.70	63.82
264.00	62.80	59.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG021916\
Data File : BG020987.D
Acq On : 20 Feb 2016 00:50
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:03:52 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

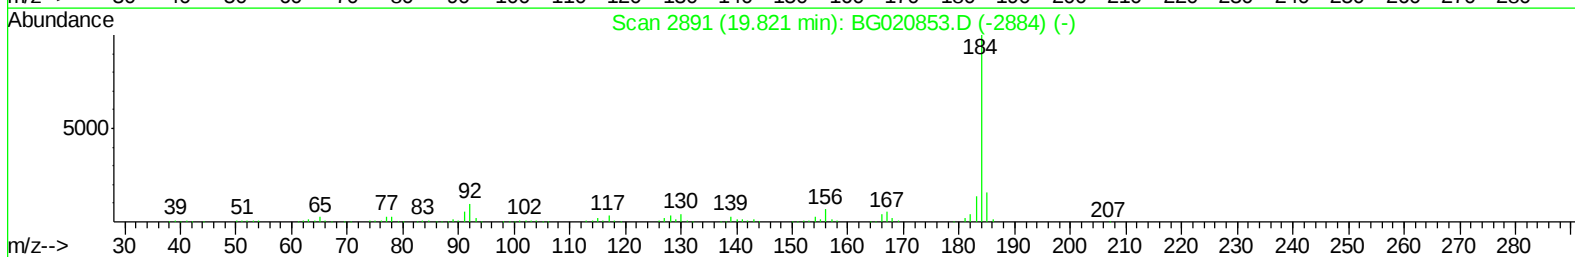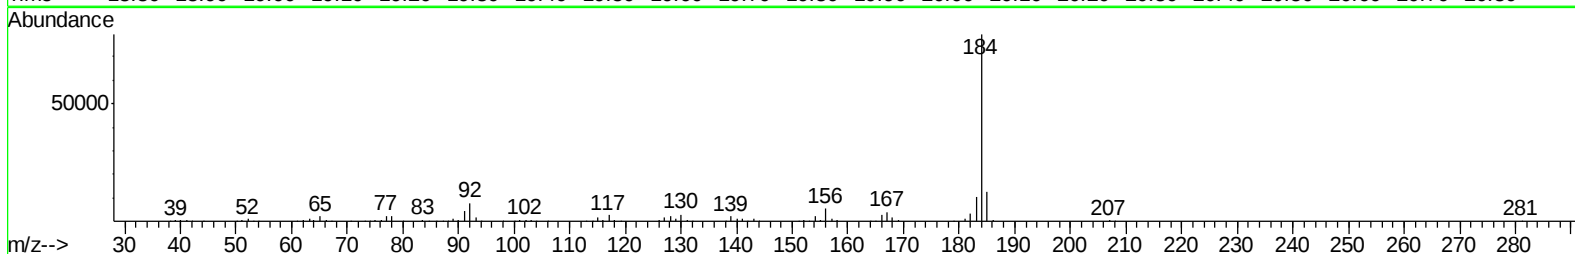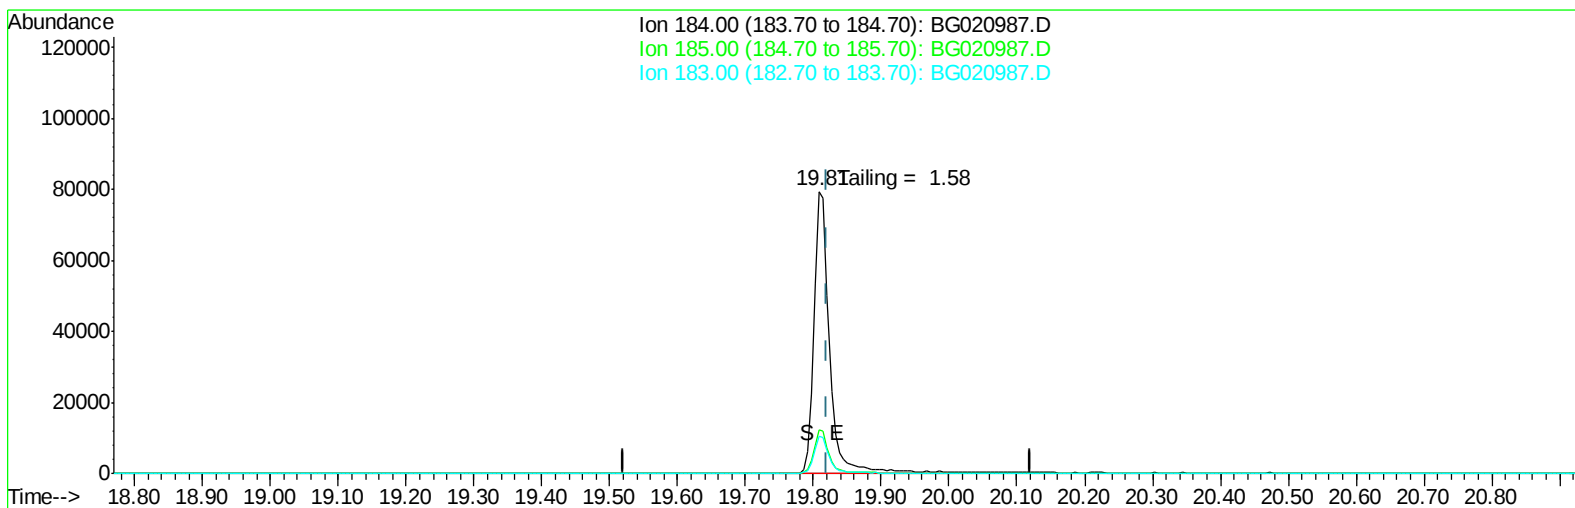

TIC: BG020987.D

(76) Benzidine

19.809min (-0.012) 0.00ng

response 124743

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.62
183.00	13.70	13.09
0.00	0.00	0.00