
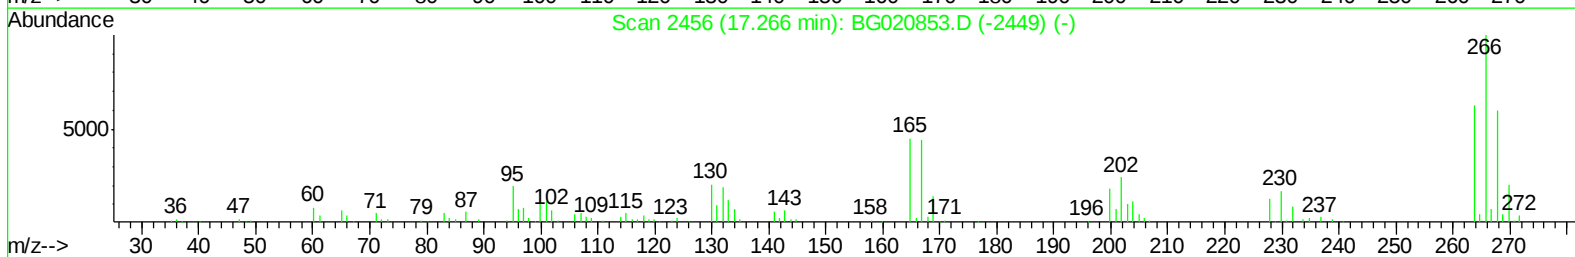
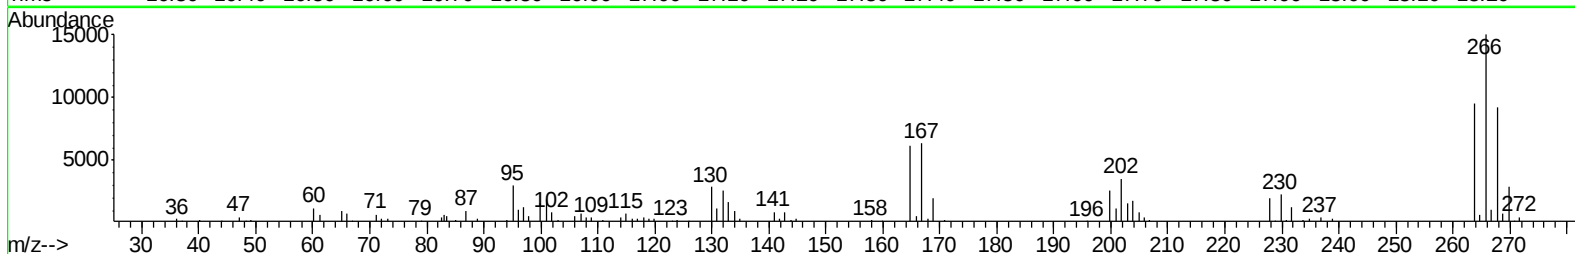


Data Path : Z:\HPCHEM1\BNA_G\Data\BG021916\
Data File : BG021005.D
Acq On : 20 Feb 2016 12:37
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:04:41 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

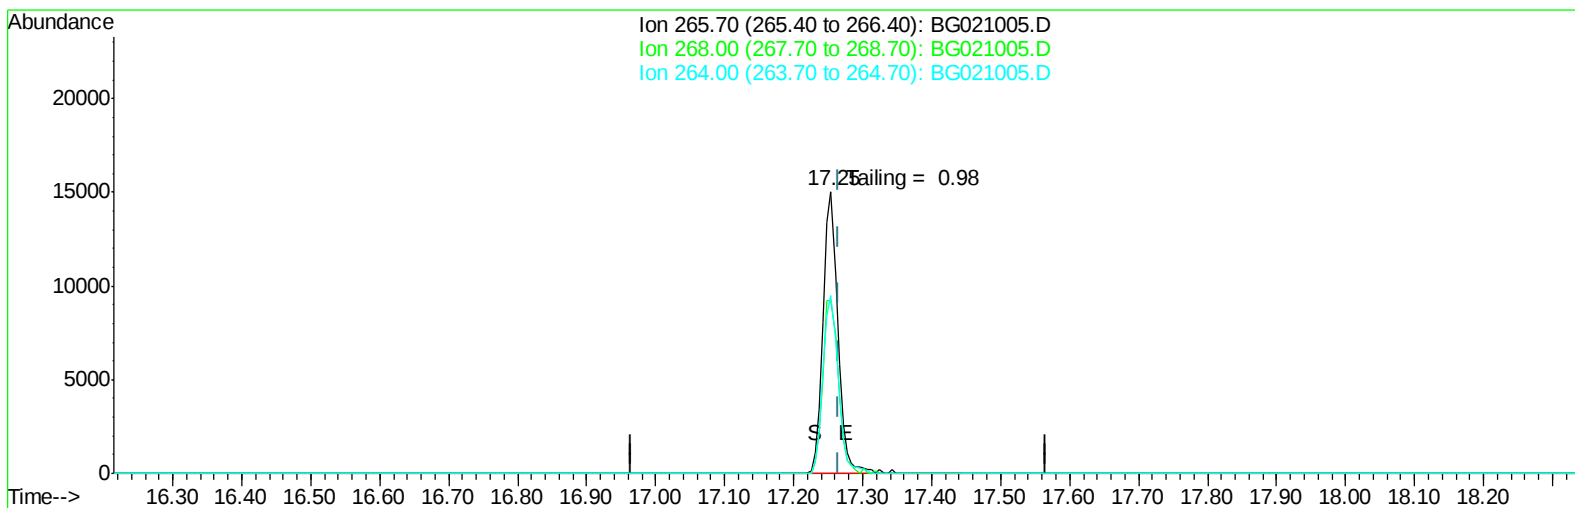

TIC: BG021005.D

(69) Pentachlorophenol (C)




17.254min (-0.012) 0.00ng

response 22367

Ion	Exp%	Act%
265.70	100	100
268.00	59.70	61.20
264.00	62.80	63.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG021916\
 Data File : BG021005.D
 Acq On : 20 Feb 2016 12:37
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:04:41 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 11 15:26:53 2016
 Response via : Initial Calibration

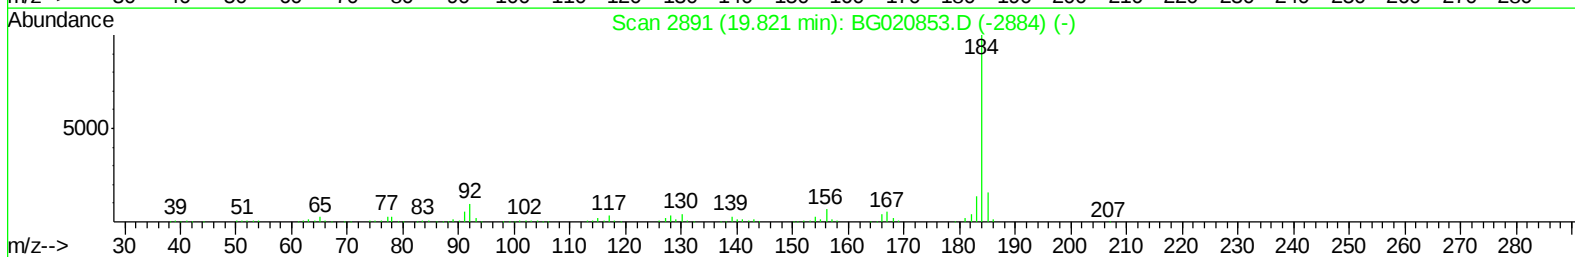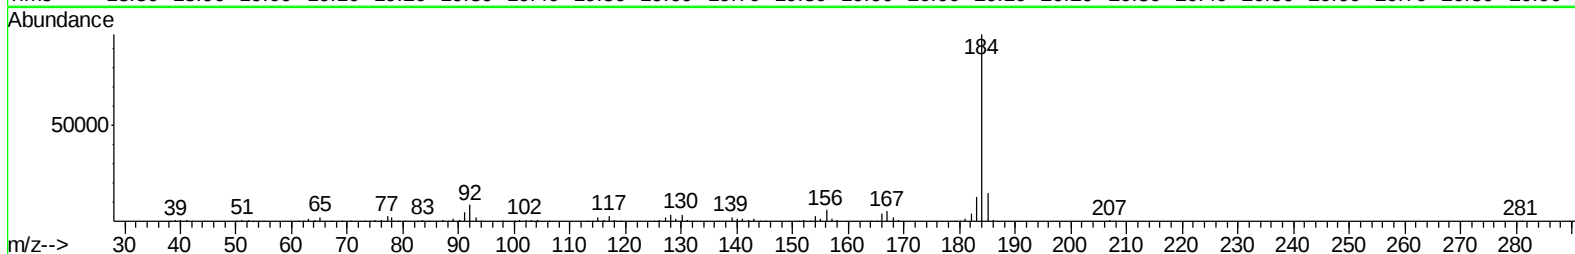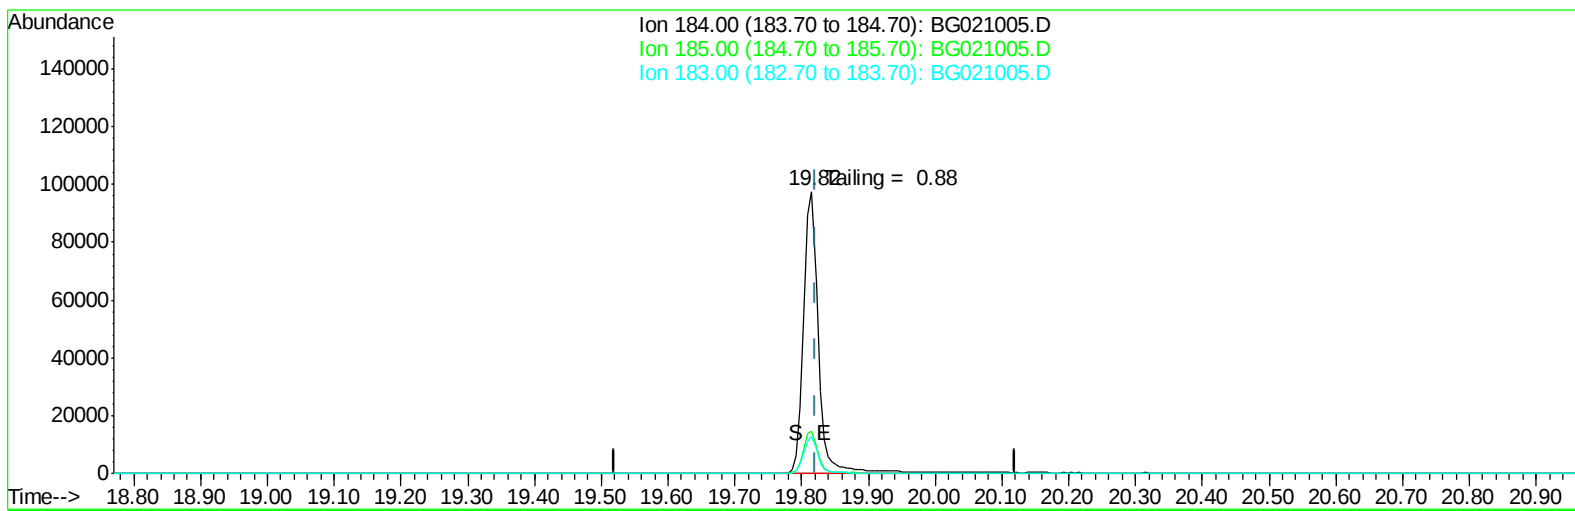

TIC: BG021005.D

(76) Benzidine

19.816min (-0.006) 0.00ng

response 145393

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.90
183.00	13.70	13.36
0.00	0.00	0.00