

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021916\
 Data File : BG021009.D
 Acq On : 20 Feb 2016 15:14
 Operator : SJ/UM
 Sample : H1453-14 20X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EGR-A-5

Quant Time: Feb 22 00:11:19 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 11 15:26:53 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.26	152	25748	20.00	ng	0.00
21) Naphthalene-d8	11.08	136	125918	20.00	ng	-0.01
38) Acenaphthene-d10	14.87	164	68623	20.00	ng	-0.01
63) Phenanthrene-d10	17.61	188	125378	20.00	ng	0.00
75) Chrysene-d12	21.89	240	118216	20.00	ng	-0.02
86) Perylene-d12	25.27	264	117484	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.79	112	5733	3.75	ng	0.00
7) Phenol-d6	7.40	99	5822	2.61	ng	0.00
23) Nitrobenzene-d5	9.43	82	13080	6.83	ng	-0.01
41) 2,4,6-Tribromophenol	16.35	330	5060	7.50	ng	0.00
44) 2-Fluorobiphenyl	13.50	172	26859	5.50	ng	-0.01
78) Terphenyl-d14	20.19	244	26419	5.21	ng	-0.01
Target Compounds						
57) Fluorene	15.92	166	18030	3.24	ng	# 83
70) Phenanthrene	17.65	178	42333	5.93	ng	# 95
77) Pyrene	20.00	202	20108	2.58	ng	# 82
83) Bis(2-ethylhexyl)phthalate	21.75	149	29338	5.30	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG021916\
Data File : BG021009.D
Acq On : 20 Feb 2016 15:14
Operator : SJ/UM
Sample : H1453-14 20X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EGR-A-5

Quant Time: Feb 22 00:11:19 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 15:26:53 2016
Response via : Initial Calibration

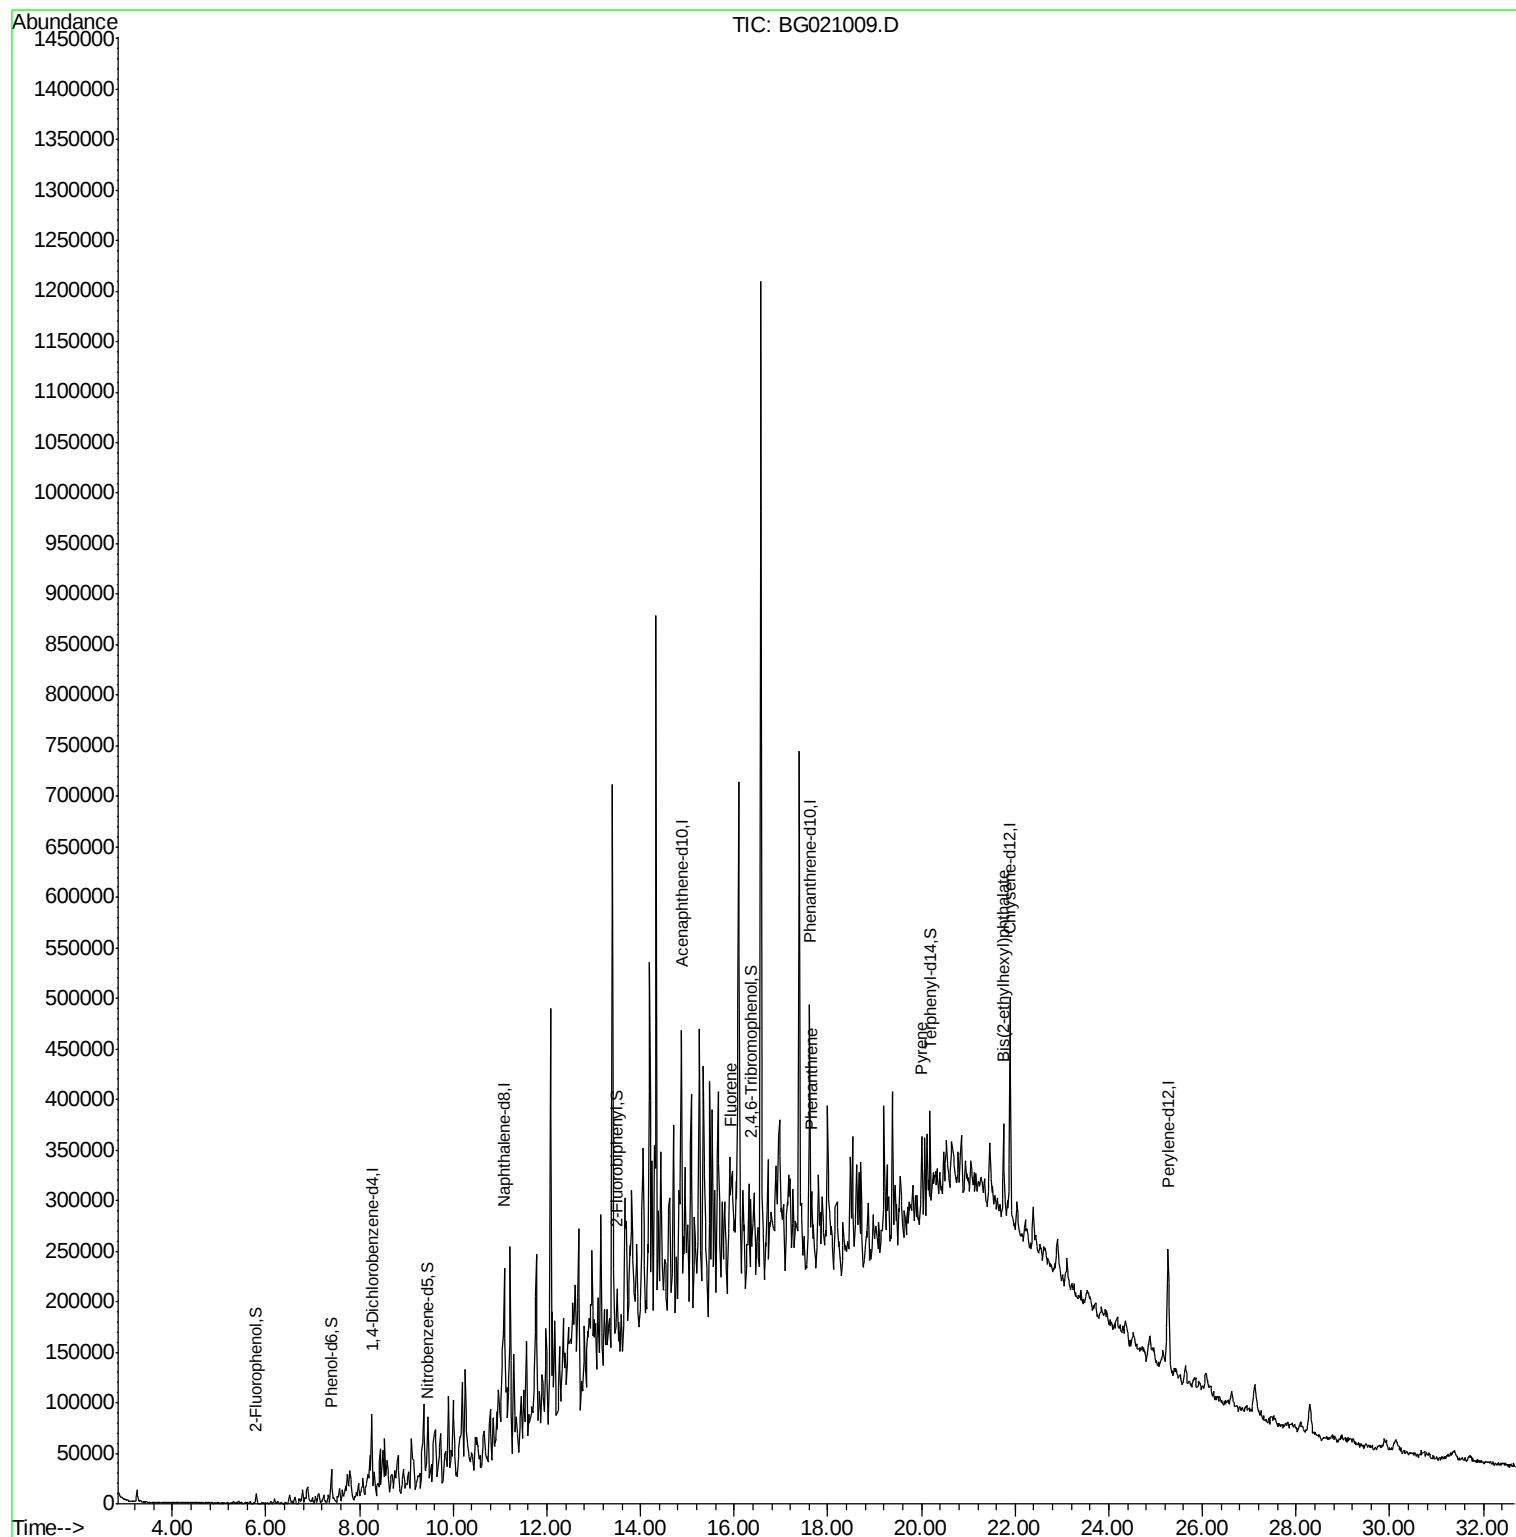




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.26 min Scan# 923
Delta R.T. -0.01 min
Lab File: BG021009.D
Acq: 20 Feb 2016 15:14

Instrument :
BNA_G
ClientSampleId :
EGR-A-5

Tot Ion:152 Resp: 25748
Ion Ratio Lower Upper
152 100
150 157.4 122.0 183.0
115 57.8 45.2 67.8

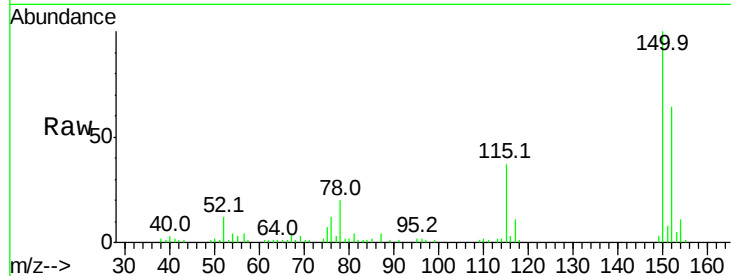


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

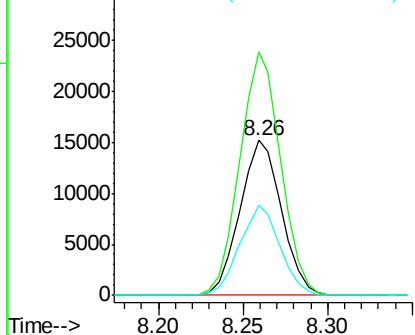



#5


2-Fluorophenol
Concen: 3.75 ng
RT: 5.79 min Scan# 503
Delta R.T. -0.01 min
Lab File: BG021009.D
Acq: 20 Feb 2016 15:14

Tgt Ion:112 Resp: 5733
Ion Ratio Lower Upper
112 100
64 45.4 39.3 58.9
63 22.7 18.2 27.4



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

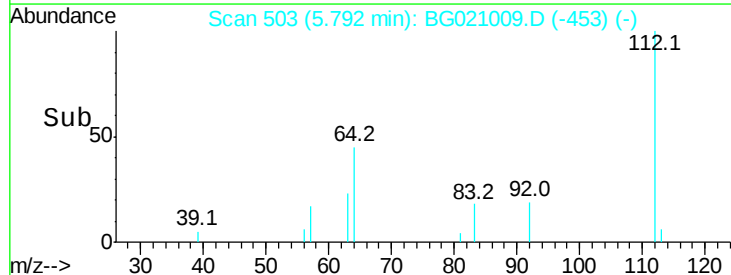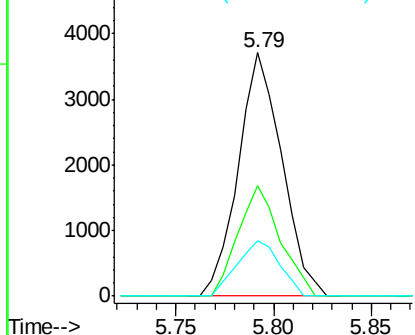



#7

Phenol-d6

Concen: 2.61 ng

RT: 7.40 min Scan# 777

Delta R.T. -0.01 min

Lab File: BG021009.D

Acq: 20 Feb 2016 15:14

Instrument :

BNA_G

ClientSampled :

EGR-A-5


Tot Ion: 99 Resp: 5822

Ion Ratio Lower Upper




99 100

42 15.5 8.4 12.6#

71 42.1 19.4 29.0#

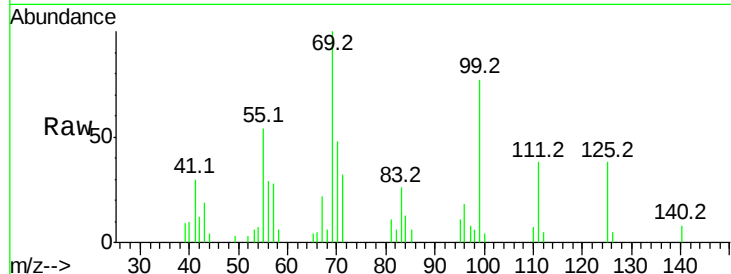

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

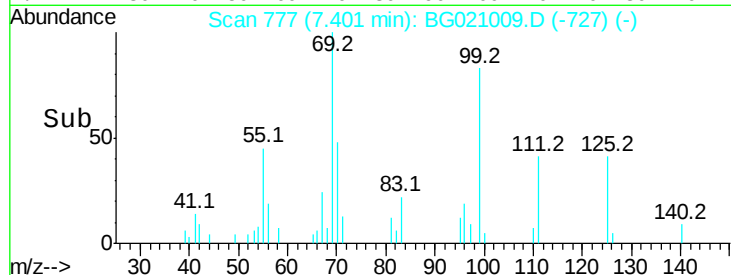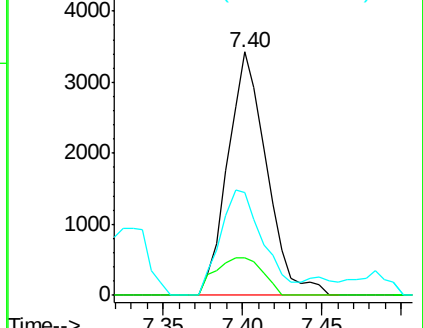

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.08 min Scan# 1404

Delta R.T. -0.01 min

Lab File: BG021009.D

Acq: 20 Feb 2016 15:14

Tgt Ion: 136 Resp: 125918


Ion Ratio Lower Upper

136 100



137 11.7 8.8 13.2


54 6.8 5.0 7.4

68 7.6 5.2 7.8

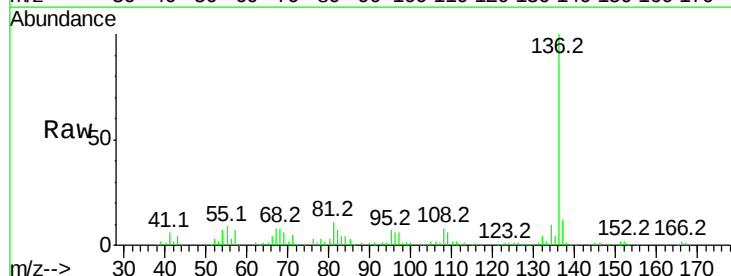

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

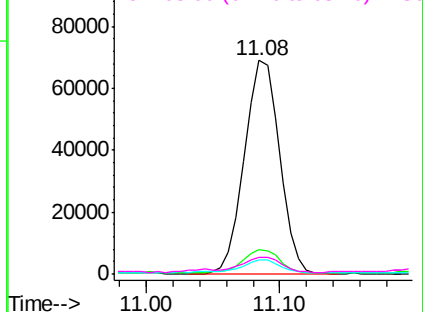

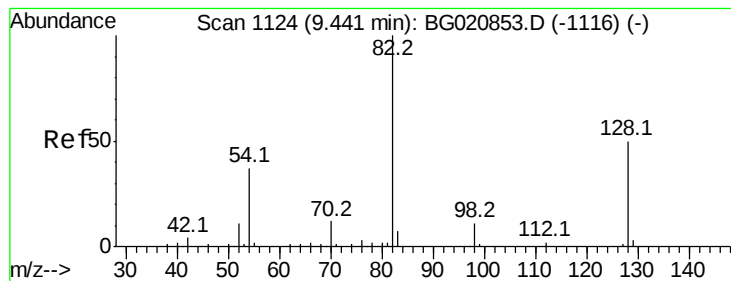

#23

Nitrobenzene-d5

Concen: 6.83 ng

RT: 9.43 min Scan# 1122

Delta R.T. -0.01 min

Lab File: BG021009.D

Acq: 20 Feb 2016 15:14

Instrument :

BNA_G

ClientSampled :

EGR-A-5


Tot Ion: 82 Resp: 13080

Ion Ratio Lower Upper




82 100

128 47.3 40.1 60.1

54 38.0 29.5 44.3

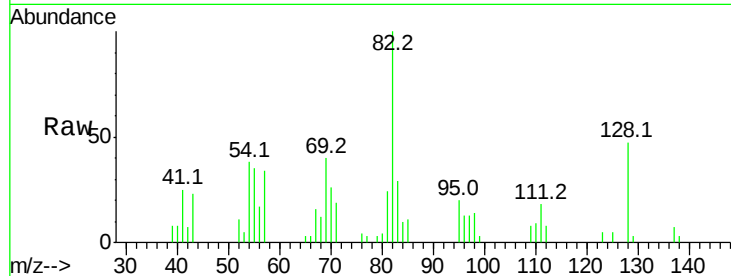

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

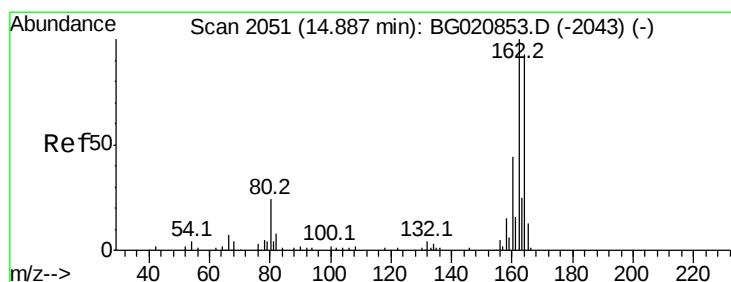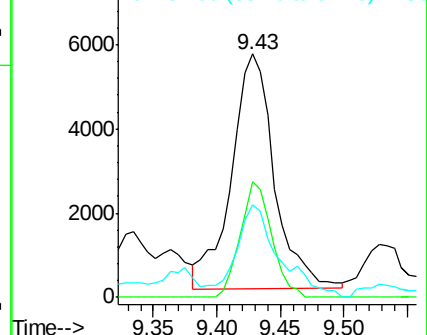

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.87 min Scan# 2049

Delta R.T. -0.01 min

Lab File: BG021009.D

Acq: 20 Feb 2016 15:14


Tgt Ion:164 Resp: 68623

Ion Ratio Lower Upper



164 100


162 106.3 85.7 128.5

160 47.2 37.4 56.0

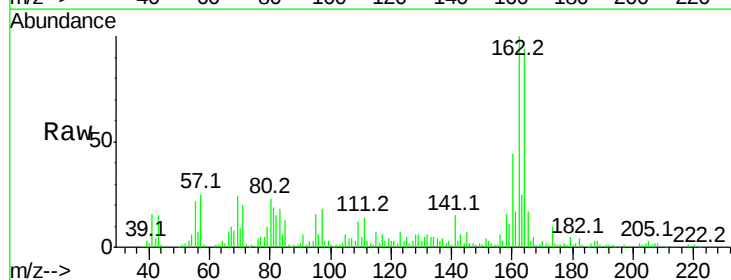

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC



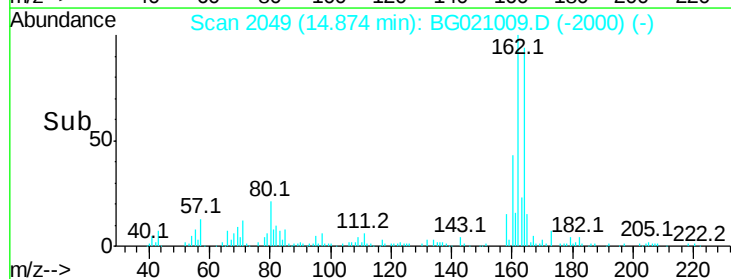
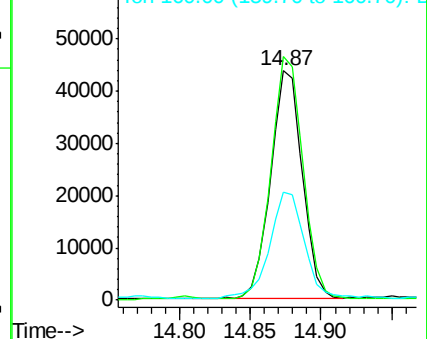


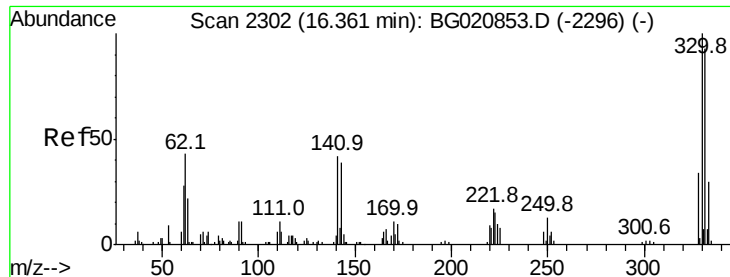

#41
 2,4,6-Tribromophenol
 Concen: 7.50 ng
 RT: 16.35 min Scan# 2301
 Delta R.T. -0.01 min
 Lab File: BG021009.D
 Acq: 20 Feb 2016 15:14




Instrument :
 BNA_G
 ClientSampled :
 EGR-A-5


Tot Ion:330 Resp: 5060
 Ion Ratio Lower Upper
 330 100
 332 98.1 76.1 114.1
 141 48.5 32.0 48.0#

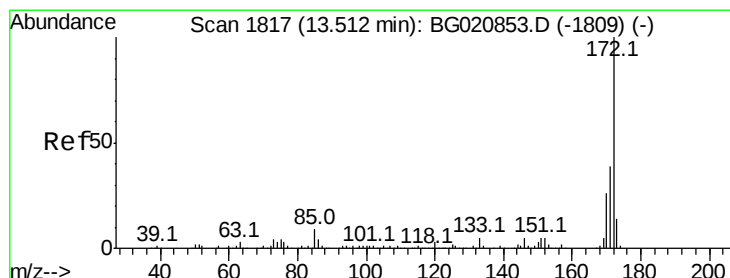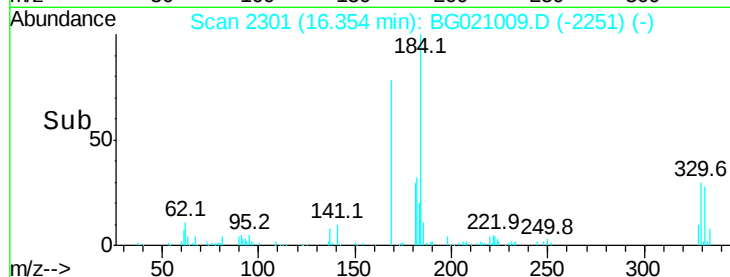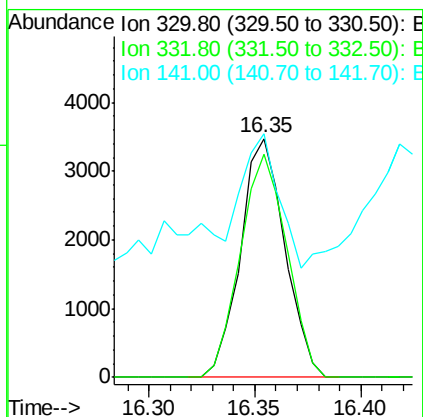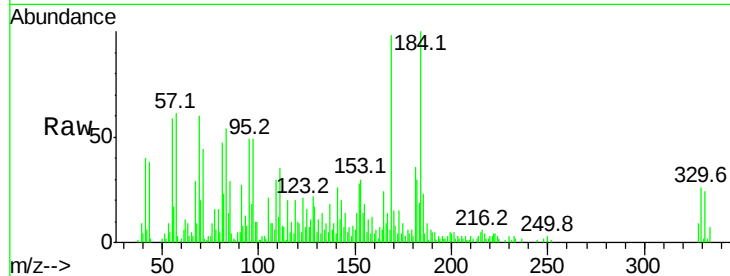

#44
 2-Fluorobiphenyl
 Concen: 5.50 ng
 RT: 13.50 min Scan# 1815
 Delta R.T. -0.01 min
 Lab File: BG021009.D
 Acq: 20 Feb 2016 15:14

Tgt Ion:172 Resp: 26859
 Ion Ratio Lower Upper
 172 100
 171 38.5 31.2 46.8
 170 24.7 20.6 30.8

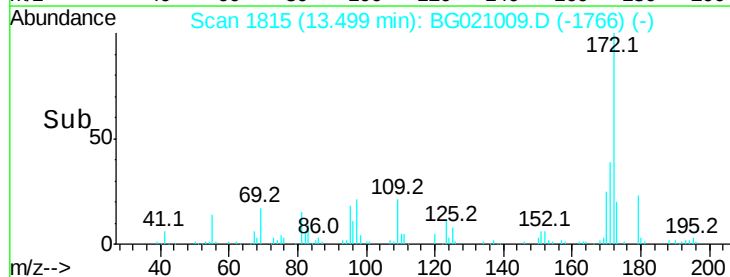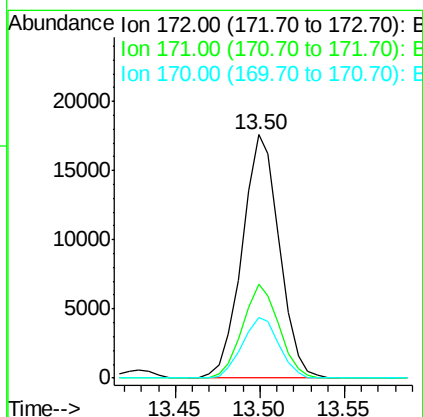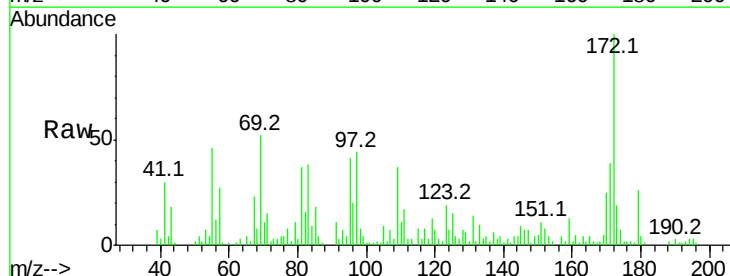



#57

Fluorene

Concen: 3.24 ng

RT: 15.92 min Scan# 2227

Delta R.T. -0.01 min

Lab File: BG021009.D

Acq: 20 Feb 2016 15:14

Instrument :

BNA_G

ClientSampleId :

EGR-A-5





Tot Ion:166 Resp: 18030

Ion Ratio Lower Upper

166 100

165 115.9 81.0 121.4

167 28.1 10.8 16.2#

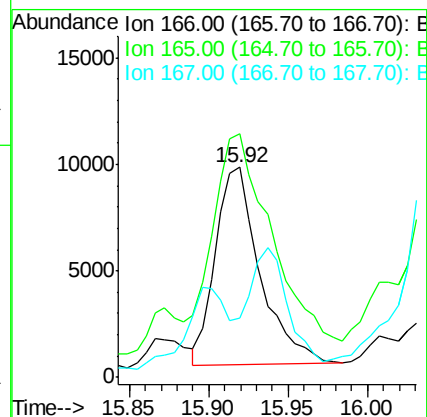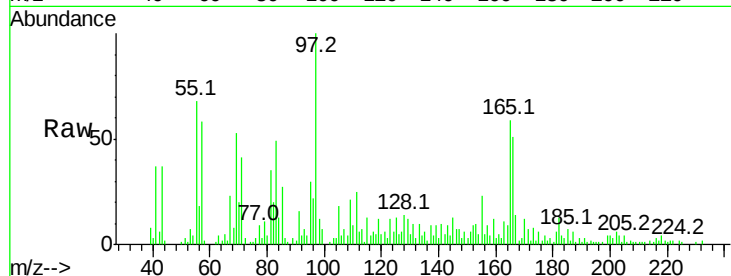

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.61 min Scan# 2515

Delta R.T. -0.01 min

Lab File: BG021009.D

Acq: 20 Feb 2016 15:14




Tgt Ion:188 Resp: 125378


Ion Ratio Lower Upper

188 100

94 12.7 9.4 14.0

80 12.7 10.2 15.4

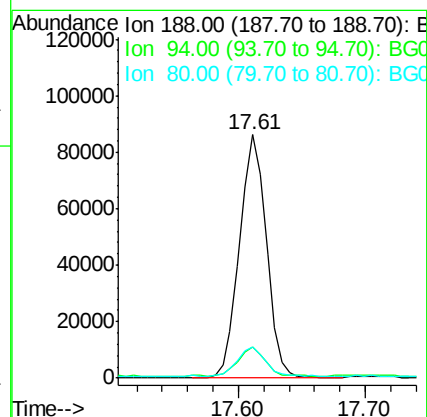







#70
Phenanthrene
Concen: 5.93 ng
RT: 17.65 min Scan# 2522
Delta R.T. -0.01 min
Lab File: BG021009.D
Acq: 20 Feb 2016 15:14

Instrument :
BNA_G
ClientSampleId :
EGR-A-5

Tot Ion	Ratio	Lower	Upper
178	100		
176	21.2	16.8	25.2
179	21.0	12.6	19.0

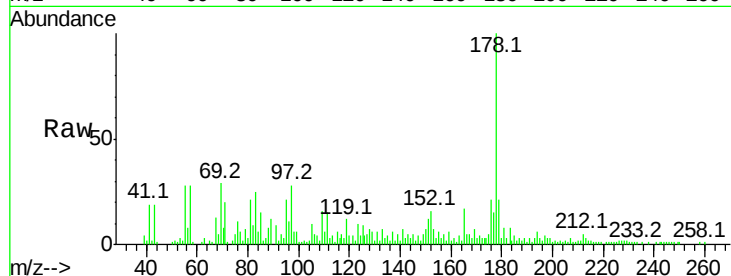


Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E


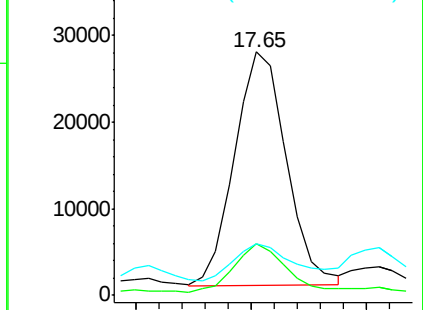



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.89 min Scan# 3243
Delta R.T. -0.02 min
Lab File: BG021009.D
Acq: 20 Feb 2016 15:14

Tgt Ion	Ratio	Lower	Upper
240	100		
120	15.8	13.0	19.4
236	26.9	21.0	31.4



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

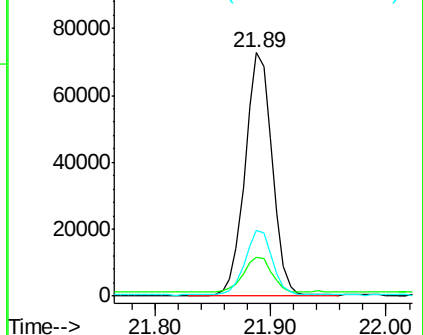



#77

Pvrene

Concen: 2.58 ng

RT: 20.00 min Scan# 2922

Delta R.T. -0.01 min

Lab File: BG021009.D

Acq: 20 Feb 2016 15:14

Instrument :

BNA_G

ClientSampleId :

EGR-A-5


Tot Ion:202 Resp: 20108

Ion Ratio Lower Upper

202 100

200 20.5 18.5 27.7




203 33.3 14.3 21.5#

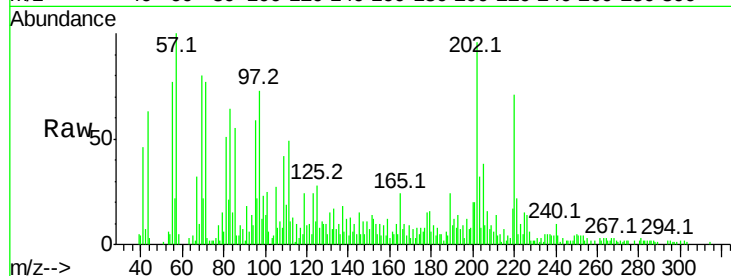

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

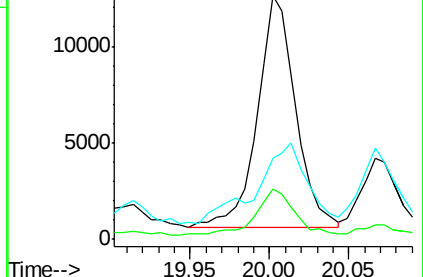

#78

Terphenyl-d14

Concen: 5.21 ng

RT: 20.19 min Scan# 2954

Delta R.T. -0.01 min

Lab File: BG021009.D

Acq: 20 Feb 2016 15:14


Tgt Ion:244 Resp: 26419

Ion Ratio Lower Upper

244 100

212 8.7 5.5 8.3#



122 17.0 11.4 17.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E




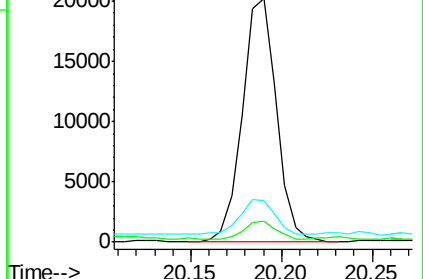


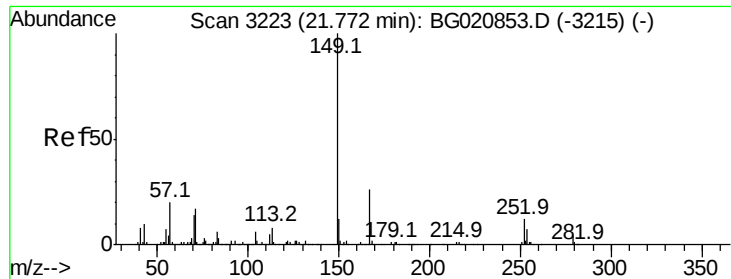

#83
 Bis(2-ethylhexyl)phthalate
 Concen: 5.30 ng
 RT: 21.75 min Scan# 3220
 Delta R.T. -0.02 min
 Lab File: BG021009.D
 Acq: 20 Feb 2016 15:14

Instrument :
 BNA_G
 ClientSampleId :
 EGR-A-5

Tot Ion:149 Resp: 29338
 Ion Ratio Lower Upper
 149 100
 167 28.3 20.9 31.3
 279 4.8 3.0 4.4#

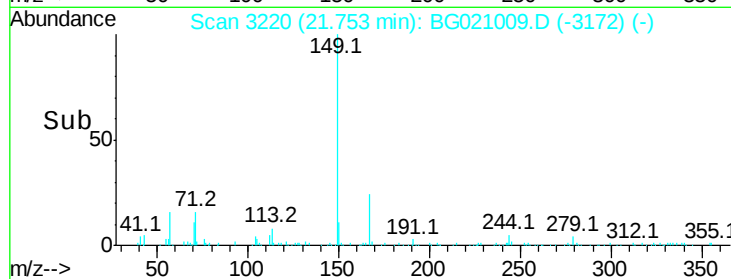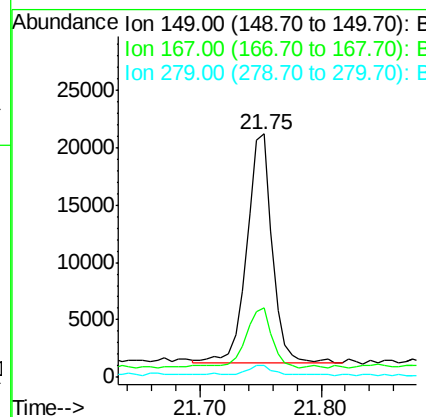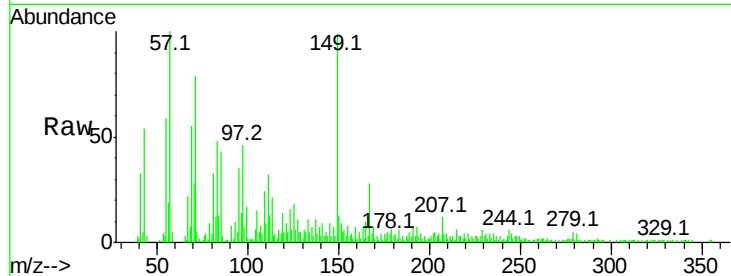

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.27 min Scan# 3818
 Delta R.T. -0.02 min
 Lab File: BG021009.D
 Acq: 20 Feb 2016 15:14

Tgt Ion:264 Resp: 117484
 Ion Ratio Lower Upper
 264 100
 260 24.5 19.9 29.9
 265 22.3 18.0 27.0

