
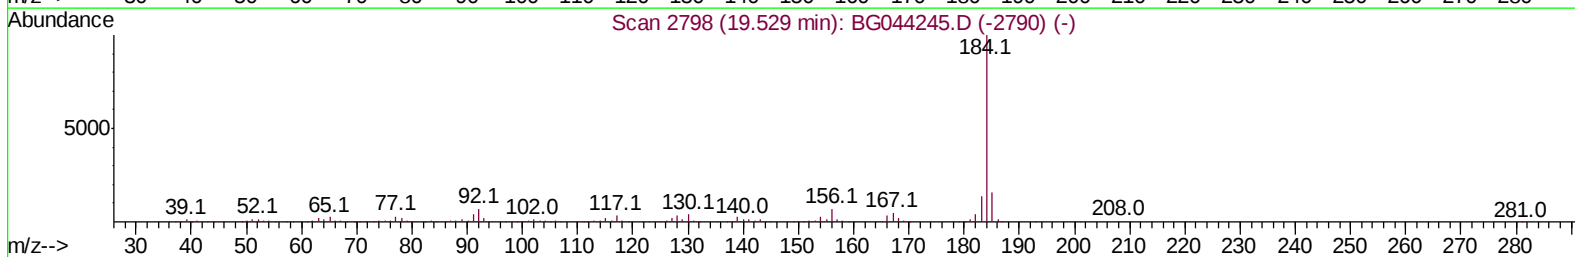
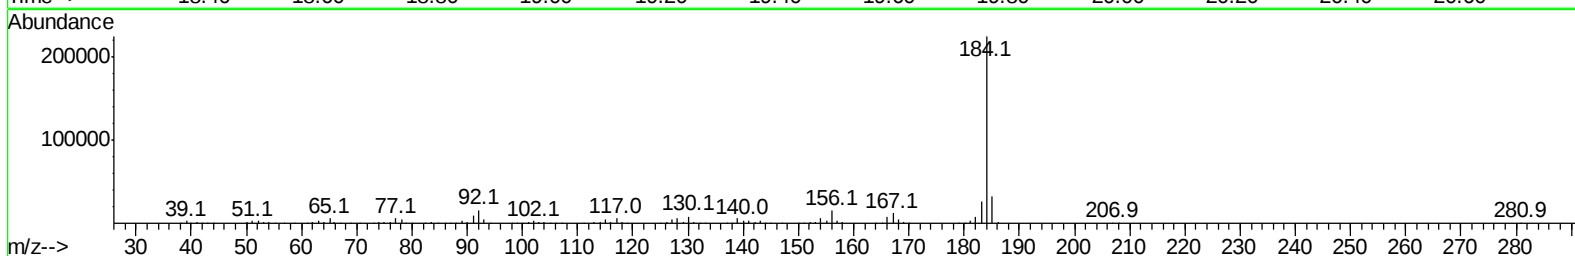


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021920\
 Data File : BG044485.D
 Acq On : 19 Feb 2020 10:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 08:52:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

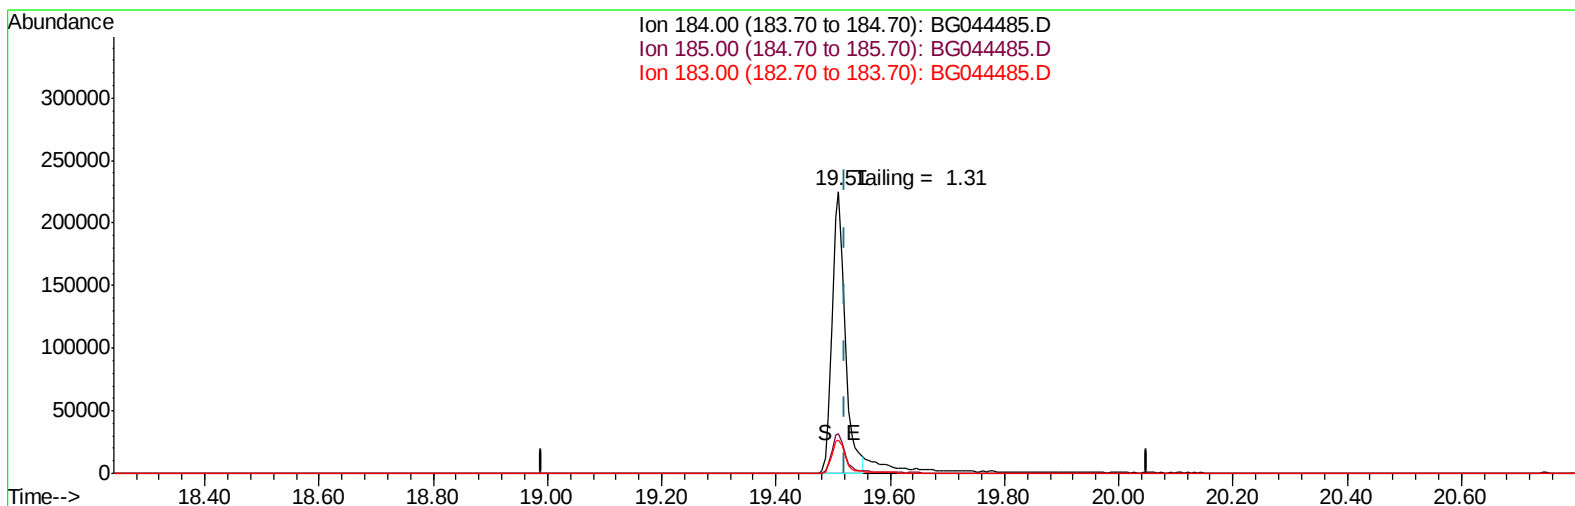

TIC: BG044485.D

(77) Benzidine




19.510min (-0.011) 0.00ng

response 395944

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	14.30
183.00	13.50	11.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021920\
Data File : BG044485.D
Acq On : 19 Feb 2020 10:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 08:52:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 10 16:11:50 2020
Response via : Initial Calibration

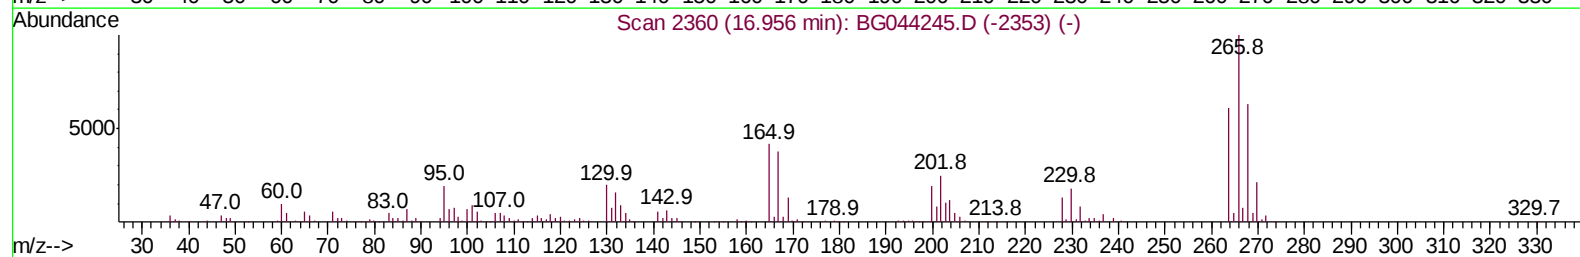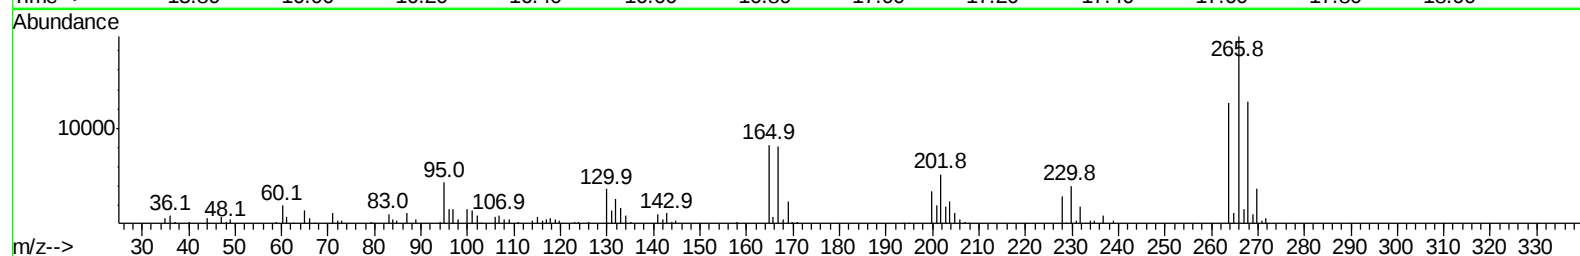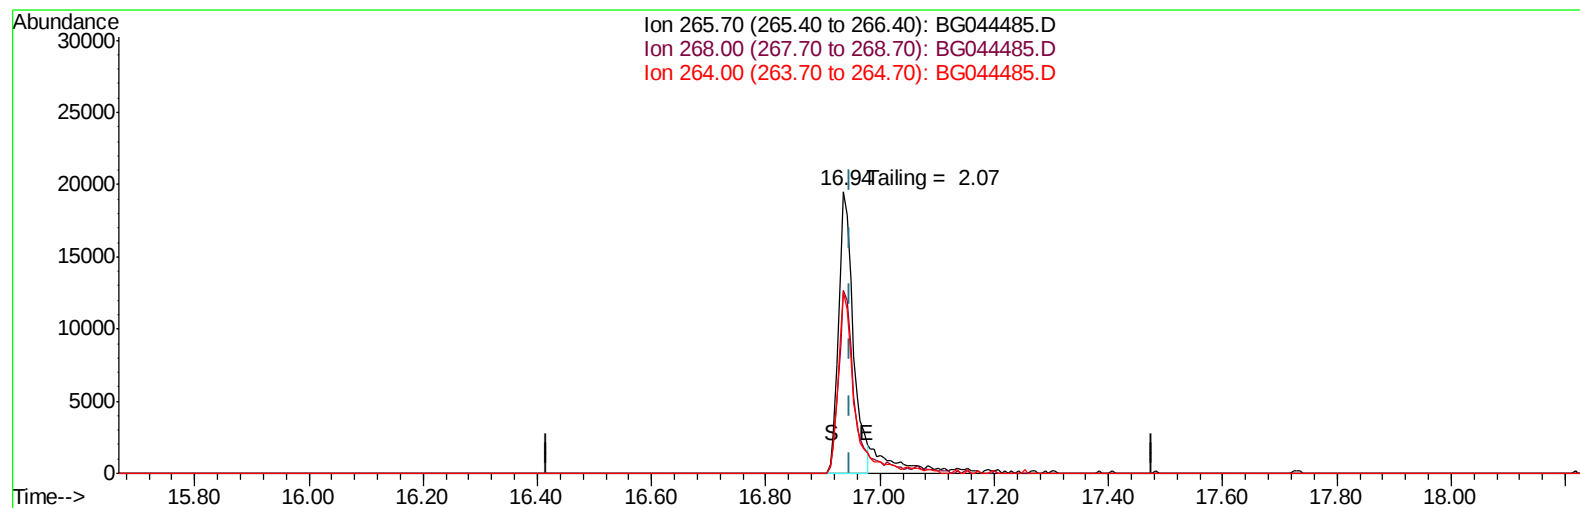

TIC: BG044485.D

(70) Pentachlorophenol (C)

16.936min (-0.011) 20810.12ng m

response 34489

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	65.11
264.00	60.90	64.59
0.00	0.00	0.00