
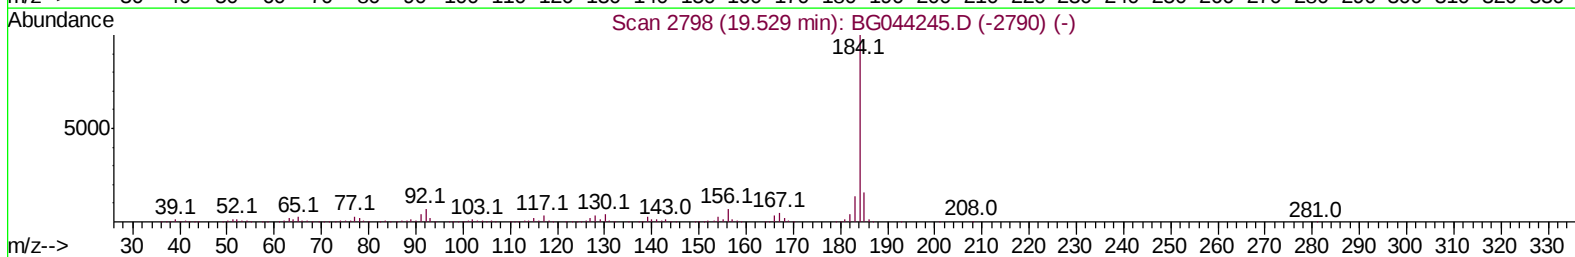
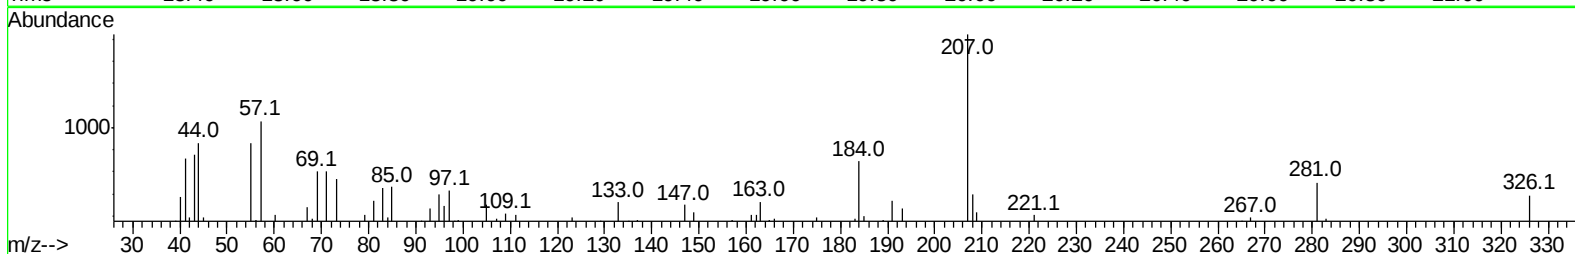


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021920\
Data File : BG044511.D
Acq On : 20 Feb 2020 6:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 08:57:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 10 16:11:50 2020
Response via : Initial Calibration

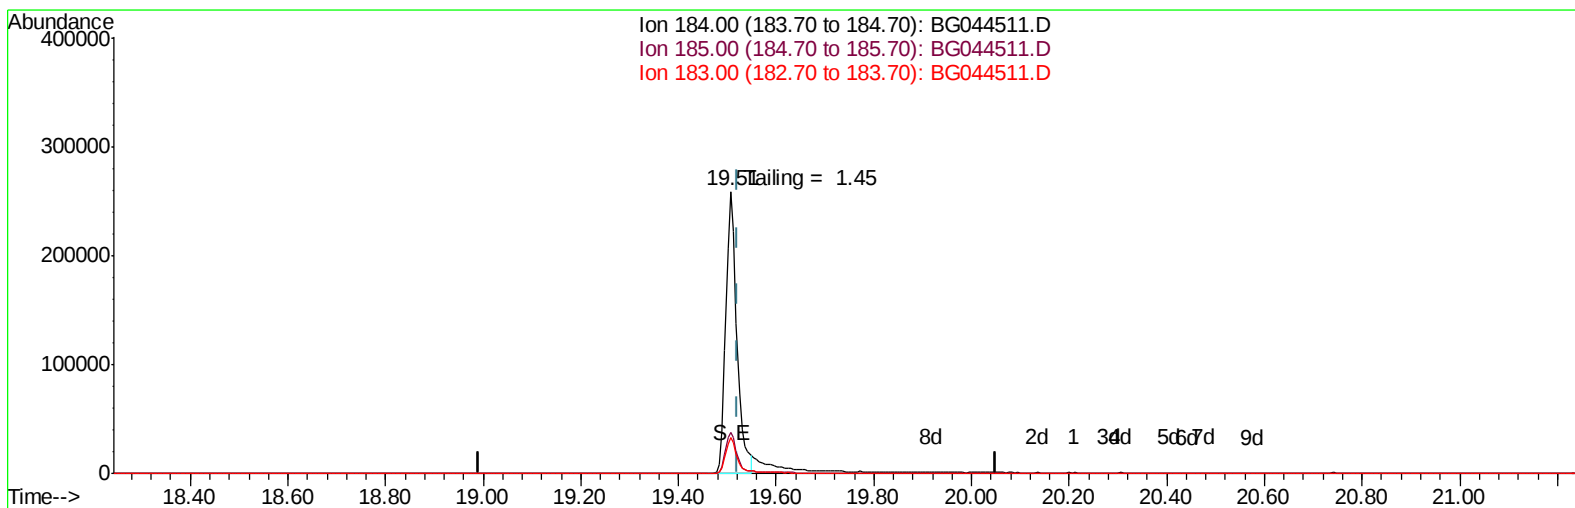

TIC: BG044511.D

(77) Benzidine




20.212min (+0.691) 179.12ng

response 313

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	27.91#
183.00	13.50	25.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021920\
 Data File : BG044511.D
 Acq On : 20 Feb 2020 6:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 08:57:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

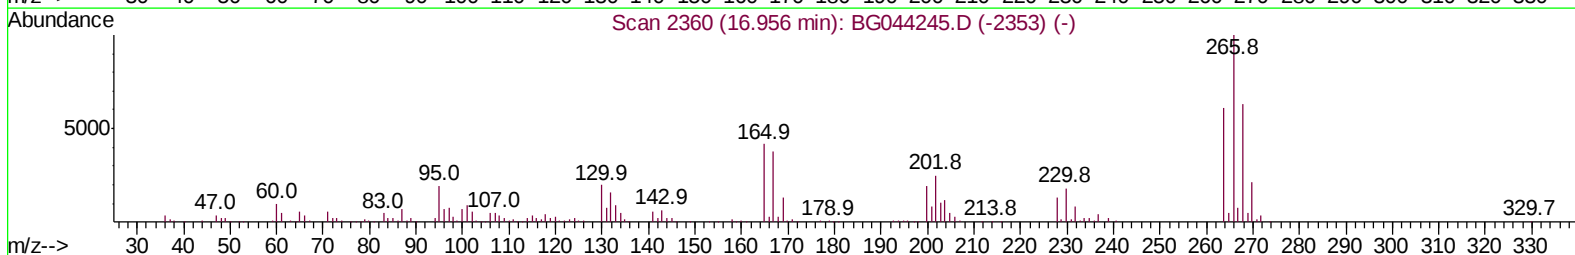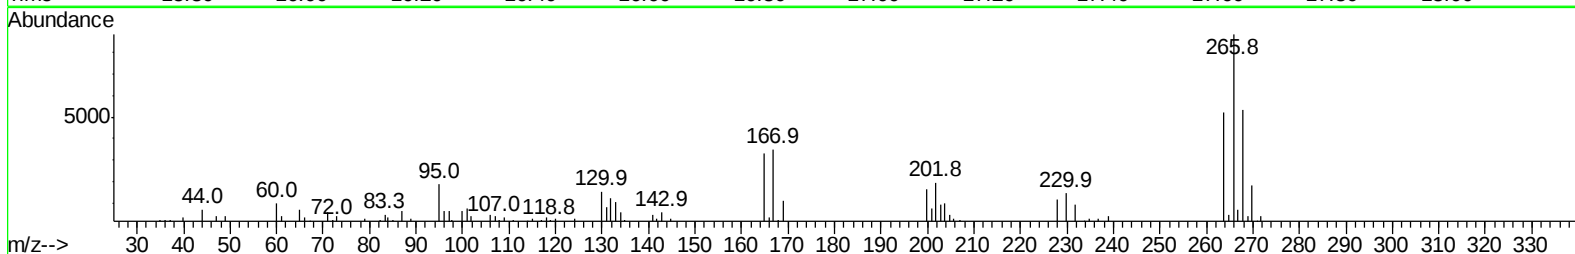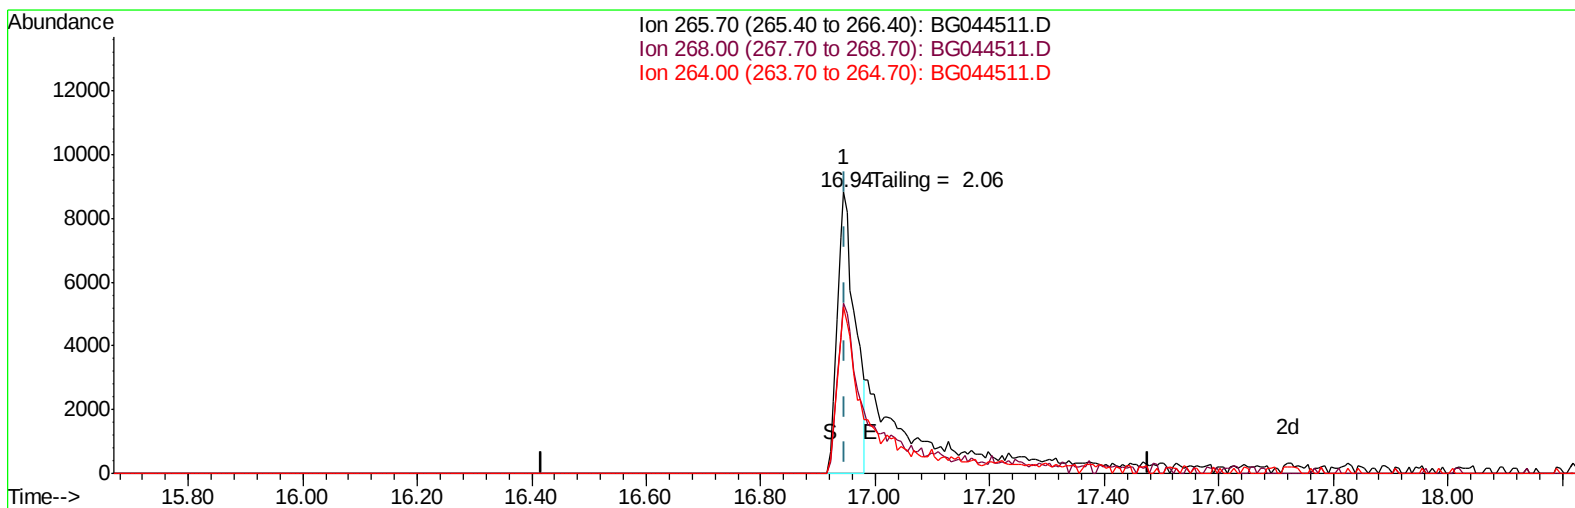

TIC: BG044511.D

(70) Pentachlorophenol (C)

16.945min (-0.003) 18023.48ng

response 23155

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	60.50
264.00	60.90	59.14
0.00	0.00	0.00