


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021920\
 Data File : BG044485.D
 Acq On : 19 Feb 2020 10:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

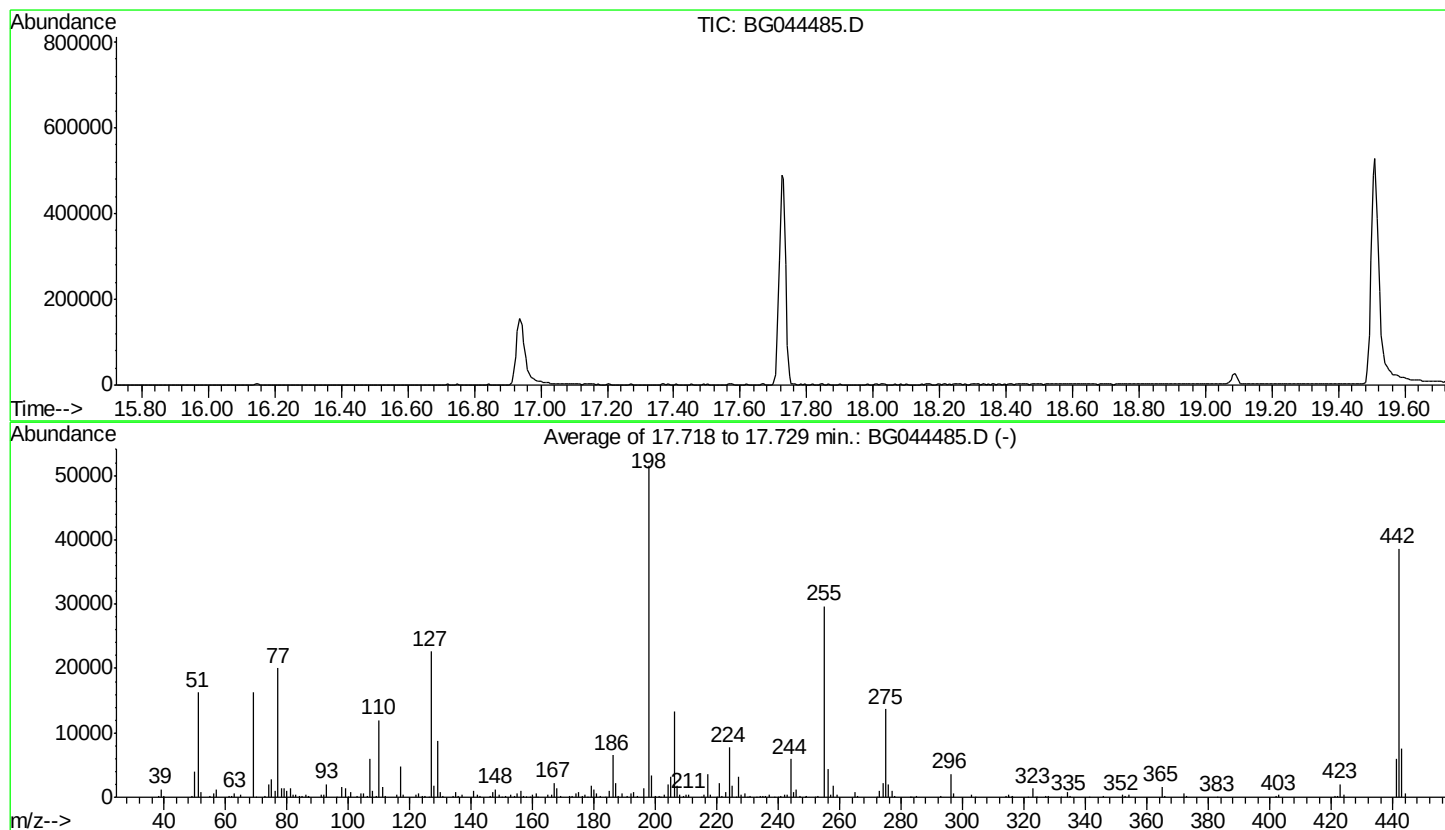

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	16301	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.6	16262	PASS
70	69	0.00	2	0.3	50	PASS
127	198	10	80	44.0	22664	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51514	PASS
199	198	5	9	6.7	3456	PASS
275	198	10	60	26.5	13654	PASS
365	198	1	100	3.1	1615	PASS
441	198	0.01	100	11.7	6026	PASS
442	198	50	100	75.1	38666	PASS
443	442	15	24	19.4	7519	PASS