


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021920\
 Data File : BG044492.D
 Acq On : 19 Feb 2020 16:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

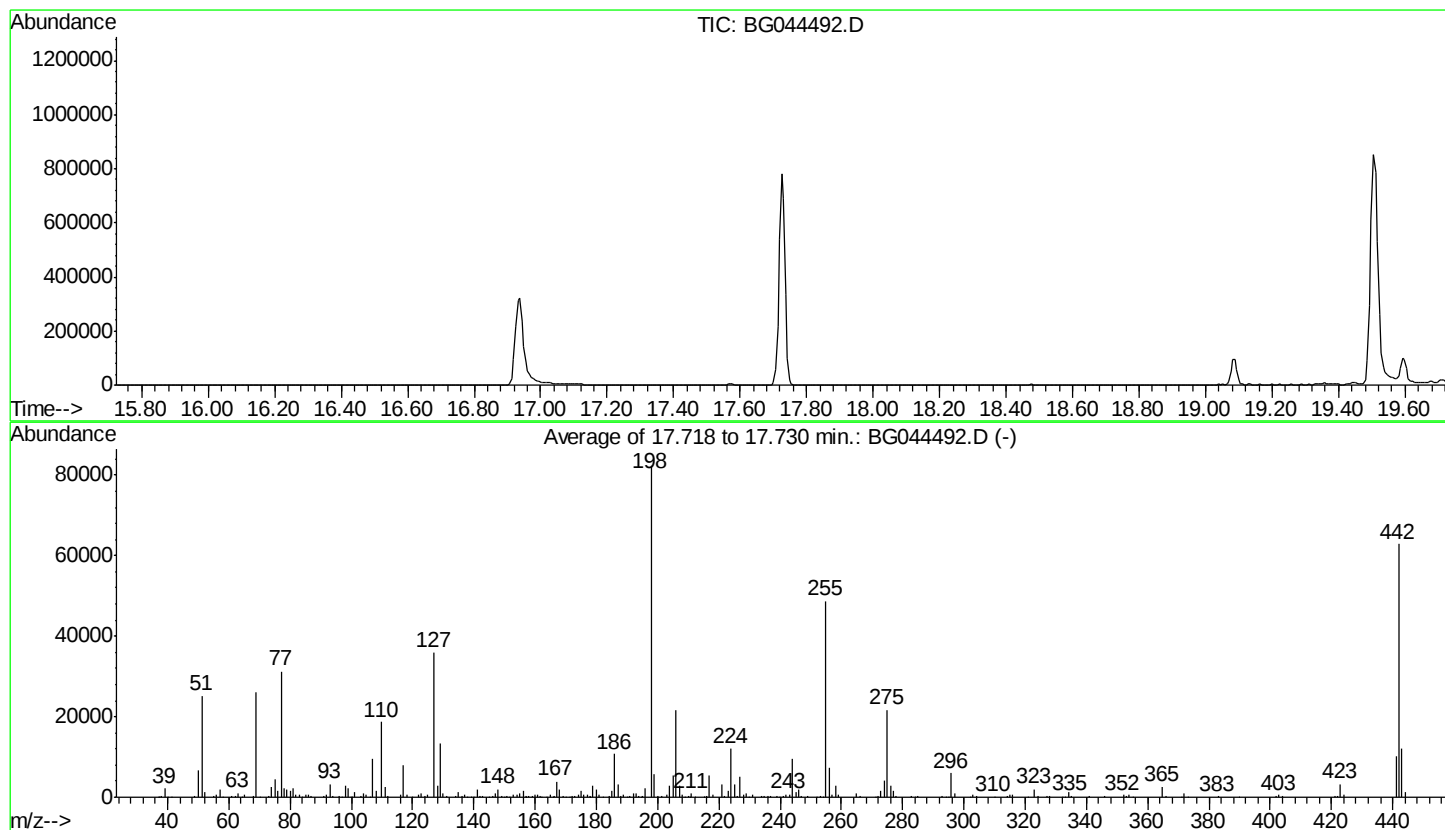

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	25178	PASS
68	69	0.00	2	1.4	355	PASS
69	198	0.00	100	31.6	26024	PASS
70	69	0.00	2	0.6	153	PASS
127	198	10	80	43.5	35797	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82344	PASS
199	198	5	9	7.0	5726	PASS
275	198	10	60	26.4	21709	PASS
365	198	1	100	3.2	2613	PASS
441	198	0.01	100	12.3	10099	PASS
442	198	50	100	76.4	62904	PASS
443	442	15	24	19.4	12195	PASS