


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021920\
 Data File : BG044511.D
 Acq On : 20 Feb 2020 6:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

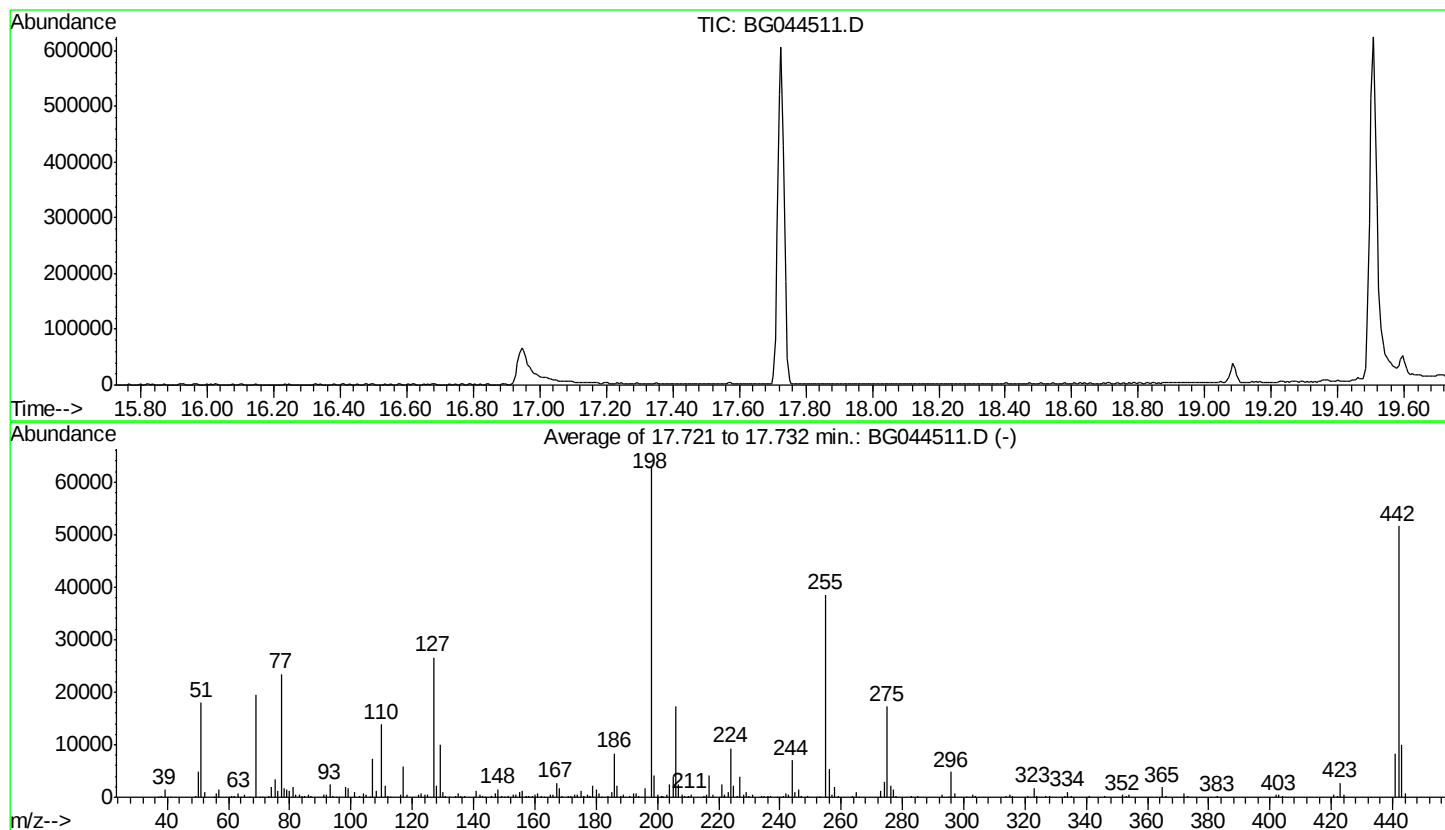

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	17957	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.8	19414	PASS
70	69	0.00	2	0.6	118	PASS
127	198	10	80	42.3	26677	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63122	PASS
199	198	5	9	6.6	4173	PASS
275	198	10	60	27.3	17243	PASS
365	198	1	100	3.0	1913	PASS
441	198	0.01	100	13.2	8340	PASS
442	198	50	100	81.7	51560	PASS
443	442	15	24	19.5	10068	PASS