

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021921\
Data File : BG048238.D
Acq On : 20 Feb 2021 15:58
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTD02042

Manual Integrations
APPROVED

mohammad
2/22/2021 2:09:05 PM

Quant Time: Feb 21 00:57:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 21 00:21:40 2021
Response via : Initial Calibration

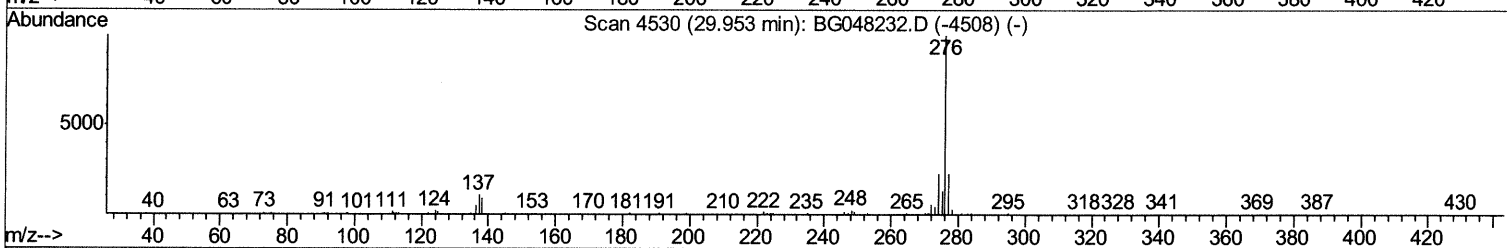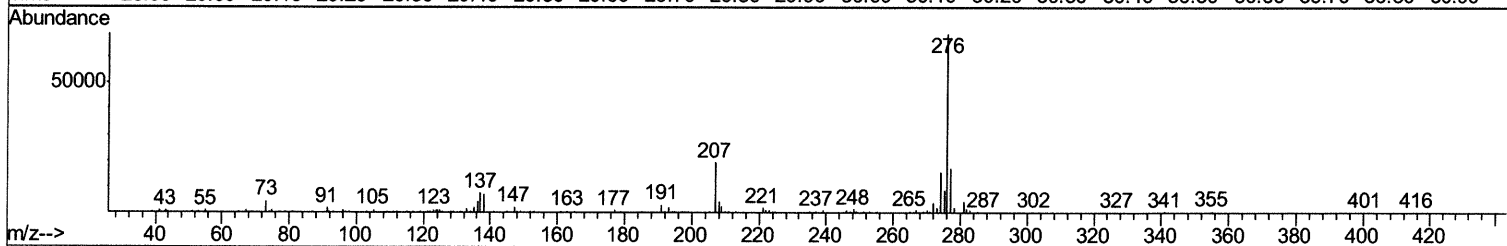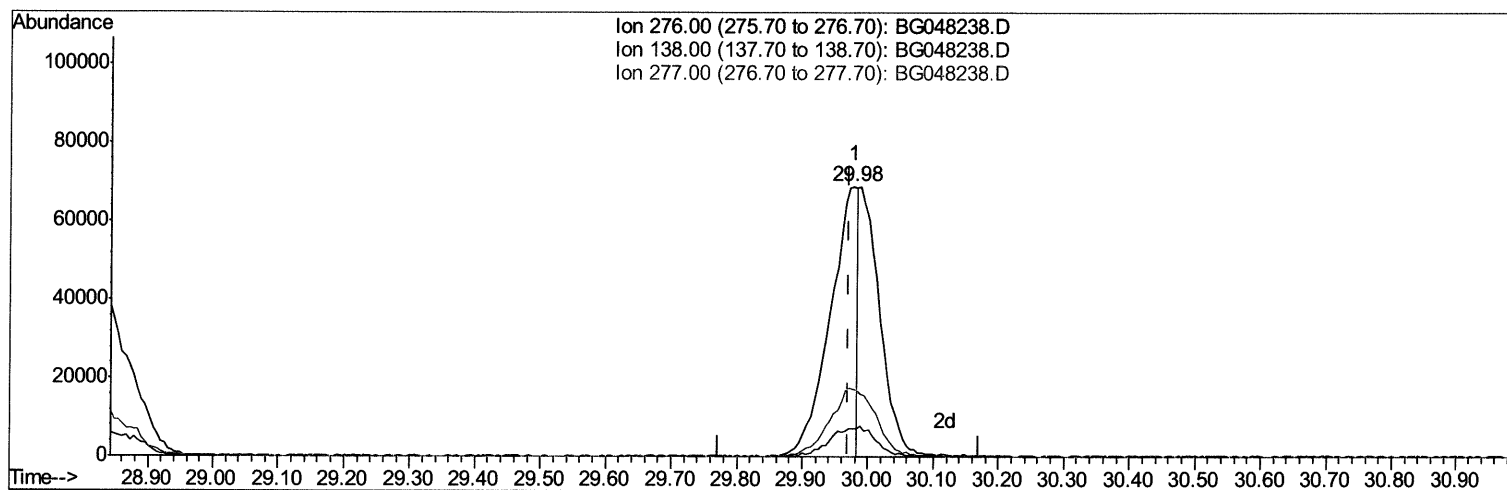

TIC: BG048238.D

(94) Benzo(g,h,i)perylene

29.977min (+0.006) 12.12ng/ul

response 203828

Ion	Exp%	Act%
276.00	100	100
138.00	8.90	10.48
277.00	22.70	24.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021921\
Data File : BG048238.D
Acq On : 20 Feb 2021 15:58
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTD02042

Manual Integrations
APPROVED

mohammad
2/22/2021 2:09:05 PM

Quant Time: Feb 21 00:57:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 21 00:21:40 2021
Response via : Initial Calibration

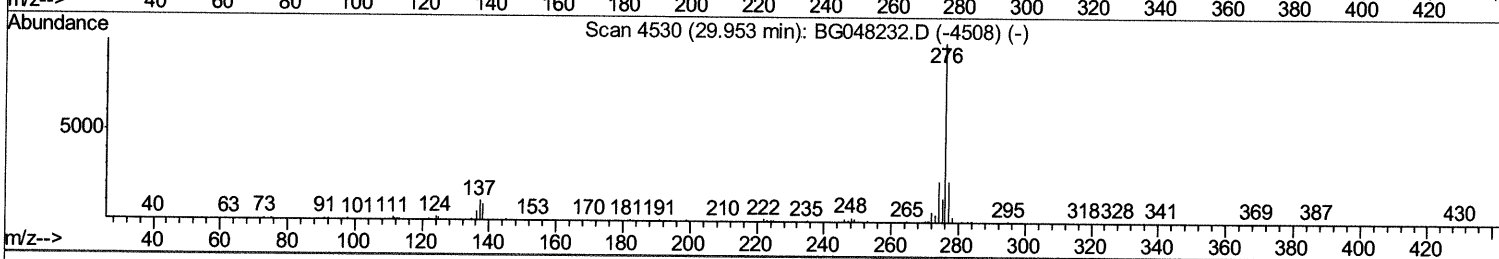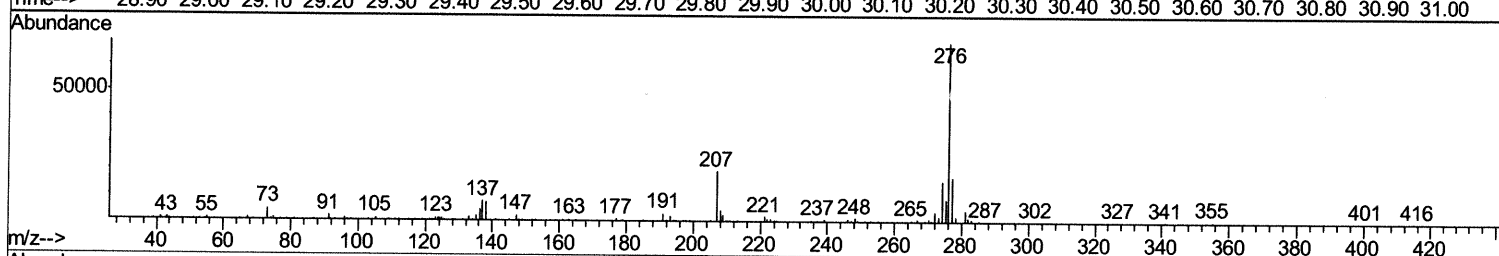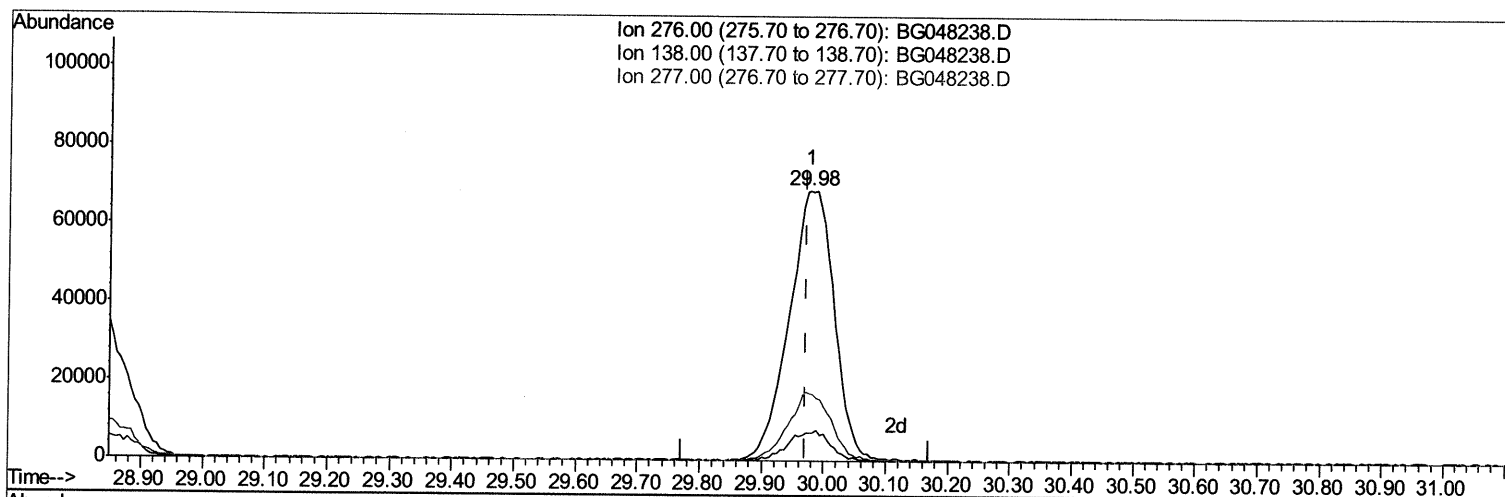

TIC: BG048238.D

(94) Benzo(g,h,i)perylene

29.977min (+0.006) 20.93ng/ul m 02/22/21 JU

response 352073

Ion	Exp%	Act%
276.00	100	100
138.00	8.90	10.48
277.00	22.70	24.94
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021921\
Data File : BG048238.D
Acq On : 20 Feb 2021 15:58
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTD02042

Manual Integrations
APPROVED

mohammad
2/22/2021 2:09:05 PM

Quant Time: Feb 21 00:59:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 21 00:21:40 2021
Response via : Initial Calibration

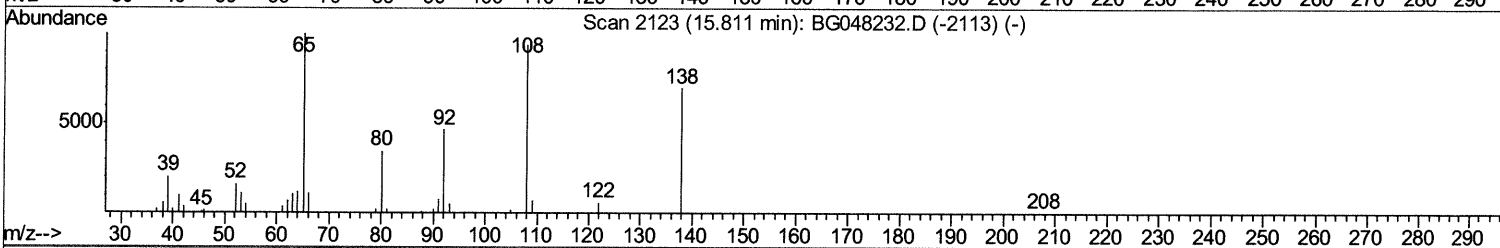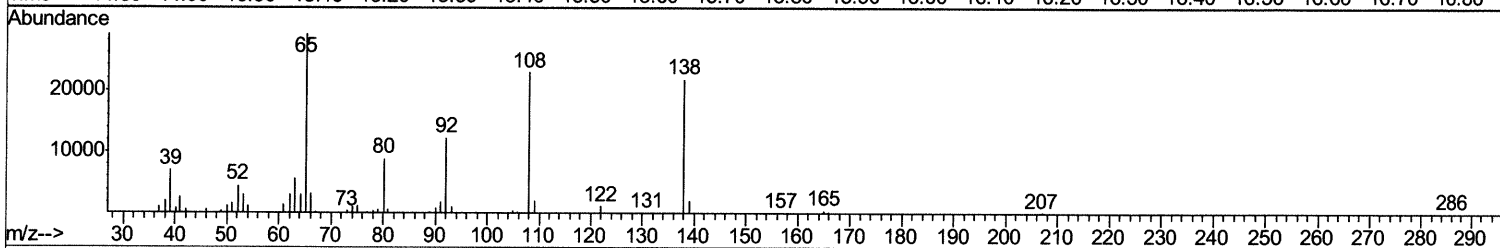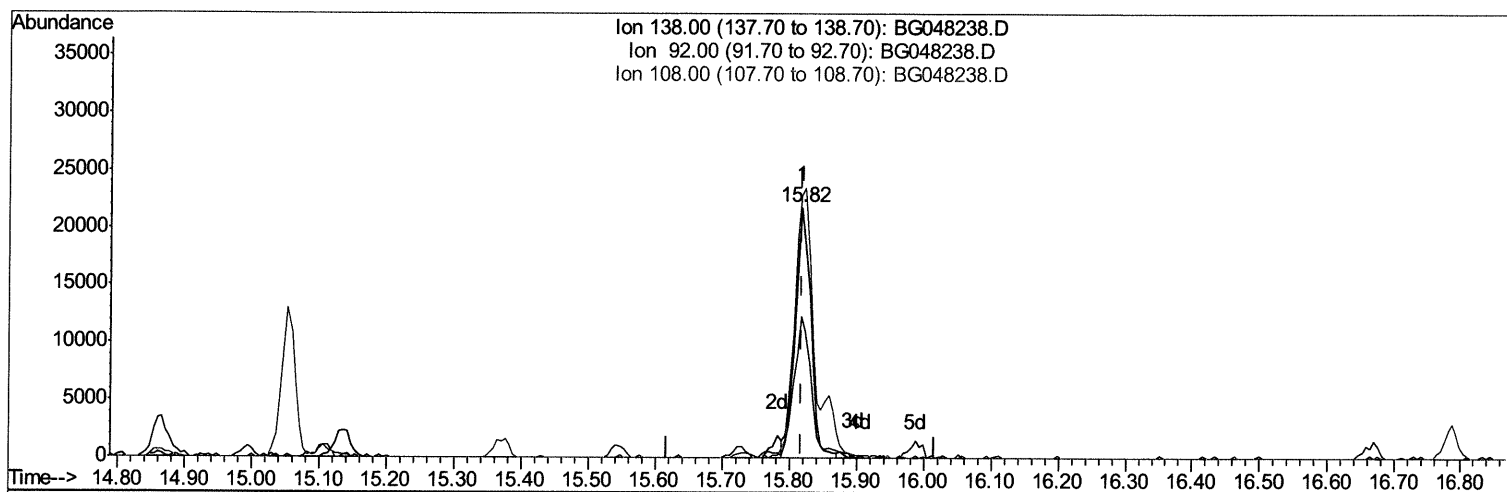

TIC: BG048238.D

(61) 4-Nitroaniline

15.817min (+0.000) 21.91ng/ul

response 35110

Ion	Exp%	Act%
138.00	100	100
92.00	67.30	56.19
108.00	126.60	104.85
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021921\
 Data File : BG048238.D
 Acq On : 20 Feb 2021 15:58
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTD02042

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:09:05 PM

Quant Time: Feb 21 00:59:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Feb 21 00:21:40 2021
 Response via : Initial Calibration

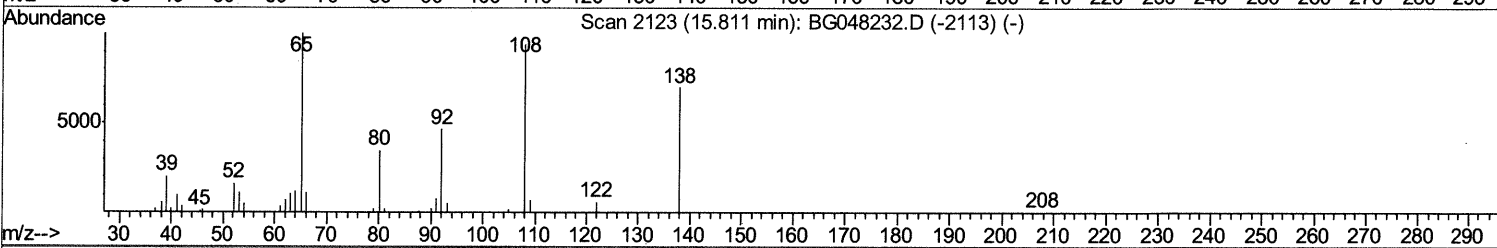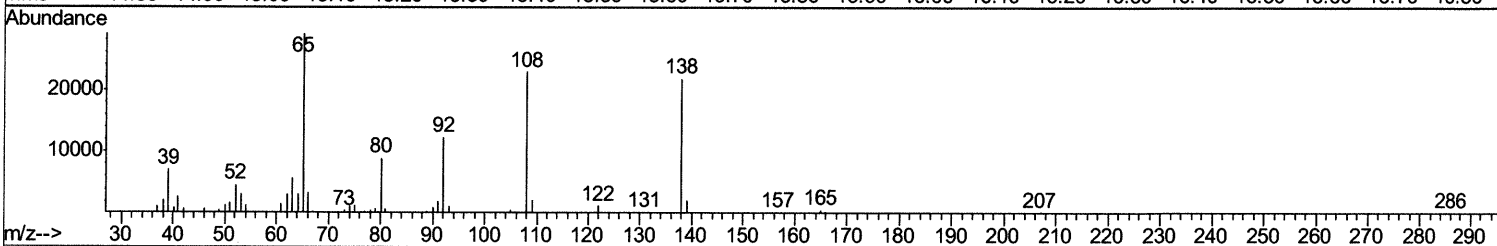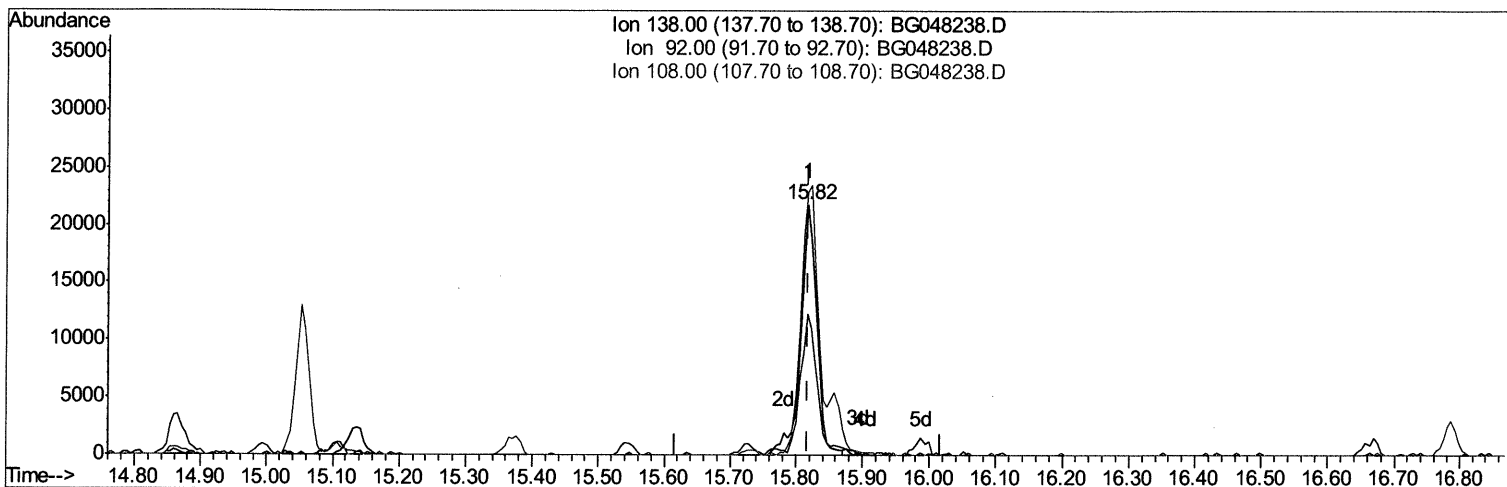

TIC: BG048238.D

(61) 4-Nitroaniline

15.817min (+0.000) 23.16ng/ul m 02/22/21JU

response 37109

Ion	Exp%	Act%
138.00	100	100
92.00	67.30	56.19
108.00	126.60	104.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021921\
 Data File : BG048238.D
 Acq On : 20 Feb 2021 15:58
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTD02042

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:09:05 PM

Quant Time: Feb 21 08:42:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Feb 21 00:21:40 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	37684	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	145758	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	104863	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.49	188	250335	20.00	ng/ul	0.00
78) Chrysene-d12	21.76	240	284727	20.00	ng/ul	0.00
86) Perylene-d12	25.05	264	286204	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.51	96	6986	7.72	ng/uL	0.00
5) Phenol-d5	7.30	99	67719	21.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	39470	20.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	47784	21.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.84	113	52255	20.98	ng/ul	0.00
19) Nitrobenzene-d5	9.28	128	23176	21.29	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	29246	22.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.56	165	55539	21.53	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	62727	24.61	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	161207	20.75	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	195654	20.61	ng/ul	0.00
52) 4-Nitrophenol-d4	14.98	143	27502	20.84	ng/ul	0.00
58) Fluorene-d10	15.73	176	146008	21.07	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.86	200	33051	21.53	ng/ul	0.00
71) Anthracene-d10	17.59	188	231398	21.56	ng/ul	0.00
79) Pyrene-d10	19.86	212	279444	19.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.82	264	298166	20.42	ng/ul	0.00

Target Compounds

					Ovalue	
2) 1,4-Dioxane	3.55	88	8386	8.078	ng/uL	94
4) Benzaldehyde	7.25	77	49277	26.399	ng/ul	94
6) Phenol	7.32	94	69618	21.237	ng/ul	97
8) Bis(2-Chloroethyl)ether	7.53	93	51833	20.936	ng/ul	89
10) 2-Chlorophenol	7.69	128	49020	20.791	ng/ul	92
11) 2-Methylphenol	8.57	108	48371	20.395	ng/ul	92
12) 2,2'-oxybis(1-Chloropropan	8.63	45	68103	21.046	ng/ul#	95
14) Acetophenone	8.94	105	86847	21.410	ng/ul	93
15) N-Nitroso-di-n-propylamine	8.92	70	47288	20.993	ng/ul	99
16) 4-Methylphenol	8.91	108	53356	20.847	ng/ul	90
17) Hexachloroethane	9.20	117	22124	21.007	ng/ul	97
20) Nitrobenzene	9.32	77	72328	21.810	ng/ul	97
21) Isophorone	9.85	82	123192	21.026	ng/ul	97
23) 2-Nitrophenol	10.04	139	29248	21.779	ng/ul	96
24) 2,4-Dimethylphenol	10.11	107	65491	22.037	ng/ul	98
25) Bis(2-Chloroethoxy)methane	10.32	93	68324	20.687	ng/ul	98
27) 2,4-Dichlorophenol	10.59	162	52990	21.476	ng/ul	88
28) Naphthalene	10.98	128	153411	20.867	ng/ul#	95
30) 4-Chloroaniline	11.09	127	61789	23.633	ng/ul	92
31) Hexachlorobutadiene	11.25	225	46666	21.685	ng/ul	90
32) Caprolactam	11.89	113	17837	20.716	ng/ul	81
33) 4-Chloro-3-methylphenol	12.23	107	57479	21.041	ng/ul#	95
34) 2-Methylnaphthalene	12.57	142	115554	20.678	ng/ul	97

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021921\
 Data File : BG048238.D
 Acq On : 20 Feb 2021 15:58
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTD02042

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:09:05 PM

Quant Time: Feb 21 08:42:28 2021

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sun Feb 21 00:21:40 2021

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.79	142	113637	21.022	ng/uL	95
37) 1,2,4,5-Tetrachlorobenzene	12.94	216	82422	21.850	ng/uL	98
38) Hexachlorocyclopentadiene	12.91	237	43142	17.739	ng/uL#	87
39) 2,4,6-Trichlorophenol	13.18	196	52972	22.805	ng/uL	95
40) 2,4,5-Trichlorophenol	13.27	196	56905	24.106	ng/uL	94
41) 1,1'-Biphenyl	13.57	154	151704	21.089	ng/uL	99
42) 2-Chloronaphthalene	13.62	162	129333	21.821	ng/uL	96
43) 2-Nitroaniline	13.83	65	47310	23.081	ng/uL	92
45) Dimethylphthalate	14.19	163	163463	20.358	ng/uL	98
46) 2,6-Dinitrotoluene	14.32	165	36100	21.377	ng/uL	91
48) Acenaphthylene	14.47	152	183148	21.567	ng/uL	97
49) 3-Nitroaniline	14.66	138	34429	24.188	ng/uL	88
50) Acenaphthene	14.80	153	134301	21.072	ng/uL	94
51) 2,4-Dinitrophenol	14.87	184	21527	20.412	ng/uL	97
53) 4-Nitrophenol	14.99	109	32271	21.658	ng/uL	91
54) Dibenzofuran	15.14	168	193505	20.803	ng/uL	99
55) 2,4-Dinitrotoluene	15.11	165	51439	21.206	ng/uL#	95
56) 2,3,4,6-Tetrachlorophenol	15.37	232	52116	21.596	ng/uL	93
57) Diethylphthalate	15.55	149	169307	20.426	ng/uL	97
59) Fluorene	15.79	166	153030	20.350	ng/uL	96
60) 4-Chlorophenyl-phenylether	15.77	204	92951	20.604	ng/uL	93
61) 4-Nitroaniline	15.82	138	37109m >	23.159	ng/uL >	02/22/21 JU
64) 4,6-Dinitro-2-methylphenol	15.87	198	33634	21.991	ng/uL	99
65) N-Nitrosodiphenylamine	15.99	169	141385	22.005	ng/uL	96
66) 4-Bromophenyl-phenylether	16.67	248	62248	21.037	ng/uL	96
67) Hexachlorobenzene	16.79	284	66245	21.121	ng/uL	99
68) Atrazine	16.94	200	62457	21.738	ng/uL	100
69) Pentachlorophenol	17.14	266	37873	21.625	ng/uL	93
70) Phenanthrene	17.53	178	268793	21.371	ng/uL	96
72) Anthracene	17.62	178	279845	22.057	ng/uL	99
73) 1,2,3,4-Tetrachlorobenzene	13.54	216	83101	22.217	ng/uL	96
74) Pentachlorobenzene	15.05	250	77854	21.228	ng/uL	95
75) Carbazole	17.90	167	250441	23.603	ng/uL	98
76) Di-n-butylphthalate	18.43	149	294436	22.749	ng/uL	99
77) Fluoranthene	19.53	202	354837	23.138	ng/uL	98
80) Pyrene	19.89	202	360737	20.392	ng/uL	98
81) Butylbenzylphthalate	20.76	149	138134	22.315	ng/uL	98
82) 3,3'-Dichlorobenzidine	21.66	252	139804	23.999	ng/uL	96
83) Benzo(a)anthracene	21.74	228	382058	21.478	ng/uL	97
84) Bis(2-ethylhexyl)phthalate	21.63	149	197210	21.941	ng/uL	98
85) Chrysene	21.81	228	368311	21.665	ng/uL	98
87) Di-n-octyl phthalate	22.86	149	335755	22.846	ng/uL	100
88) Benzo(b)fluoranthene	24.00	252	382164	21.264	ng/uL	99
89) Benzo(k)fluoranthene	24.07	252	369462	20.990	ng/uL	95
91) Benzo(a)pyrene	24.89	252	336812	21.299	ng/uL#	99
92) Indeno(1,2,3-cd)pyrene	28.80	276	424404	20.979	ng/uL	99
93) Dibenzo(a,h)anthracene	28.87	278	359602	21.257	ng/uL	96
94) Benzo(a,h,i)perylene	29.98	276	352073m >	20.928	ng/uL >	02/22/21 JU

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021921\
Data File : BG048238.D
Acq On : 20 Feb 2021 15:58
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTD02042

Manual Integrations
APPROVED

mohammad
2/22/2021 2:09:05 PM

Quant Time: Feb 21 08:42:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 21 00:21:40 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed