

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
 Data File : BG048239.D
 Acq On : 20 Feb 2021 16:38
 Operator : CG/JU
 Sample : PB134730BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.432	14	16	19	rVB3	1704	1973	0.15%	0.015%
2	3.479	23	24	26	rVV2	1955	1515	0.12%	0.011%
3	3.514	26	30	33	rVV	10968	16257	1.24%	0.123%
4	3.561	37	38	44	rBV4	1532	2313	0.18%	0.018%
5	3.784	72	76	78	rBV3	2004	2245	0.17%	0.017%
6	3.896	91	95	96	rBV2	1073	1576	0.12%	0.012%
7	4.137	131	136	137	rBV2	1235	1955	0.15%	0.015%
8	4.260	154	157	160	rBV3	2522	3746	0.29%	0.028%
9	4.336	167	170	174	rVB3	1024	1634	0.12%	0.012%
10	4.724	234	236	239	rVB2	1924	1671	0.13%	0.013%
11	4.765	239	243	246	rBV3	1335	1902	0.14%	0.014%
12	6.839	594	596	601	rBV	1420	1641	0.13%	0.012%
13	7.292	664	673	684	rBV	194706	349927	26.67%	2.649%
14	7.433	691	697	708	rBV	131287	218911	16.68%	1.657%
15	7.650	728	734	743	rVB	192940	329234	25.09%	2.493%
16	7.862	766	770	773	rVB2	1133	1420	0.11%	0.011%
17	7.961	781	787	788	rVB	1441	1607	0.12%	0.012%
18	8.108	805	812	821	rBV	147310	246442	18.78%	1.866%
19	8.837	927	936	946	rBV2	237384	416744	31.76%	3.155%
20	9.283	1003	1012	1020	rBV	175839	319205	24.32%	2.417%
21	10.006	1127	1135	1142	rBV	171568	307501	23.43%	2.328%
22	10.359	1191	1195	1199	rBV	1042	1473	0.11%	0.011%
23	10.558	1222	1229	1243	rVV	244637	446113	33.99%	3.378%
24	10.699	1252	1253	1257	rVB	1905	1436	0.11%	0.011%
25	10.923	1283	1291	1300	rBV	195120	348386	26.55%	2.638%
26	11.070	1307	1316	1326	rVV	218829	413265	31.49%	3.129%
27	11.146	1328	1329	1331	rBV	1852	1416	0.11%	0.011%
28	11.175	1333	1334	1338	rVB	1380	1427	0.11%	0.011%
29	11.816	1440	1443	1448	rVB	972	1568	0.12%	0.012%
30	12.509	1555	1561	1564	rBV3	3493	6256	0.48%	0.047%
31	13.020	1647	1648	1656	rVB	1380	1892	0.14%	0.014%
32	13.379	1705	1709	1712	rVB	1418	1486	0.11%	0.011%
33	13.708	1763	1765	1769	rVB2	2083	2041	0.16%	0.015%
34	14.137	1831	1838	1848	rBV	466716	696515	53.08%	5.273%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
 Data File : BG048239.D
 Acq On : 20 Feb 2021 16:38
 Operator : CG/JU
 Sample : PB134730BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

35	14.383	1875	1880	1882	rBV	1410	2919	0.22%	0.022%
36	14.430	1882	1888	1900	rVV	485516	778898	59.35%	5.897%
37	14.507	1900	1901	1908	rVB2	1125	1853	0.14%	0.014%
38	14.736	1933	1940	1947	rBV2	338951	521633	39.75%	3.949%
39	14.783	1947	1948	1951	rVV2	2101	1508	0.11%	0.011%
40	14.877	1960	1964	1968	rBV2	1900	2999	0.23%	0.023%
41	14.977	1974	1981	1998	rVV	217438	384334	29.29%	2.910%
42	15.177	2013	2015	2017	rBV2	1618	1440	0.11%	0.011%
43	15.306	2036	2037	2042	rVB	1960	1990	0.15%	0.015%
44	15.359	2045	2046	2048	rBV	1764	1474	0.11%	0.011%
45	15.441	2059	2060	2063	rBV	1323	1509	0.11%	0.011%
46	15.535	2074	2076	2079	rBV3	1452	2023	0.15%	0.015%
47	15.729	2102	2109	2117	rBV	628854	973161	74.16%	7.368%
48	15.852	2124	2130	2144	rBV	247958	376762	28.71%	2.853%
49	15.964	2145	2149	2156	rVB2	8543	12439	0.95%	0.094%
50	16.105	2169	2173	2174	rVB	2114	2288	0.17%	0.017%
51	16.117	2174	2175	2178	rBV3	2072	1794	0.14%	0.014%
52	16.181	2185	2186	2190	rVB3	1643	1698	0.13%	0.013%
53	16.246	2195	2197	2198	rBV	2306	1577	0.12%	0.012%
54	16.293	2202	2205	2208	rBV4	1812	1610	0.12%	0.012%
55	16.405	2222	2224	2226	rBV2	1963	1700	0.13%	0.013%
56	16.428	2226	2228	2230	rVB3	2144	1568	0.12%	0.012%
57	16.481	2235	2237	2238	rBV2	2391	1466	0.11%	0.011%
58	16.504	2238	2241	2246	rVB4	4499	6283	0.48%	0.048%
59	16.616	2258	2260	2262	rVB	3631	2301	0.18%	0.017%
60	16.687	2269	2272	2274	rBV2	2504	2220	0.17%	0.017%
61	16.751	2279	2283	2285	rBV2	2418	2939	0.22%	0.022%
62	16.781	2285	2288	2291	rVB4	2650	3647	0.28%	0.028%
63	16.839	2296	2298	2301	rVB3	2033	1642	0.13%	0.012%
64	16.875	2303	2304	2307	rVV3	3051	2549	0.19%	0.019%
65	16.910	2307	2310	2313	rVV4	2177	2523	0.19%	0.019%
66	16.951	2313	2317	2319	rVV4	3011	3915	0.30%	0.030%
67	17.004	2322	2326	2327	rVV2	1731	2084	0.16%	0.016%
68	17.033	2327	2331	2332	rVV3	3040	3551	0.27%	0.027%
69	17.104	2339	2343	2346	rVB5	4227	5638	0.43%	0.043%
70	17.321	2378	2380	2383	rBV3	3312	3776	0.29%	0.029%
71	17.480	2400	2407	2418	rVV	439442	670699	51.11%	5.078%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
 Data File : BG048239.D
 Acq On : 20 Feb 2021 16:38
 Operator : CG/JU
 Sample : PB134730BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

72	17.580	2418	2424	2436	rVB	720117	1106597	84.33%	8.378%
73	17.674	2438	2440	2441	rVV2	4119	2342	0.18%	0.018%
74	17.697	2442	2444	2447	rVV3	3342	3335	0.25%	0.025%
75	17.727	2447	2449	2450	rVV2	3299	2105	0.16%	0.016%
76	17.762	2453	2455	2456	rBV2	3282	1635	0.12%	0.012%
77	17.832	2466	2467	2469	rBV2	2324	2068	0.16%	0.016%
78	17.950	2485	2487	2490	rVB3	3296	2340	0.18%	0.018%
79	18.014	2497	2498	2500	rVB2	4453	1635	0.12%	0.012%
80	18.050	2502	2504	2506	rVB3	4780	2320	0.18%	0.018%
81	18.073	2506	2508	2510	rBV2	2738	3038	0.23%	0.023%
82	18.150	2520	2521	2524	rBV3	4354	3433	0.26%	0.026%
83	18.208	2528	2531	2532	rBV3	3318	3115	0.24%	0.024%
84	18.273	2541	2542	2543	rBV	5368	2036	0.16%	0.015%
85	18.296	2543	2546	2548	rVV4	4771	5775	0.44%	0.044%
86	18.332	2550	2552	2553	rVV2	2961	2647	0.20%	0.020%
87	18.361	2556	2557	2558	rBV	3524	1606	0.12%	0.012%
88	18.379	2558	2560	2561	rBV2	4947	3436	0.26%	0.026%
89	18.408	2563	2565	2567	rVB3	4380	3520	0.27%	0.027%
90	18.432	2567	2569	2573	rBV5	4675	7722	0.59%	0.058%
91	18.567	2591	2592	2596	rBV4	3678	4058	0.31%	0.031%
92	18.672	2608	2610	2611	rVB2	4809	2330	0.18%	0.018%
93	18.696	2611	2614	2615	rBV3	4538	4437	0.34%	0.034%
94	19.072	2676	2678	2679	rBV2	4169	2272	0.17%	0.017%
95	19.090	2679	2681	2683	rVV3	4656	3653	0.28%	0.028%
96	19.195	2697	2699	2700	rBV2	5026	4467	0.34%	0.034%
97	19.859	2806	2812	2818	rBV	906570	1312294	100.00%	9.936%
98	21.757	3129	3135	3143	rVB2	443684	714363	54.44%	5.409%
99	24.818	3647	3656	3665	rVB	457779	1226860	93.49%	9.289%
100	25.047	3685	3695	3704	rVB3	277924	827519	63.06%	6.265%


Sum of corrected areas: 13208061

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
Data File : BG048239.D
Acq On : 20 Feb 2021 16:38
Operator : CG/JU
Sample : PB134730BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK30

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

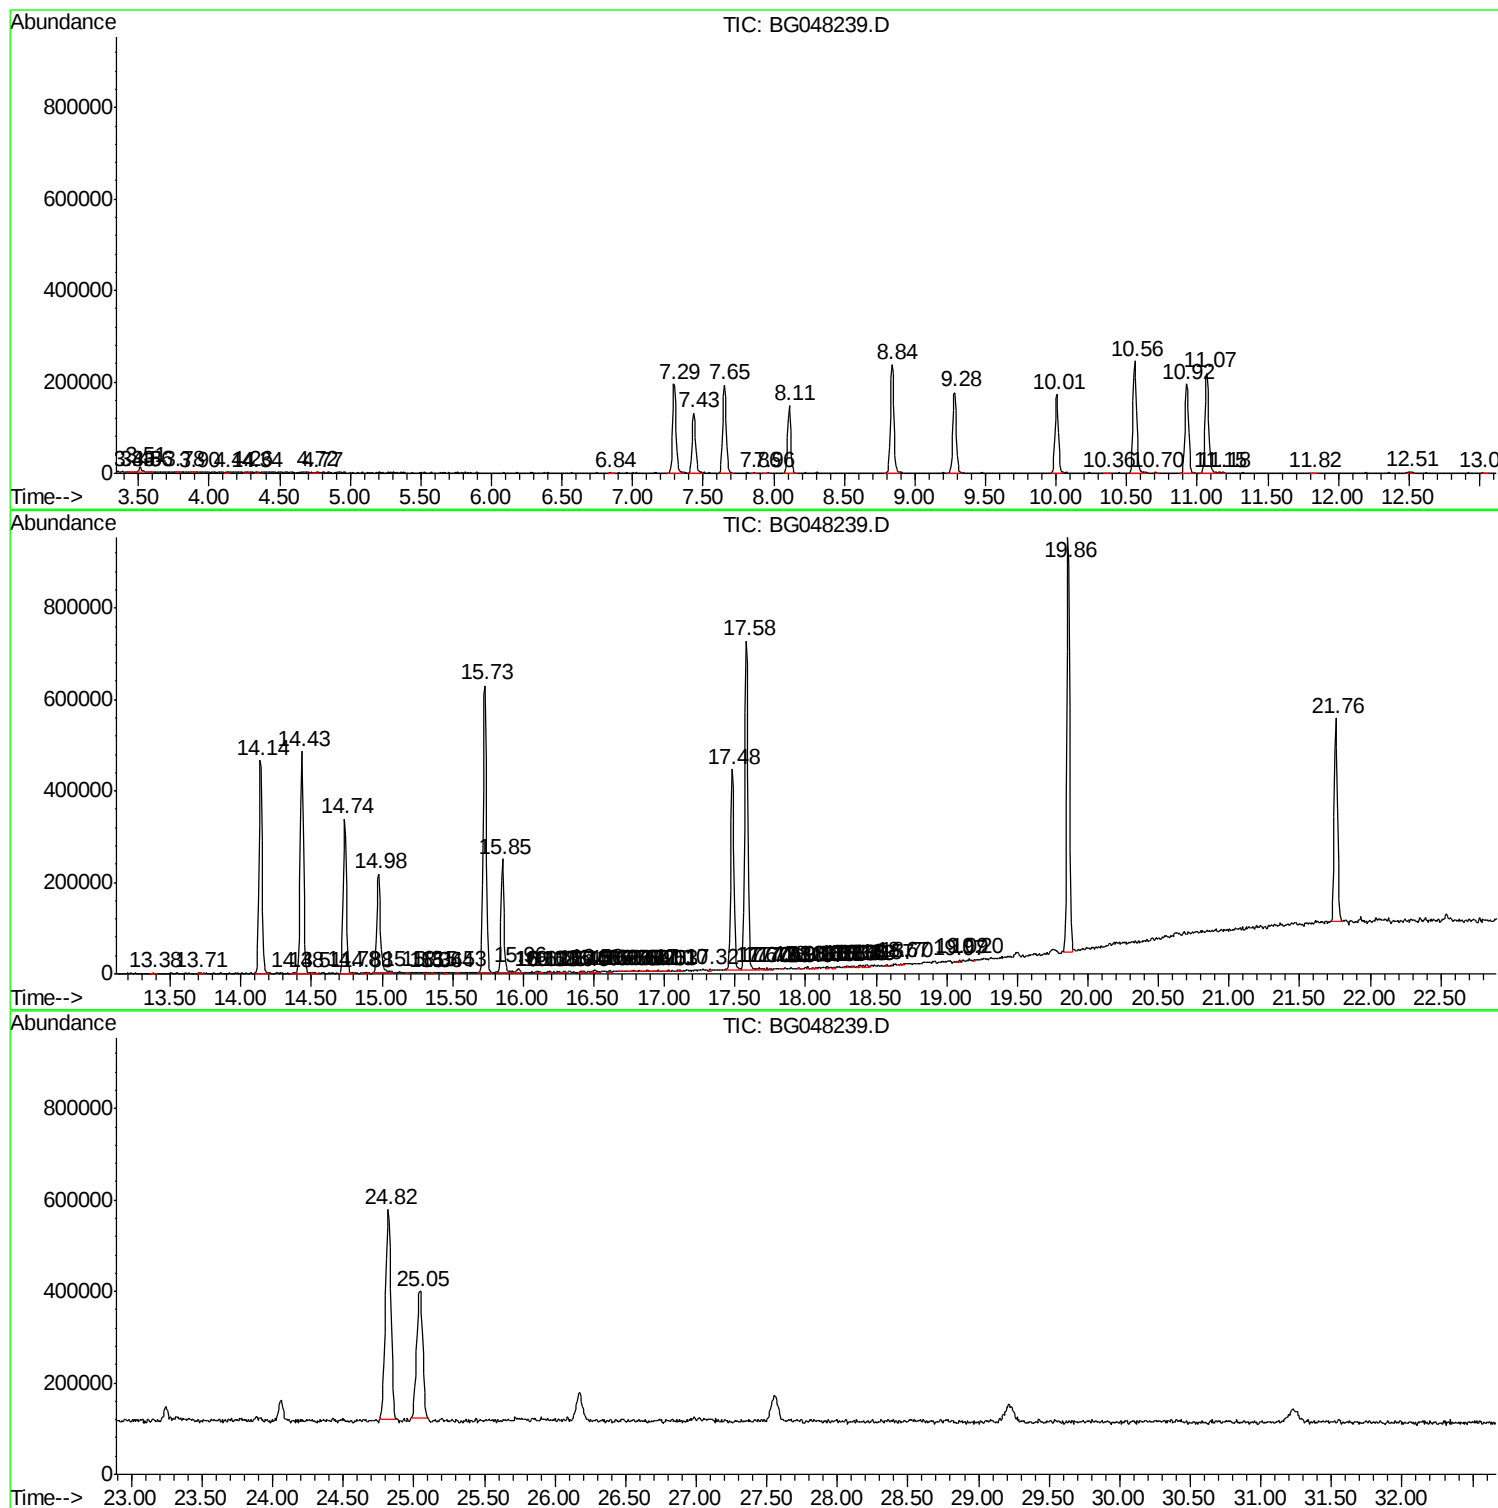

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021921\
Data File : BG048239.D
Acq On : 20 Feb 2021 16:38
Operator : CG/JU
Sample : PB134730BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK30

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021921\
Data File : BG048239.D
Acq On : 20 Feb 2021 16:38
Operator : CG/JU
Sample : PB134730BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK30

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc