

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
 Data File : BG048247.D
 Acq On : 20 Feb 2021 22:07
 Operator : CG/JU
 Sample : M1415-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBH14

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.520	29	31	37	rVB5	4539	4525	0.73%	0.079%
2	3.567	37	39	41	rVB2	1991	1363	0.22%	0.024%
3	3.761	70	72	75	rBV3	1403	1485	0.24%	0.026%
4	3.996	110	112	117	rBV	1628	3198	0.52%	0.056%
5	4.049	119	121	125	rVV3	1272	1637	0.26%	0.029%
6	4.166	137	141	143	rBV3	2516	2874	0.46%	0.050%
7	4.266	156	158	163	rVB2	3266	5271	0.85%	0.092%
8	4.354	171	173	176	rBV4	1264	1337	0.22%	0.023%
9	4.713	233	234	237	rBV	1539	1238	0.20%	0.022%
10	4.960	274	276	279	rBV3	1256	1509	0.24%	0.026%
11	5.054	289	292	295	rVB3	1413	1719	0.28%	0.030%
12	5.201	313	317	319	rBV4	2771	4413	0.71%	0.077%
13	5.958	445	446	449	rBV	1247	1231	0.20%	0.021%
14	6.029	455	458	459	rBV2	1605	1268	0.20%	0.022%
15	6.070	464	465	468	rBV2	1400	1656	0.27%	0.029%
16	6.152	476	479	481	rBV2	1527	1200	0.19%	0.021%
17	6.264	493	498	499	rVB	1277	1510	0.24%	0.026%
18	6.317	504	507	509	rVB	1428	1494	0.24%	0.026%
19	6.358	509	514	515	rBV3	1451	1891	0.30%	0.033%
20	6.564	548	549	552	rVB2	2013	1542	0.25%	0.027%
21	6.605	552	556	557	rBV	1112	1316	0.21%	0.023%
22	6.740	576	579	583	rVB3	1074	1671	0.27%	0.029%
23	7.040	628	630	632	rVB3	2076	1841	0.30%	0.032%
24	7.169	651	652	658	rVB	1225	1450	0.23%	0.025%
25	7.322	672	678	692	rVB2	77607	164160	26.45%	2.867%
26	7.445	692	699	708	rBV	54184	90275	14.55%	1.576%
27	7.662	730	736	748	rBV	76581	141509	22.80%	2.471%
28	7.839	765	766	769	rBV2	1484	1296	0.21%	0.023%
29	8.121	806	814	822	rBV	156647	275115	44.33%	4.804%
30	8.473	872	874	877	rBV	1092	1247	0.20%	0.022%
31	8.514	877	881	883	rVB2	1397	1432	0.23%	0.025%
32	8.544	885	886	892	rBV3	1005	1417	0.23%	0.025%
33	8.755	920	922	928	rBV3	1088	1892	0.30%	0.033%
34	8.861	934	940	950	rBV2	93076	169506	27.31%	2.960%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
 Data File : BG048247.D
 Acq On : 20 Feb 2021 22:07
 Operator : CG/JU
 Sample : M1415-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBH14

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

35	8.955	952	956	963	rVB6	2410	4826	0.78%	0.084%
36	9.290	1007	1013	1020	rBV	71685	133603	21.53%	2.333%
37	9.672	1073	1078	1080	rVB3	1616	2552	0.41%	0.045%
38	9.801	1097	1100	1103	rBV	987	1312	0.21%	0.023%
39	9.942	1122	1124	1126	rBV	1878	1357	0.22%	0.024%
40	10.013	1128	1136	1144	rBV2	69186	129081	20.80%	2.254%
41	10.436	1206	1208	1211	rVB2	1872	1641	0.26%	0.029%
42	10.577	1225	1232	1240	rBV	101763	183365	29.55%	3.202%
43	10.935	1285	1293	1300	rBV	210135	374715	60.38%	6.543%
44	10.982	1300	1301	1303	rBV2	2280	1402	0.23%	0.024%
45	11.088	1310	1319	1330	rBV2	75724	150653	24.27%	2.631%
46	11.199	1334	1338	1341	rBV2	1132	1726	0.28%	0.030%
47	11.464	1378	1383	1384	rBV	1162	1488	0.24%	0.026%
48	11.511	1388	1391	1395	rBV	928	1397	0.23%	0.024%
49	11.716	1423	1426	1429	rBV	1530	1863	0.30%	0.033%
50	11.975	1467	1470	1471	rBV	2013	1866	0.30%	0.033%
51	12.316	1525	1528	1530	rVB	2215	2018	0.33%	0.035%
52	12.521	1558	1563	1565	rBV4	1917	2927	0.47%	0.051%
53	12.551	1565	1568	1569	rBV	2587	1301	0.21%	0.023%
54	12.692	1591	1592	1596	rVB	1280	1331	0.21%	0.023%
55	12.892	1624	1626	1629	rVB	1625	1203	0.19%	0.021%
56	12.974	1638	1640	1643	rVB	1600	1536	0.25%	0.027%
57	13.080	1656	1658	1661	rBV2	1013	1295	0.21%	0.023%
58	13.244	1685	1686	1688	rBV2	1572	1339	0.22%	0.023%
59	13.285	1690	1693	1694	rBV3	1473	1456	0.23%	0.025%
60	13.344	1701	1703	1705	rBV2	2073	2016	0.32%	0.035%
61	13.491	1726	1728	1730	rBV2	1685	1584	0.26%	0.028%
62	13.532	1733	1735	1738	rBV3	1562	1465	0.24%	0.026%
63	13.626	1748	1751	1752	rBV2	2497	2510	0.40%	0.044%
64	13.661	1755	1757	1759	rVV3	1709	1790	0.29%	0.031%
65	13.679	1759	1760	1765	rVB3	2352	2150	0.35%	0.038%
66	13.755	1771	1773	1774	rBV	1856	1413	0.23%	0.025%
67	13.814	1781	1783	1784	rVB	2830	1908	0.31%	0.033%
68	13.832	1784	1786	1787	rBV2	2991	1787	0.29%	0.031%
69	13.849	1787	1789	1791	rVV2	1839	1915	0.31%	0.033%
70	13.879	1791	1794	1797	rVV2	1624	2695	0.43%	0.047%
71	14.043	1821	1822	1824	rBV	2057	1684	0.27%	0.029%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
 Data File : BG048247.D
 Acq On : 20 Feb 2021 22:07
 Operator : CG/JU
 Sample : M1415-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBH14

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

72	14.149	1831	1840	1845	rBV	177556	270284	43.55%	4.720%
73	14.196	1845	1848	1853	rVB	33572	48648	7.84%	0.850%
74	14.325	1867	1870	1872	rBV3	2319	2296	0.37%	0.040%
75	14.360	1872	1876	1877	rBV4	2204	2096	0.34%	0.037%
76	14.443	1884	1890	1902	rVB	191388	303268	48.87%	5.296%
77	14.525	1902	1904	1906	rBV2	3474	2081	0.34%	0.036%
78	14.578	1911	1913	1914	rBV2	2754	1741	0.28%	0.030%
79	14.672	1927	1929	1932	rBV4	3174	3608	0.58%	0.063%
80	14.748	1935	1942	1953	rVB2	324877	520399	83.85%	9.087%
81	15.013	1981	1987	1996	rBV	62950	112599	18.14%	1.966%
82	15.735	2105	2110	2117	rVB	246830	358175	57.71%	6.255%
83	15.870	2128	2133	2138	rVB	70617	97387	15.69%	1.701%
84	17.492	2404	2409	2416	rVB	390654	578623	93.23%	10.104%
85	17.592	2421	2426	2433	rVB	264461	394833	63.62%	6.895%
86	19.872	2809	2814	2819	rBV2	337050	483337	77.88%	8.440%
87	21.769	3133	3137	3145	rVB	380541	620615	100.00%	10.837%


Sum of corrected areas: 5726648

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
Data File : BG048247.D
Acq On : 20 Feb 2021 22:07
Operator : CG/JU
Sample : M1415-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBH14

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

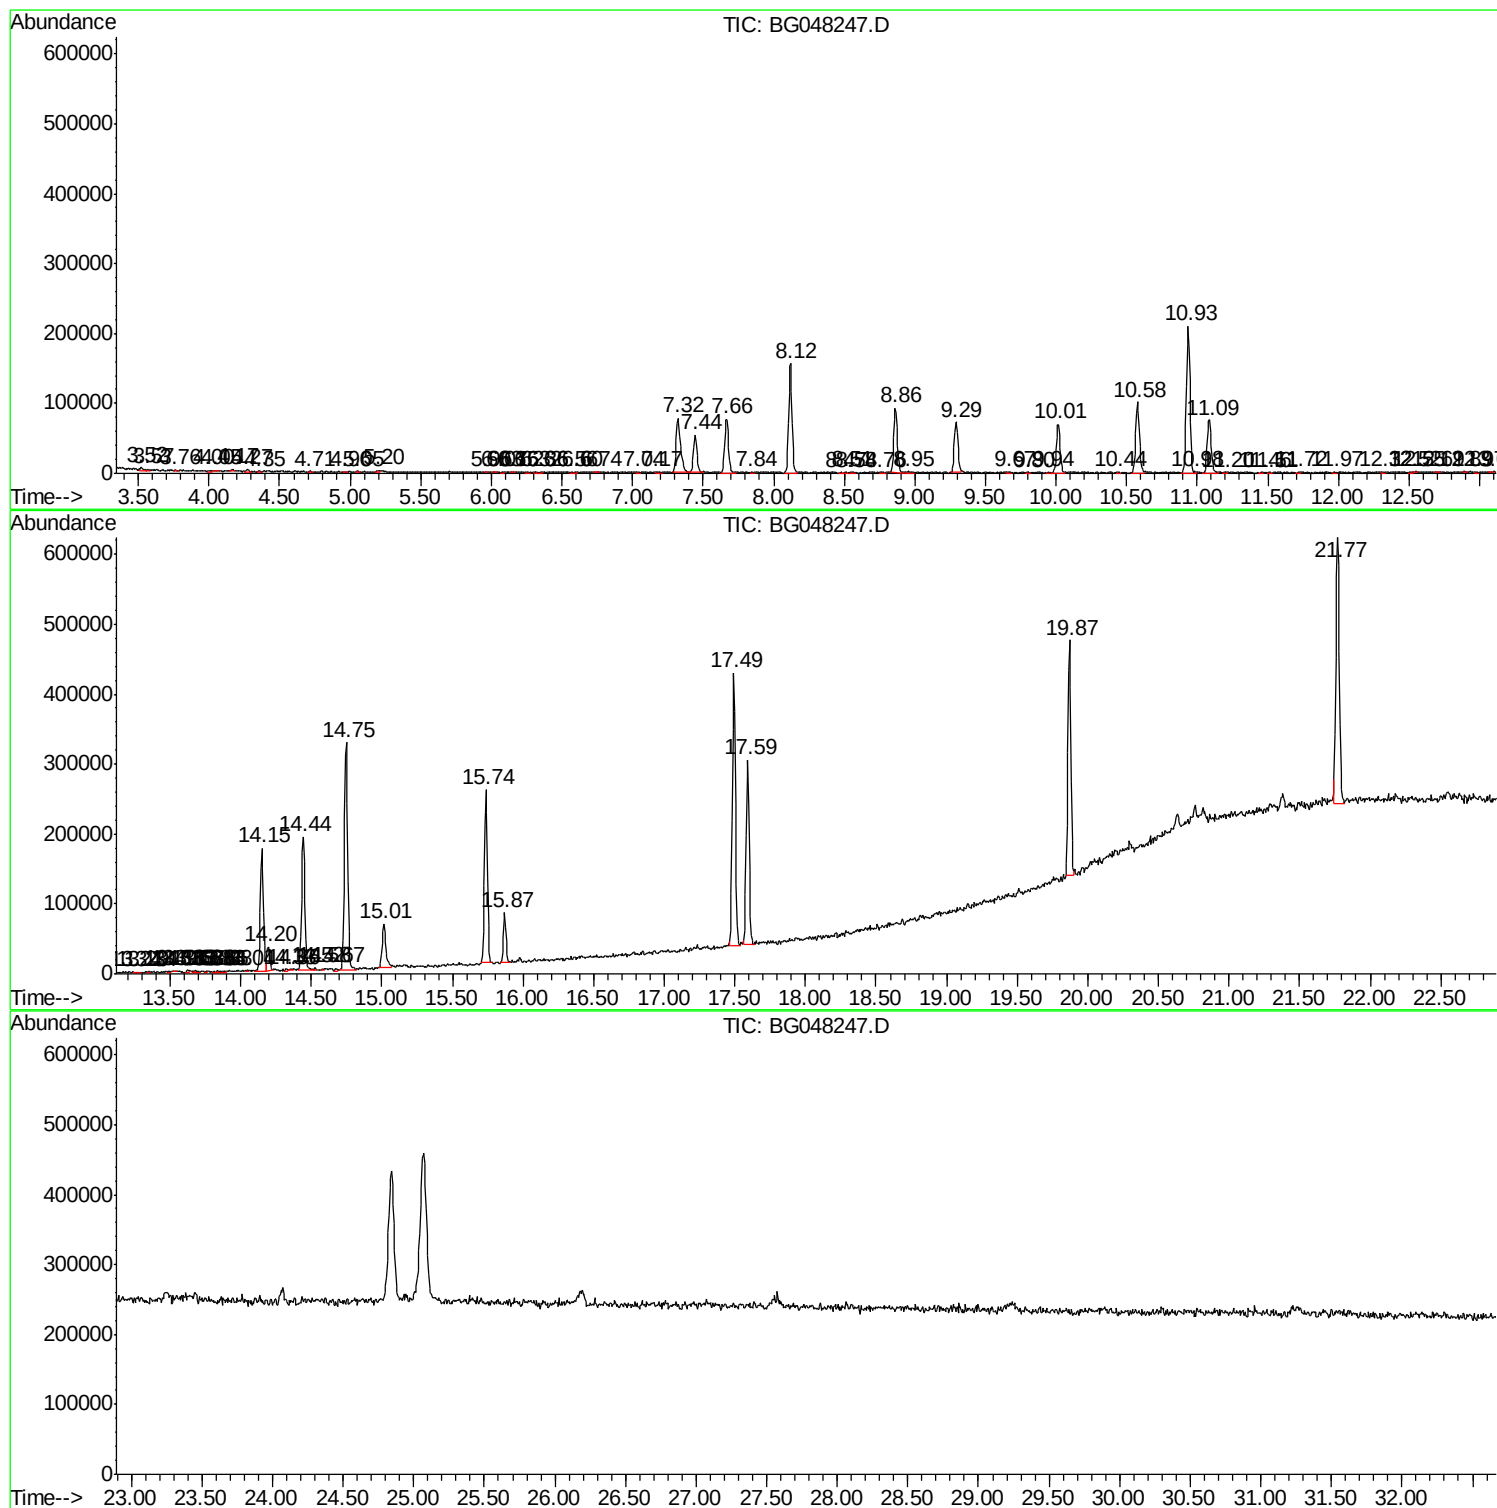

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021921\
Data File : BG048247.D
Acq On : 20 Feb 2021 22:07
Operator : CG/JU
Sample : M1415-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBH14

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021921\
Data File : BG048247.D
Acq On : 20 Feb 2021 22:07
Operator : CG/JU
Sample : M1415-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBH14

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc