

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
 Data File : BG048259.D
 Acq On : 21 Feb 2021 6:54
 Operator : CG/JU
 Sample : M1415-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBH26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.423	12	14	17	rVB3	2171	2092	0.26%	0.031%
2	3.511	26	29	34	rBV2	4350	6391	0.79%	0.094%
3	3.810	78	80	82	rBV2	1808	1206	0.15%	0.018%
4	4.040	117	119	121	rVB3	1769	1319	0.16%	0.019%
5	4.169	136	141	145	rVB3	3982	5513	0.69%	0.081%
6	4.269	153	158	161	rBV5	3232	4841	0.60%	0.071%
7	4.433	185	186	192	rBV4	1181	1987	0.25%	0.029%
8	4.604	213	215	217	rVB	1767	1159	0.14%	0.017%
9	4.645	219	222	224	rBV2	1367	1308	0.16%	0.019%
10	5.103	298	300	302	rVB2	1811	1325	0.16%	0.019%
11	5.185	308	314	316	rBV	2225	3323	0.41%	0.049%
12	5.309	334	335	339	rBV3	1456	1450	0.18%	0.021%
13	5.526	371	372	376	rVB	1443	1131	0.14%	0.017%
14	5.649	390	393	395	rVB2	1242	1329	0.17%	0.019%
15	5.679	395	398	402	rBV	1758	2617	0.33%	0.038%
16	5.820	420	422	425	rBV	1129	1249	0.16%	0.018%
17	5.861	425	429	432	rVB3	1240	2006	0.25%	0.029%
18	5.978	447	449	453	rBV2	1168	1524	0.19%	0.022%
19	6.319	504	507	508	rBV2	1255	1242	0.15%	0.018%
20	6.454	526	530	532	rBV2	1100	1328	0.17%	0.019%
21	6.619	555	558	561	rVB2	1290	1221	0.15%	0.018%
22	7.171	649	652	655	rVB2	1652	2044	0.25%	0.030%
23	7.312	669	676	689	rBV3	92379	190461	23.69%	2.789%
24	7.436	692	697	706	rVB	53064	94956	11.81%	1.390%
25	7.659	727	735	741	rBV	90362	150887	18.77%	2.209%
26	7.706	741	743	747	rVV4	3243	4354	0.54%	0.064%
27	7.759	750	752	754	rVB2	1235	1162	0.14%	0.017%
28	7.776	754	755	758	rBV2	1373	1229	0.15%	0.018%
29	8.111	806	812	820	rBV	166754	280000	34.82%	4.099%
30	8.640	900	902	905	rVB2	1111	1130	0.14%	0.017%
31	8.781	922	926	931	rVB2	1444	1653	0.21%	0.024%
32	8.852	931	938	948	rBV	100723	188175	23.40%	2.755%
33	9.098	976	980	983	rBV3	669	1143	0.14%	0.017%
34	9.286	1004	1012	1019	rBV2	79639	144794	18.01%	2.120%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
 Data File : BG048259.D
 Acq On : 21 Feb 2021 6:54
 Operator : CG/JU
 Sample : M1415-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBH26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

35	9.656	1069	1075	1080	rVB4	2747	4524	0.56%	0.066%
36	10.009	1127	1135	1143	rBV2	75033	140957	17.53%	2.064%
37	10.573	1223	1231	1240	rBV	102386	196931	24.49%	2.883%
38	10.673	1244	1248	1250	rVB3	1683	2103	0.26%	0.031%
39	10.732	1256	1258	1261	rVB	1473	1202	0.15%	0.018%
40	10.767	1261	1264	1266	rBV	1194	1272	0.16%	0.019%
41	10.931	1284	1292	1300	rBV	215947	385901	47.99%	5.650%
42	11.078	1310	1317	1328	rBV	88378	167607	20.85%	2.454%
43	11.184	1333	1335	1339	rVB2	1489	1246	0.15%	0.018%
44	11.302	1350	1355	1357	rVB	1248	1694	0.21%	0.025%
45	11.537	1392	1395	1396	rBV	1528	1639	0.20%	0.024%
46	11.566	1396	1400	1406	rVB2	820	1768	0.22%	0.026%
47	11.795	1433	1439	1443	rVB2	1084	1791	0.22%	0.026%
48	11.913	1457	1459	1462	rBV	1555	1906	0.24%	0.028%
49	12.024	1475	1478	1479	rBV	1260	1246	0.15%	0.018%
50	12.159	1497	1501	1502	rVB	1545	1595	0.20%	0.023%
51	12.183	1502	1505	1507	rBV	1050	1203	0.15%	0.018%
52	12.436	1544	1548	1555	rVB2	8249	13020	1.62%	0.191%
53	12.729	1594	1598	1599	rVB2	1135	1270	0.16%	0.019%
54	12.882	1620	1624	1627	rBV2	1040	1378	0.17%	0.020%
55	12.982	1640	1641	1644	rBV2	1685	1346	0.17%	0.020%
56	13.076	1652	1657	1658	rBV4	3438	4406	0.55%	0.065%
57	13.147	1664	1669	1673	rBV7	4436	9880	1.23%	0.145%
58	13.241	1683	1685	1688	rBV4	1367	1445	0.18%	0.021%
59	13.305	1694	1696	1700	rBV2	1981	2649	0.33%	0.039%
60	13.370	1706	1707	1711	rVB2	2111	1506	0.19%	0.022%
61	13.476	1723	1725	1728	rBV3	1416	1817	0.23%	0.027%
62	13.546	1736	1737	1738	rBV	2108	1381	0.17%	0.020%
63	13.587	1738	1744	1747	rVV4	7074	16212	2.02%	0.237%
64	13.687	1754	1761	1763	rBV7	7357	12736	1.58%	0.186%
65	13.816	1781	1783	1786	rBV4	4930	4363	0.54%	0.064%
66	14.139	1833	1838	1843	rBV	204354	313903	39.04%	4.596%
67	14.186	1843	1846	1852	rVB	39757	58213	7.24%	0.852%
68	14.292	1862	1864	1865	rVB2	2446	1176	0.15%	0.017%
69	14.304	1865	1866	1868	rBV	1692	1378	0.17%	0.020%
70	14.328	1868	1870	1871	rVB2	2680	1658	0.21%	0.024%
71	14.439	1883	1889	1896	rVB	228733	340401	42.34%	4.984%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
 Data File : BG048259.D
 Acq On : 21 Feb 2021 6:54
 Operator : CG/JU
 Sample : M1415-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBH26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

72	14.563	1908	1910	1911	rVB2	1994	1282	0.16%	0.019%
73	14.674	1926	1929	1930	rBV3	2185	2156	0.27%	0.032%
74	14.739	1933	1940	1948	rBV	357974	581621	72.34%	8.516%
75	14.921	1964	1971	1972	rBV2	20942	33897	4.22%	0.496%
76	15.009	1981	1986	1995	rVB3	71116	130857	16.27%	1.916%
77	15.732	2102	2109	2115	rBV	290130	444463	55.28%	6.507%
78	15.867	2127	2132	2140	rVB	100572	153085	19.04%	2.241%
79	15.967	2147	2149	2150	rBV2	4138	2238	0.28%	0.033%
80	16.249	2195	2197	2200	rBV3	2926	2825	0.35%	0.041%
81	16.296	2203	2205	2208	rVB4	3214	3040	0.38%	0.045%
82	17.488	2402	2408	2415	rVB	472514	716054	89.06%	10.484%
83	17.588	2419	2425	2431	rBV	334871	520827	64.78%	7.625%
84	19.868	2808	2813	2818	rVB	439060	621450	77.29%	9.099%
85	21.766	3131	3136	3144	rVB	475038	804046	100.00%	11.772%


Sum of corrected areas: 6830113

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021921\
Data File : BG048259.D
Acq On : 21 Feb 2021 6:54
Operator : CG/JU
Sample : M1415-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBH26

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

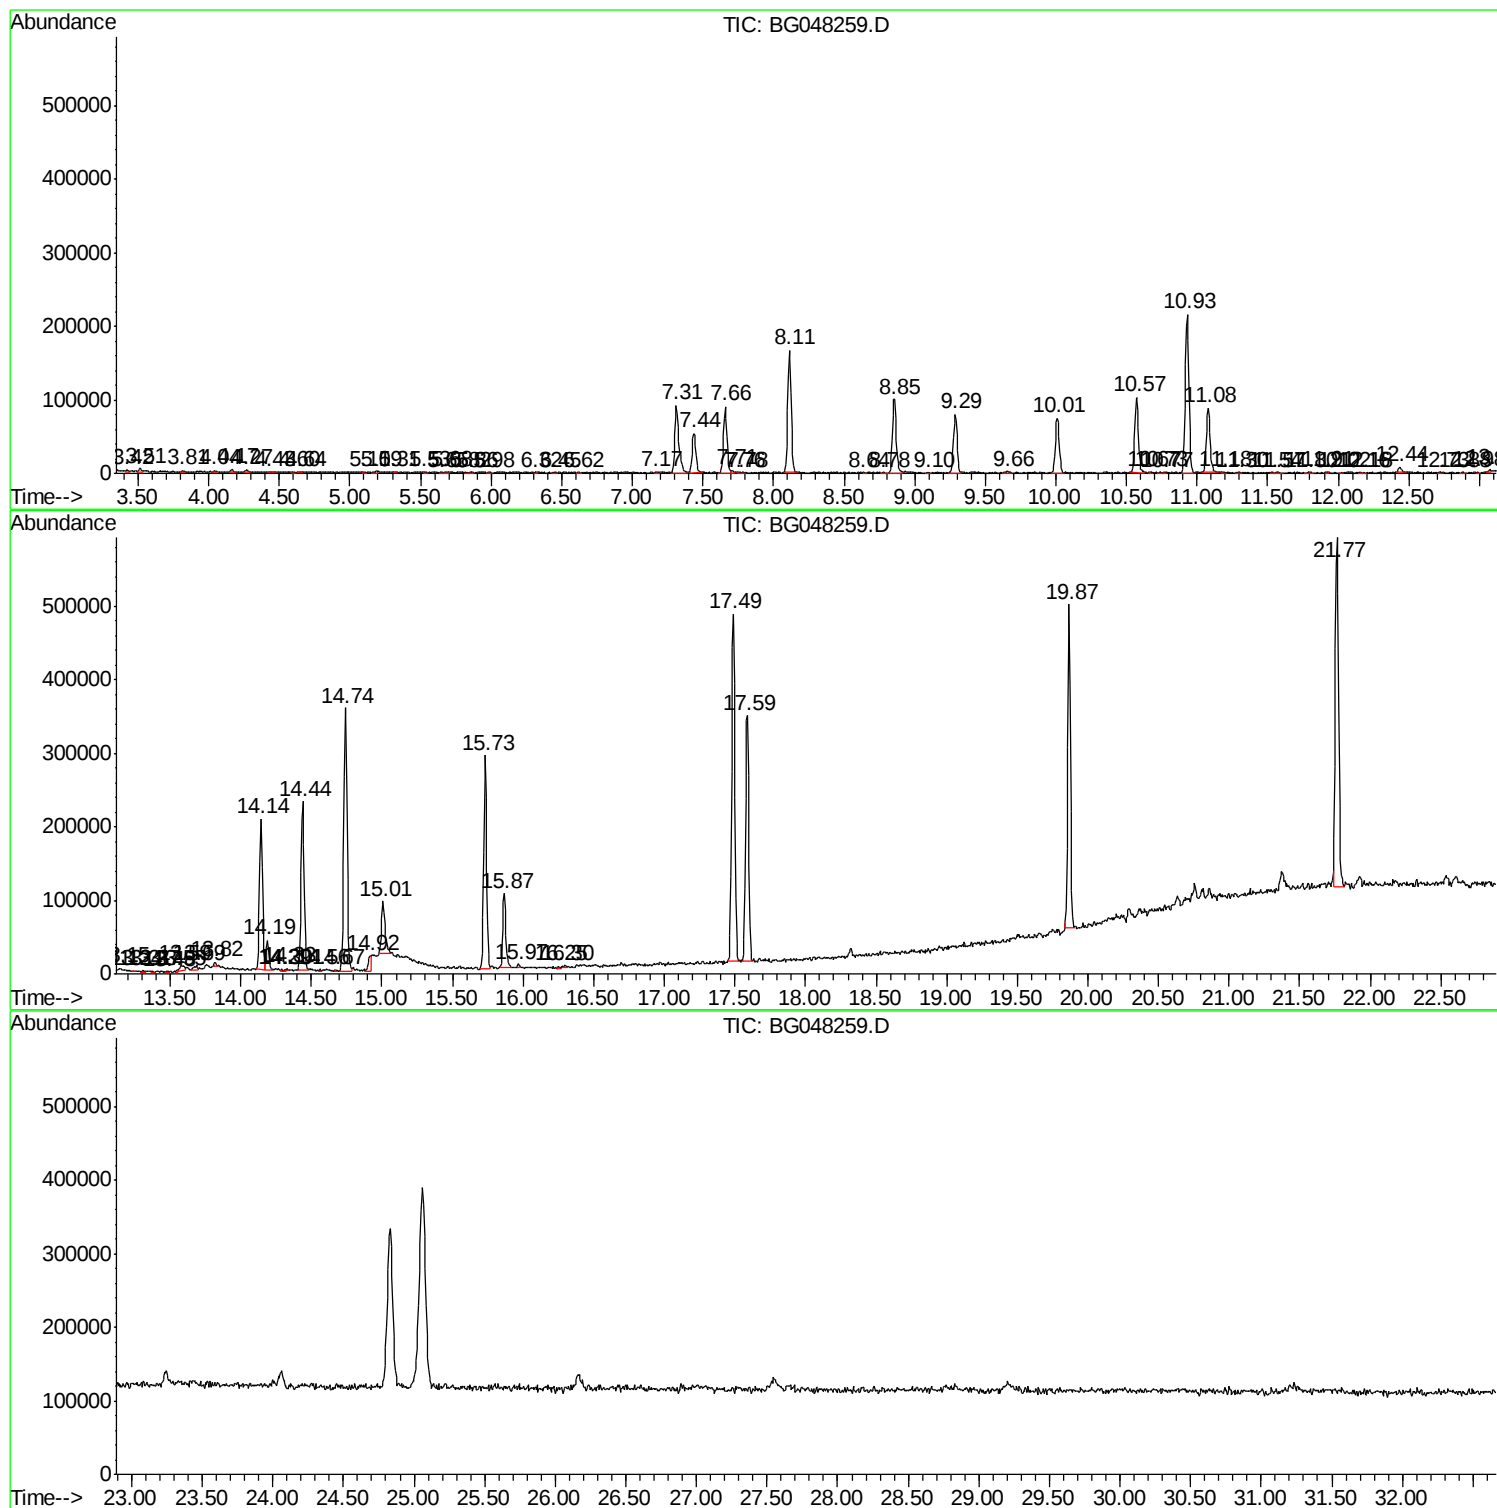

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021921\
Data File : BG048259.D
Acq On : 21 Feb 2021 6:54
Operator : CG/JU
Sample : M1415-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBH26

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021921\
Data File : BG048259.D
Acq On : 21 Feb 2021 6:54
Operator : CG/JU
Sample : M1415-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBH26

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc