

Data File : BG025892.D
Acq On : 21 Feb 2017 3:18
Operator : SJ/MA
Sample : I1898-23
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DABC6

Quant Time: Feb 21 04:01:53 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.3-EPA-BG021617MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 21 02:22:54 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	138452	20.00	ng/ul	0.00
2) Naphthalene-d8	10.88	136	677560	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.69	164	426885	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.41	188	953746	20.00	ng/ul	0.00
17) Chrysene-d12	21.67	240	926783	20.00	ng/ul	0.00
22) Perylene-d12	24.87	264	887946	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.38	160	945200	26.74	ng/ul	0.00
10) Fluorene-d10	15.67	176	694419	25.58	ng/ul	0.00
14) Anthracene-d10	17.51	188	1027831	23.84	ng/ul	0.00
18) Pyrene-d10	19.79	212	1056588	23.65	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.65	264	976658	24.85	ng/ul	0.00
Target Compounds						
16) Fluoranthene	19.45	202	111763	2.00	ng/ul	Qvalue 98
19) Pyrene	19.82	202	96377	1.72	ng/ul#	94
20) Benzo(a)anthracene	21.65	228	56594	1.09	ng/ul	97
21) Chrysene	21.65	228	56589	1.14	ng/ul	94
23) Benzo(b)fluoranthene	23.85	252	91740	1.79	ng/ul#	94
26) Benzo(a)pyrene	24.72	252	55396	1.12	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG025892.D

Acq On : 21 Feb 2017 3:18

Operator : SJ/MA

Sample : I1898-23

Misc :

ALS Vial : 26 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

DABC6


Quant Time: Feb 21 04:01:53 2017


Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.3-EPA-BG021617MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Feb 21 02:22:54 2017

Response via : Initial Calibration

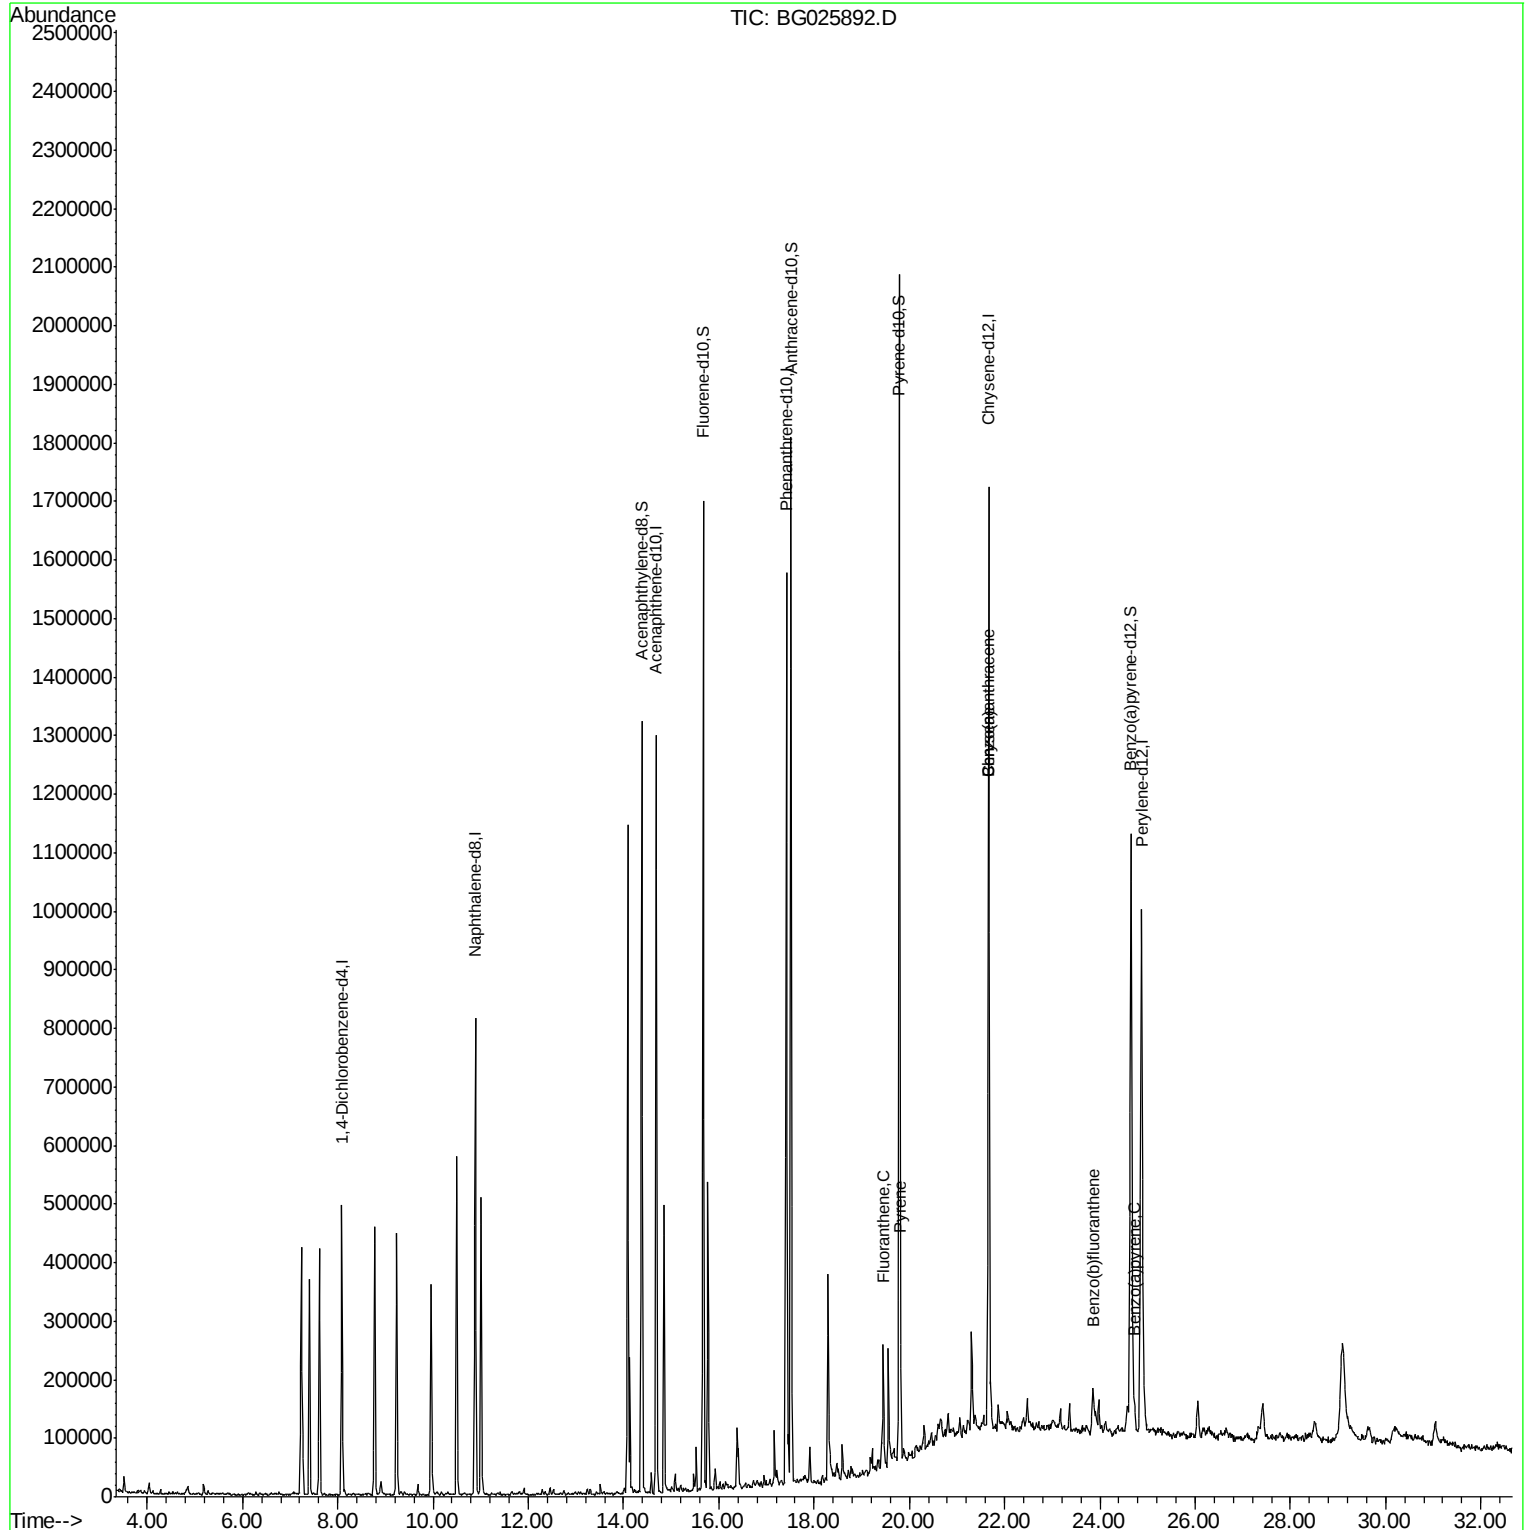


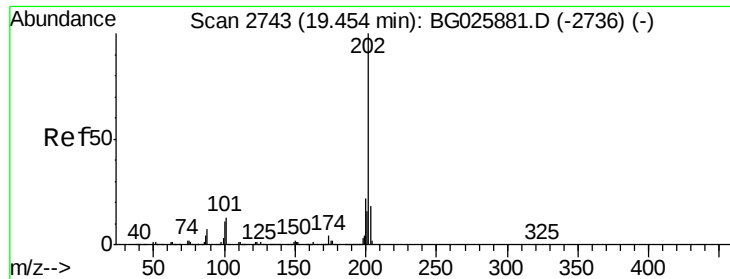




#16
Fluoranthene
 Concen: 2.00 ng/ul
 RT: 19.45 min Scan# 2742
 Delta R.T. -0.00 min
 Lab File: BG025892.D
 Acq: 21 Feb 2017 3:18

Instrument :
 BNA_G
 ClientSampleId :
 DABC6

Tgt Ion	Ratio	Lower	Upper
202	100		
101	13.4	9.9	14.9
100	9.8	7.4	11.0

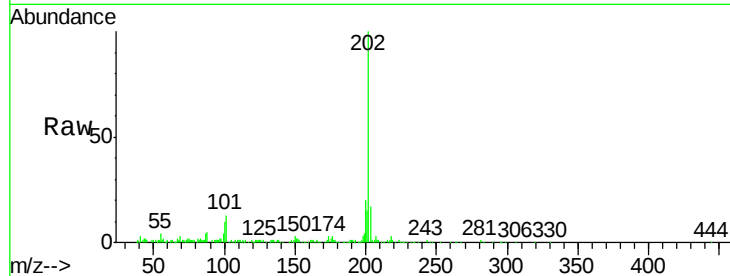


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

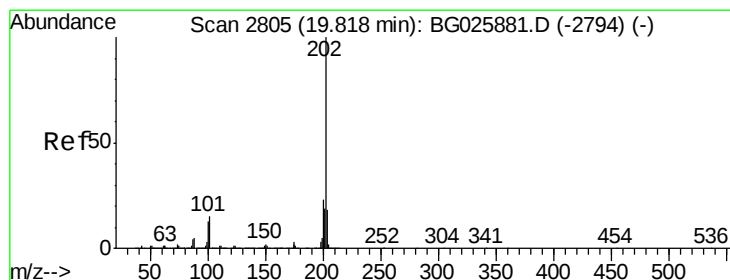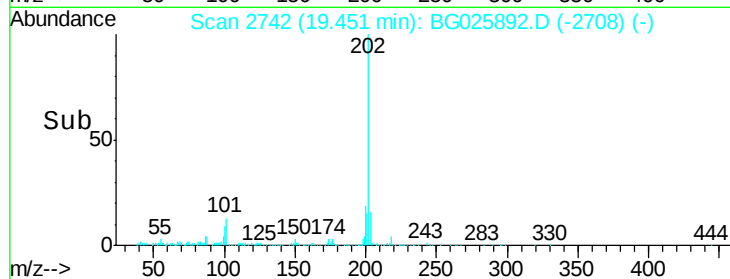
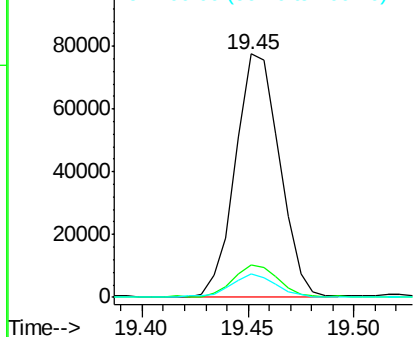



#19
Pyrene
 Concen: 1.72 ng/ul
 RT: 19.82 min Scan# 2804
 Delta R.T. -0.00 min
 Lab File: BG025892.D
 Acq: 21 Feb 2017 3:18

Tgt Ion	Ratio	Lower	Upper
202	100		
101	15.1	11.0	16.4
100	14.0	8.1	12.1

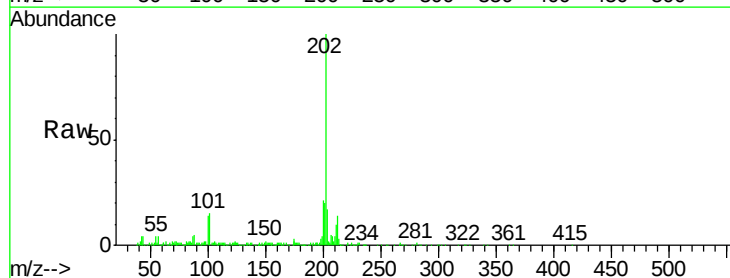

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

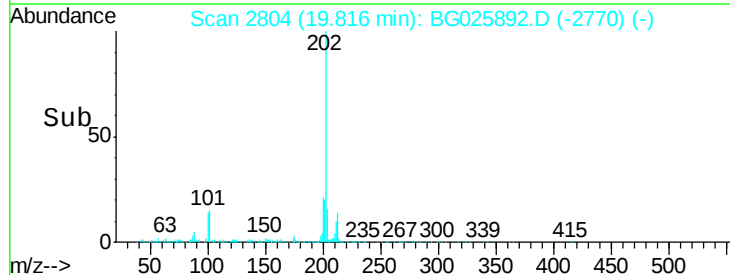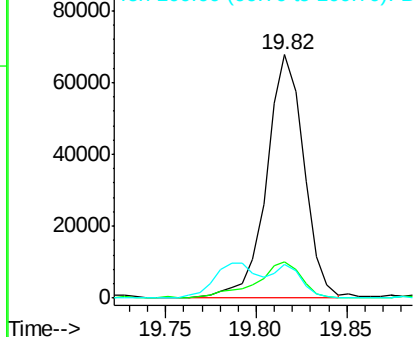

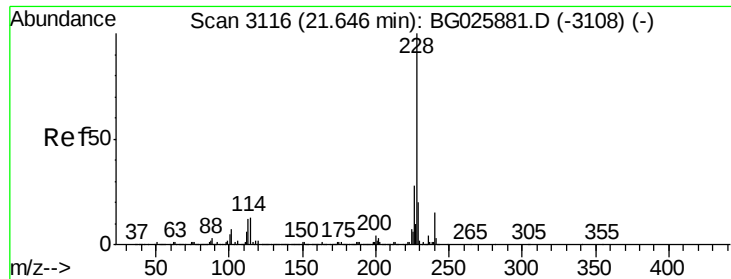

#20

Benzo(a)anthracene

Concen: 1.09 ng/ul

RT: 21.65 min Scan# 3116

Delta R.T. 0.00 min

Lab File: BG025892.D

Acq: 21 Feb 2017 3:18

Instrument :

BNA_G

ClientSampleId :

DABC6


Tgt Ion:228 Resp: 56594

Ion Ratio Lower Upper

228 100

229 22.0 15.7 23.5




226 26.8 21.1 31.7

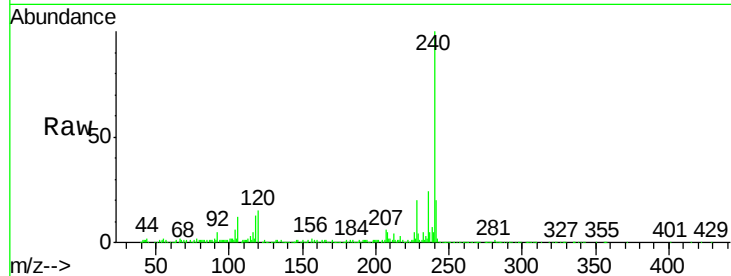

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

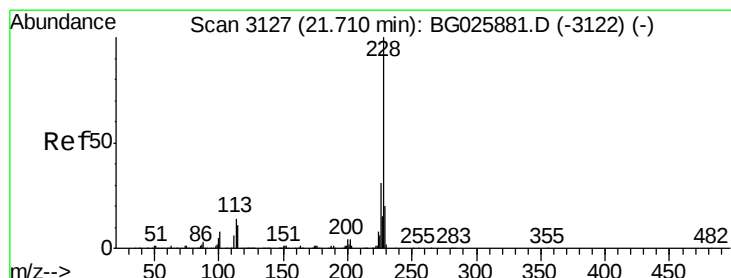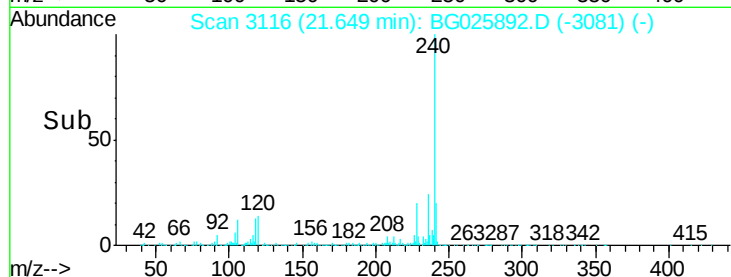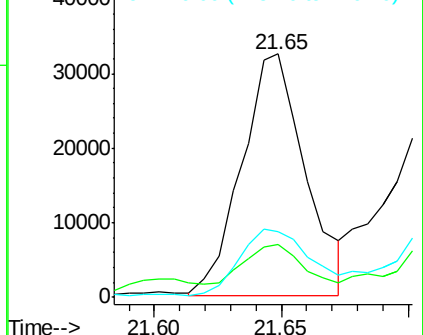

#21

Chrysene

Concen: 1.14 ng/ul

RT: 21.65 min Scan# 3116

Delta R.T. -0.06 min

Lab File: BG025892.D

Acq: 21 Feb 2017 3:18


Tgt Ion:228 Resp: 56589

Ion Ratio Lower Upper

228 100

226 26.8 24.5 36.7



229 22.0 15.8 23.8

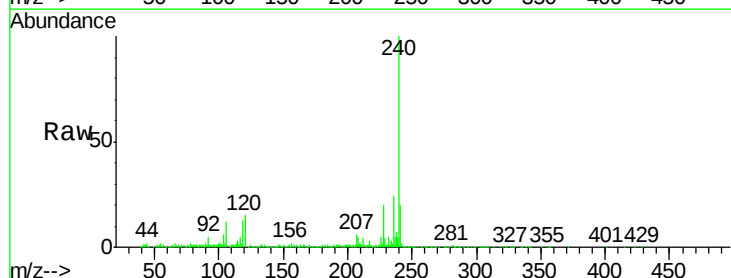


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

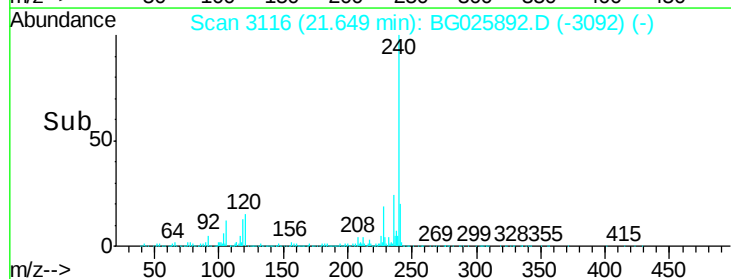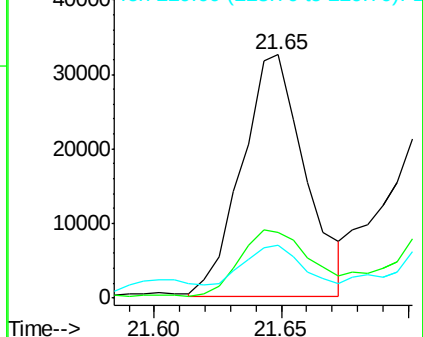

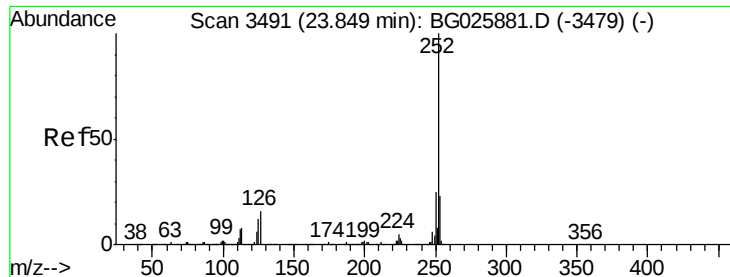

#23

Benzo(b)fluoranthene

Concen: 1.79 ng/ul

RT: 23.85 min Scan# 3491

Delta R.T. 0.00 min

Lab File: BG025892.D

Acq: 21 Feb 2017 3:18

Instrument :

BNA_G

ClientSampleId :

DABC6


Tgt Ion:252 Resp: 91740

Ion Ratio Lower Upper

252 100

253 21.0 18.0 27.0




125 14.7 8.0 12.0#

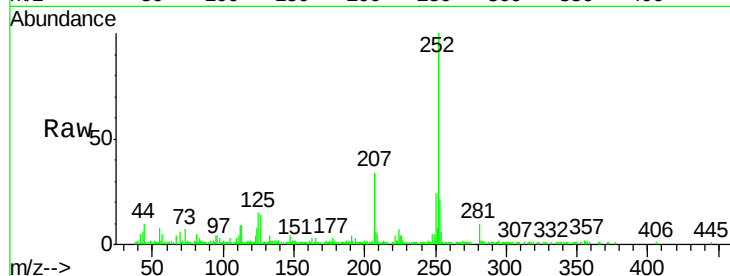

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

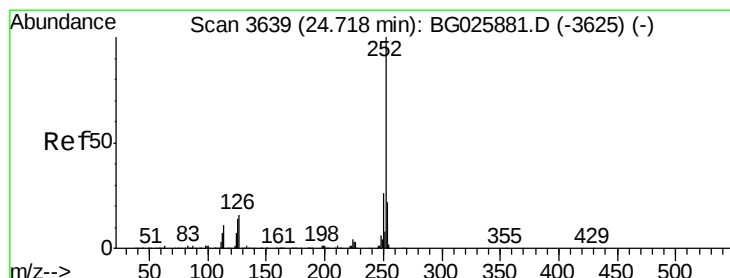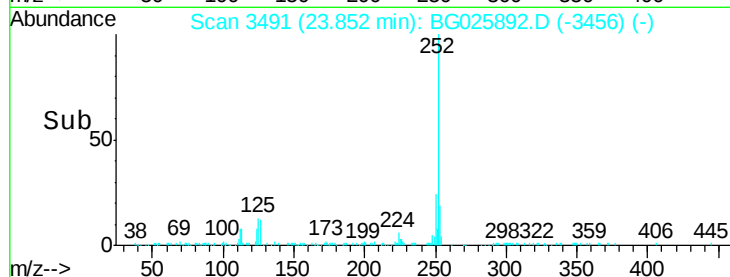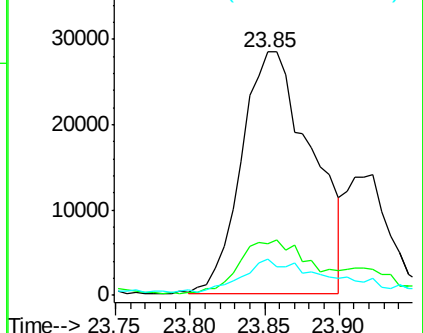

#26

Benzo(a)pyrene

Concen: 1.12 ng/ul

RT: 24.72 min Scan# 3639

Delta R.T. 0.00 min

Lab File: BG025892.D

Acq: 21 Feb 2017 3:18


Tgt Ion:252 Resp: 55396

Ion Ratio Lower Upper

252 100

253 29.3 17.2 25.8#

125 12.9 8.2 12.4#

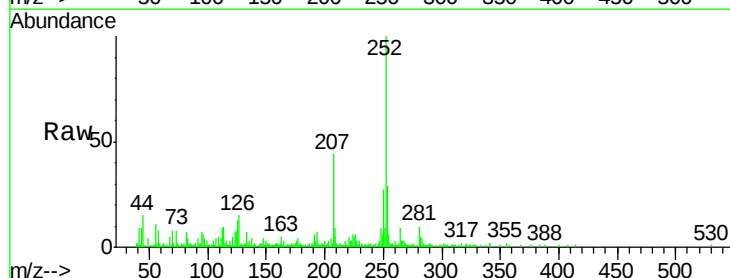

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

