

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022017\
 Data File : BG025889.D
 Acq On : 21 Feb 2017 1:20
 Operator : SJ/MA
 Sample : I1898-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DABB7

Manual Integrations
 APPROVED

mohammad
 2/21/2017 10:34:07 AM

Quant Time: Feb 21 02:53:48 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.3-EPA-BG021617MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 21 02:22:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	123232	20.00	ng/ul	0.00
2) Naphthalene-d8	10.88	136	602959	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.68	164	386676	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.42	188	875355	20.00	ng/ul	0.00
17) Chrysene-d12	21.66	240	818993	20.00	ng/ul	0.00
22) Perylene-d12	24.87	264	793828	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.38	160	907400	28.34	ng/ul	0.00
10) Fluorene-d10	15.67	176	673949	27.41	ng/ul	0.00
14) Anthracene-d10	17.52	188	984696	24.88	ng/ul	0.00
18) Pyrene-d10	19.79	212	994836	25.20	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.65	264	915702	26.07	ng/ul	0.00
Target Compounds						
13) Phenanthrene	17.46	178	70332	1.51	ng/ul	Qvalue 99
16) Fluoranthene	19.45	202	144792	2.82	ng/ul	99
19) Pyrene	19.81	202	114503	2.31	ng/ul#	97
20) Benzo(a)anthracene	21.65	228	64665	1.40	ng/ul	95
21) Chrysene	21.71	228	64789	1.47	ng/ul	95
23) Benzo(b)fluoranthene	23.86	252	78351m	1.71	ng/ul	
26) Benzo(a)pyrene	24.73	252	47673	1.07	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022017\
Data File : BG025889.D
Acq On : 21 Feb 2017 1:20
Operator : SJ/MA
Sample : I1898-14
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
DABB7

Manual Integrations
APPROVED

mohammad
2/21/2017 10:34:07 AM

Quant Time: Feb 21 02:53:48 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.3-EPA-BG021617MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 21 02:22:54 2017
Response via : Initial Calibration

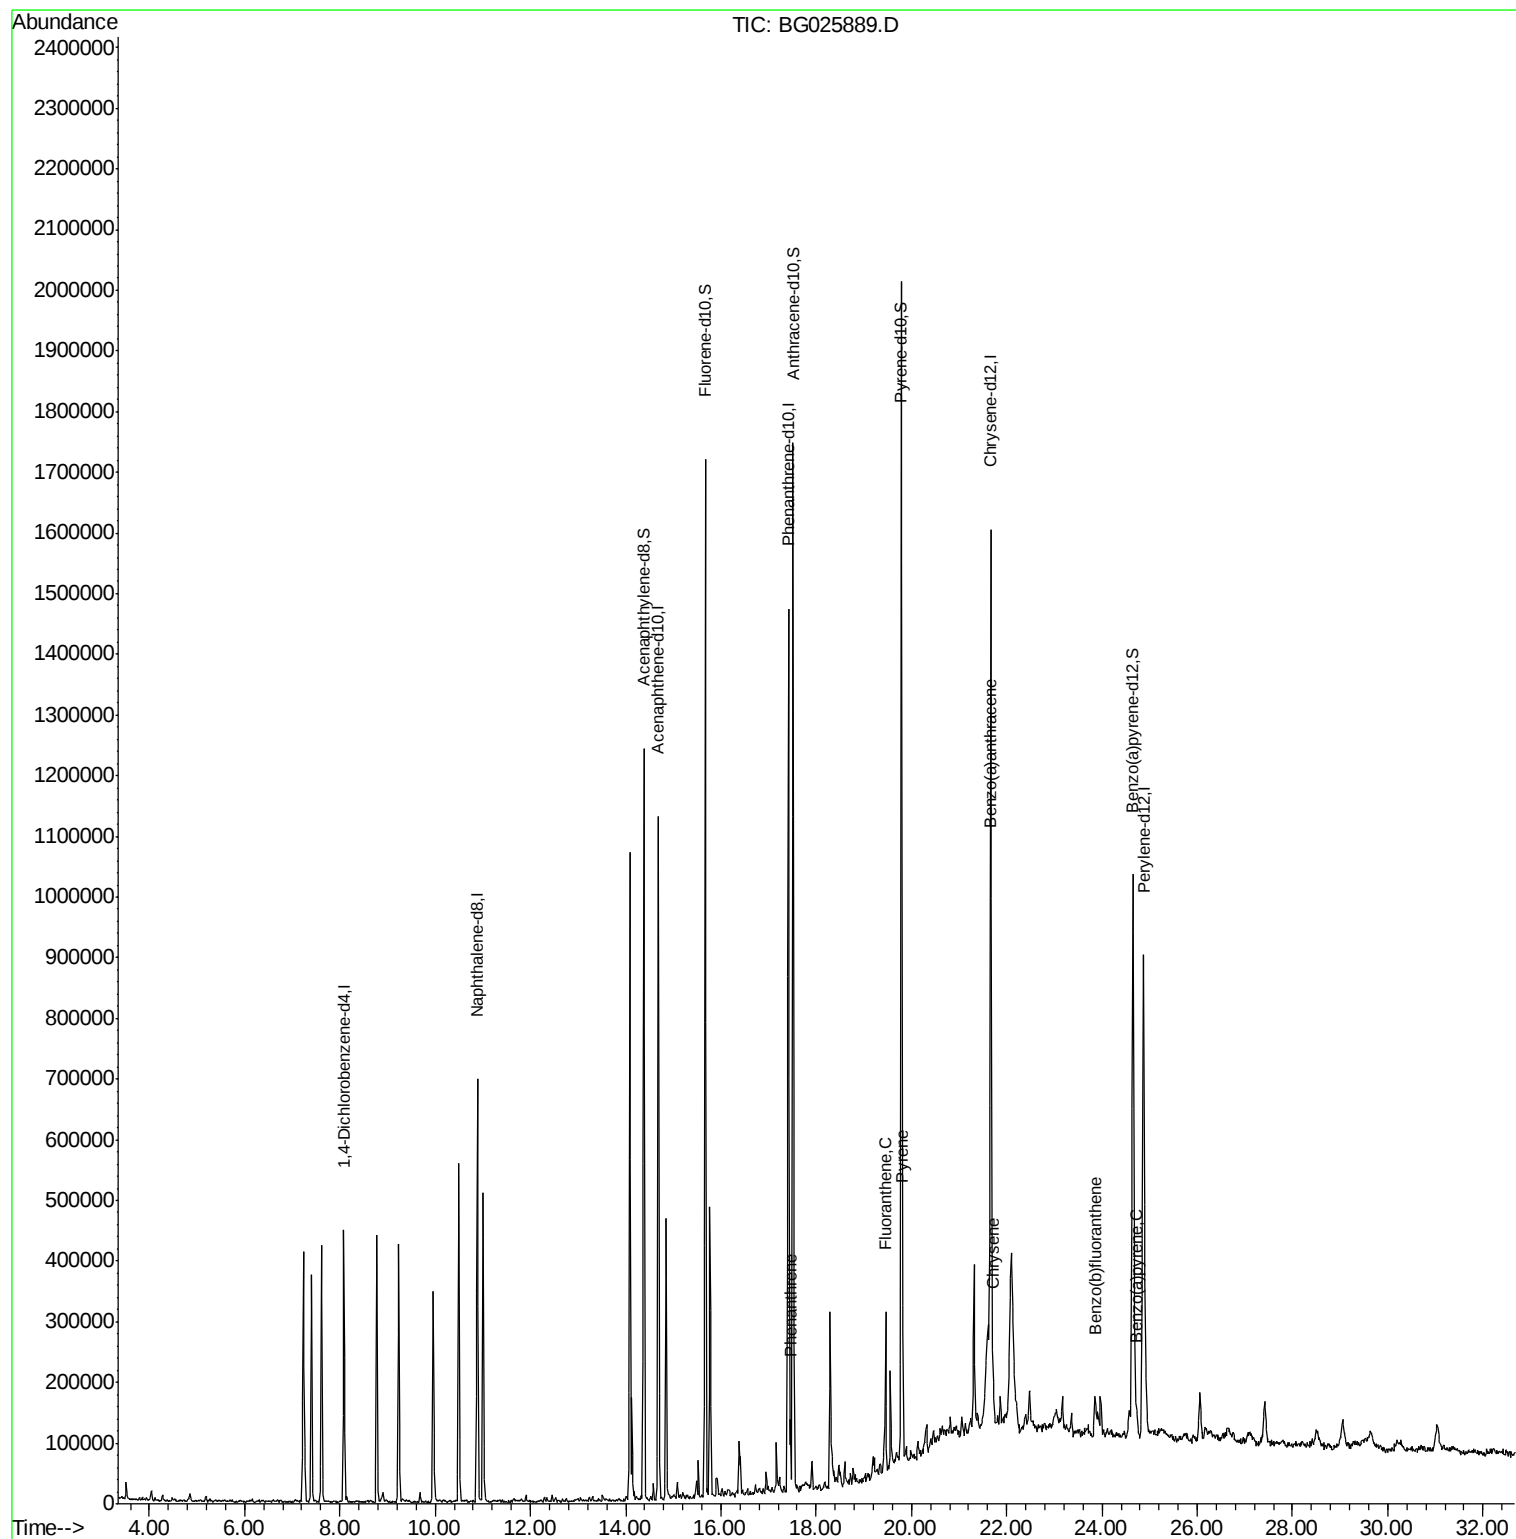

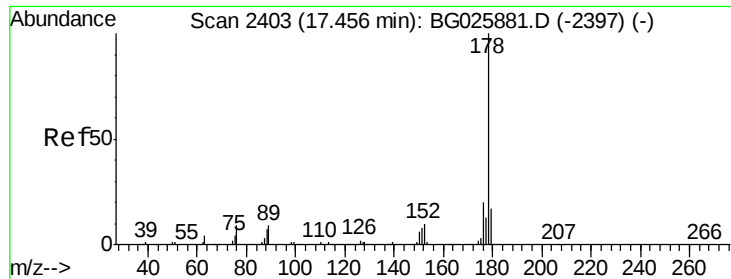

#13

Phenanthrene

Concen: 1.51 ng/ul

RT: 17.46 min Scan# 2403

Delta R.T. 0.00 min

Lab File: BG025889.D

Acq: 21 Feb 2017 1:20

Instrument :

BNA_G





ClientSampleId :

DABB7

Tgt Ion:	178	Resp:	70332
Ion Ratio	Lower	Upper	
178	100		
179	15.8	12.3	18.5
176	18.1	15.1	22.7

Manual Integrations
APPROVED

mohammad
2/21/2017 10:34:07 AM

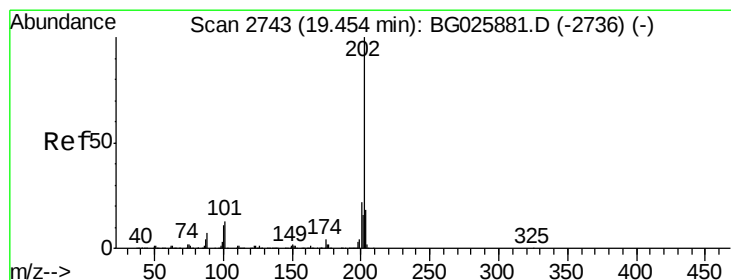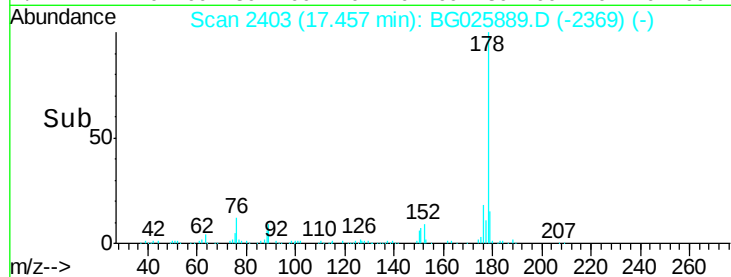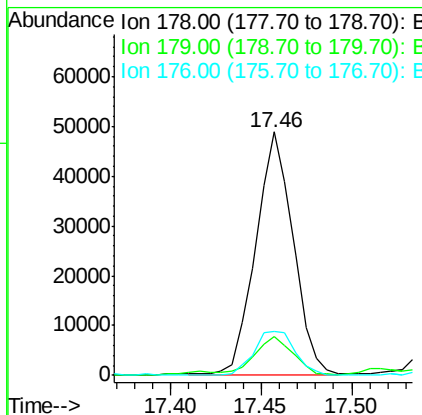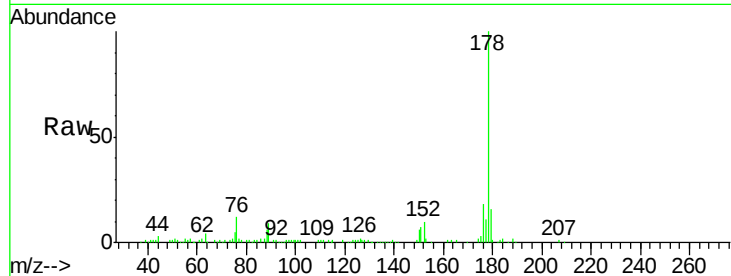

#16

Fluoranthene

Concen: 2.82 ng/ul




RT: 19.45 min Scan# 2743


Delta R.T. 0.00 min

Lab File: BG025889.D

Acq: 21 Feb 2017 1:20

Tgt Ion:	202	Resp:	144792
Ion Ratio	Lower	Upper	
202	100		
101	12.5	9.9	14.9
100	9.8	7.4	11.0

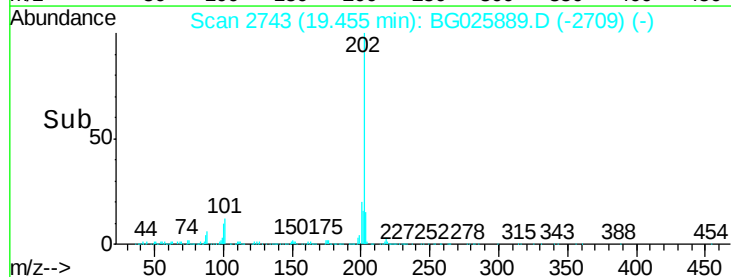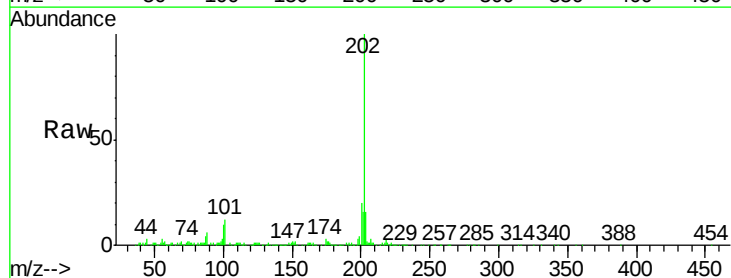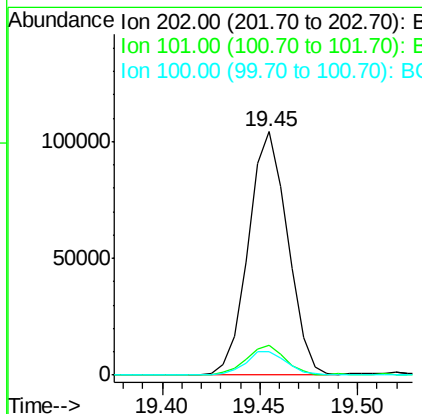

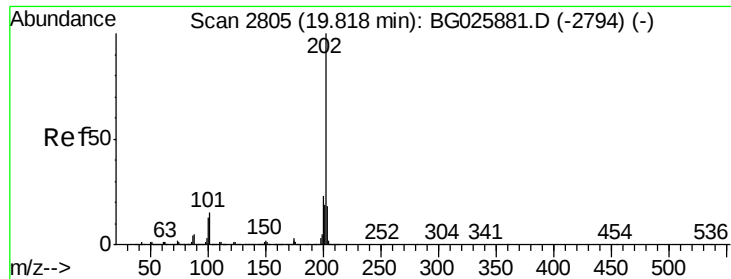





#19
Pyrene
Concen: 2.31 ng/ul
RT: 19.81 min Scan# 2804
Delta R.T. -0.01 min
Lab File: BG025889.D
Acq: 21 Feb 2017 1:20

Instrument :
BNA_G
ClientSampleId :
DABB7

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	13.8	11.0	16.4
100	12.5	8.1	12.1




Manual Integrations
APPROVED


mohammad
2/21/2017 10:34:07 AM

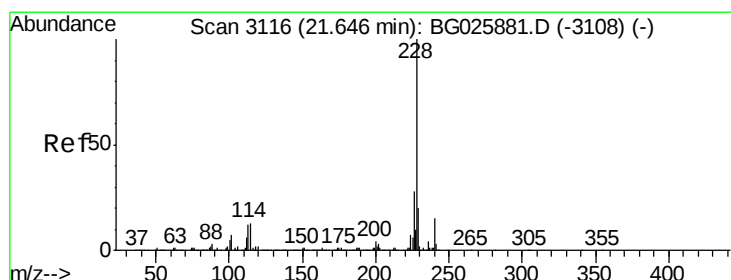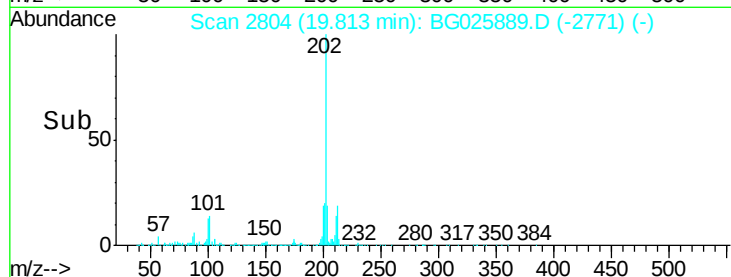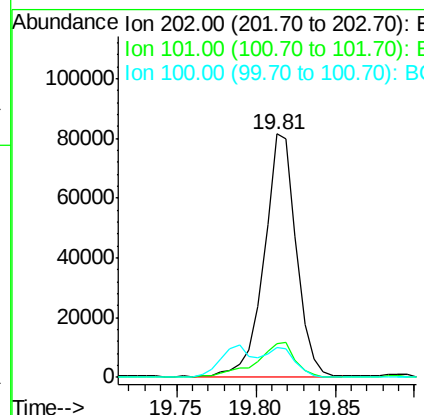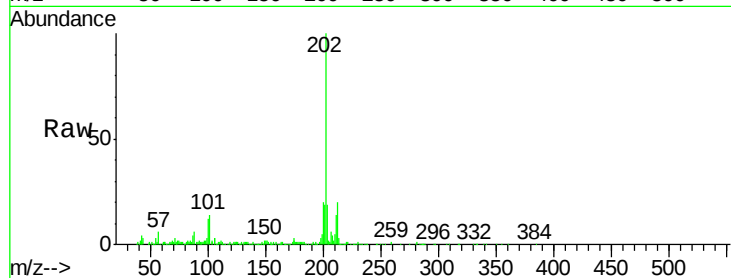

#20
Benzo(a)anthracene
Concen: 1.40 ng/ul
RT: 21.65 min Scan# 3116
Delta R.T. 0.00 min
Lab File: BG025889.D
Acq: 21 Feb 2017 1:20

Tgt Ion	Ratio	Resp Lower	Resp Upper
228	100		
229	21.0	15.7	23.5
226	29.7	21.1	31.7

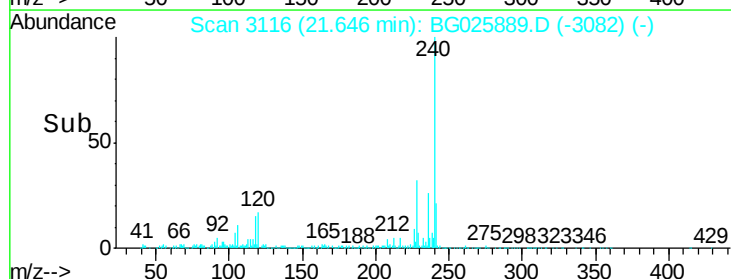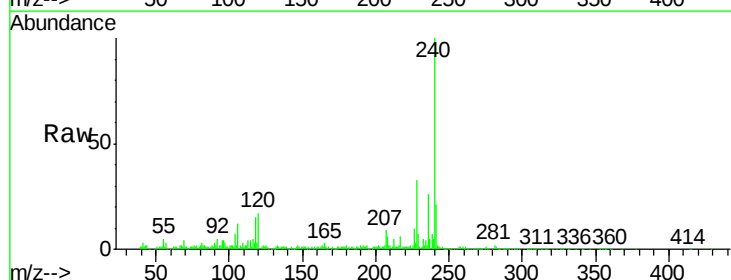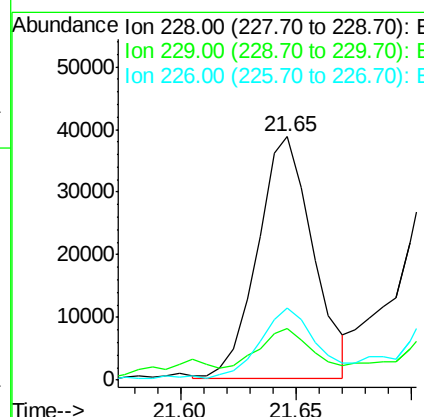

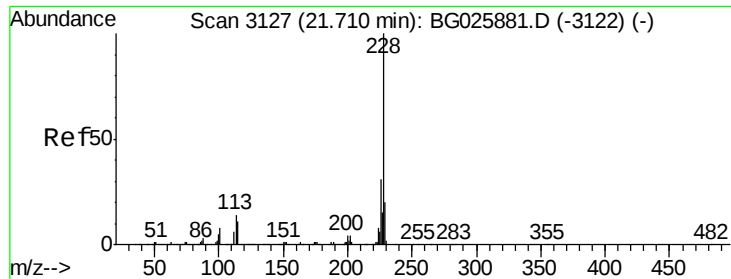

#21

Chrysene

Concen: 1.47 ng/ul

RT: 21.71 min Scan# 3127

Delta R.T. 0.00 min

Lab File: BG025889.D

Acq: 21 Feb 2017 1:20

Instrument :

BNA_G





ClientSampleId :

DABB7

Tgt Ion:	228	Resp:	64789
Ion Ratio	Lower	Upper	
228	100		
226	32.2	24.5	36.7
229	23.5	15.8	23.8

Manual Integrations
APPROVED

mohammad
2/21/2017 10:34:07 AM

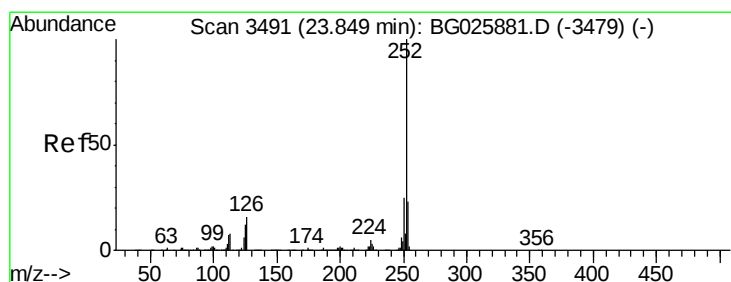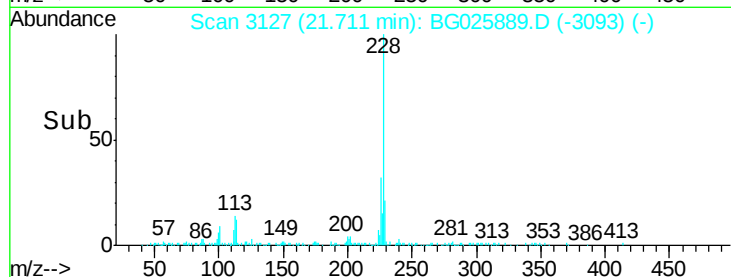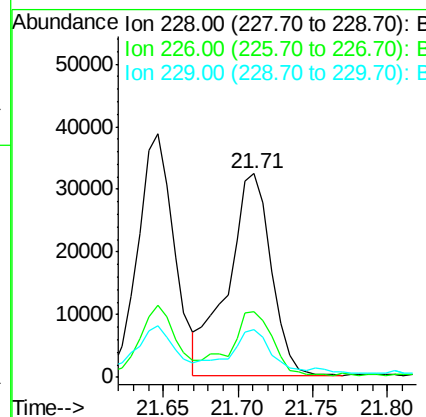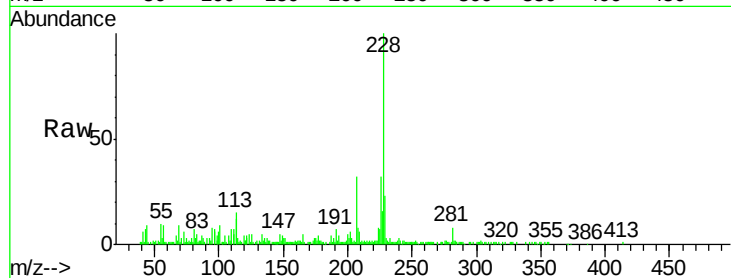

#23

Benzo(b)fluoranthene

Concen: 1.71 ng/ul m




RT: 23.86 min Scan# 3492


Delta R.T. 0.01 min

Lab File: BG025889.D

Acq: 21 Feb 2017 1:20

Tgt Ion:	252	Resp:	78351
Ion Ratio	Lower	Upper	
252	100		
253	25.1	18.0	27.0
125	13.2	8.0	12.0#

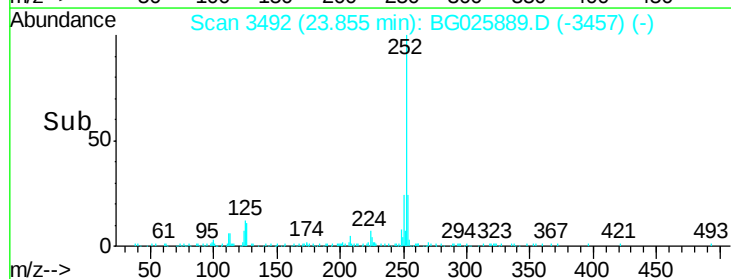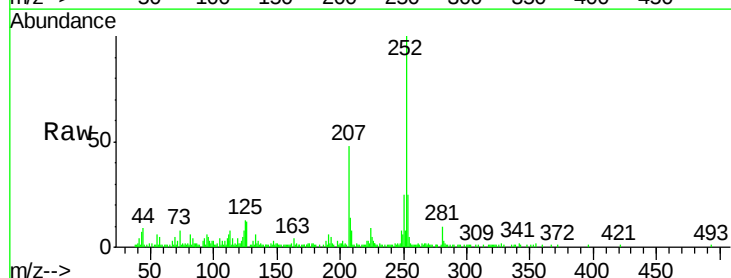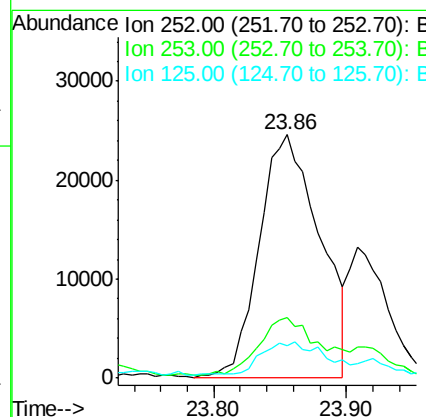

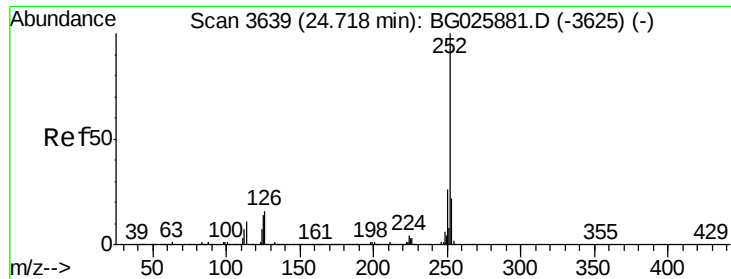

#26
 Benzo(a)pyrene
 Concen: 1.07 ng/ul
 RT: 24.73 min Scan# 3640
 Delta R.T. 0.01 min
 Lab File: BG025889.D
 Acq: 21 Feb 2017 1:20

Instrument :
 BNA_G
 ClientSampleId :
 DABB7

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.0	17.2	25.8
125	15.6	8.2	12.4

Manual Integrations
 APPROVED

mohammad
 2/21/2017 10:34:07 AM

