


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022020\
 Data File : BG044516.D
 Acq On : 20 Feb 2020 11:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

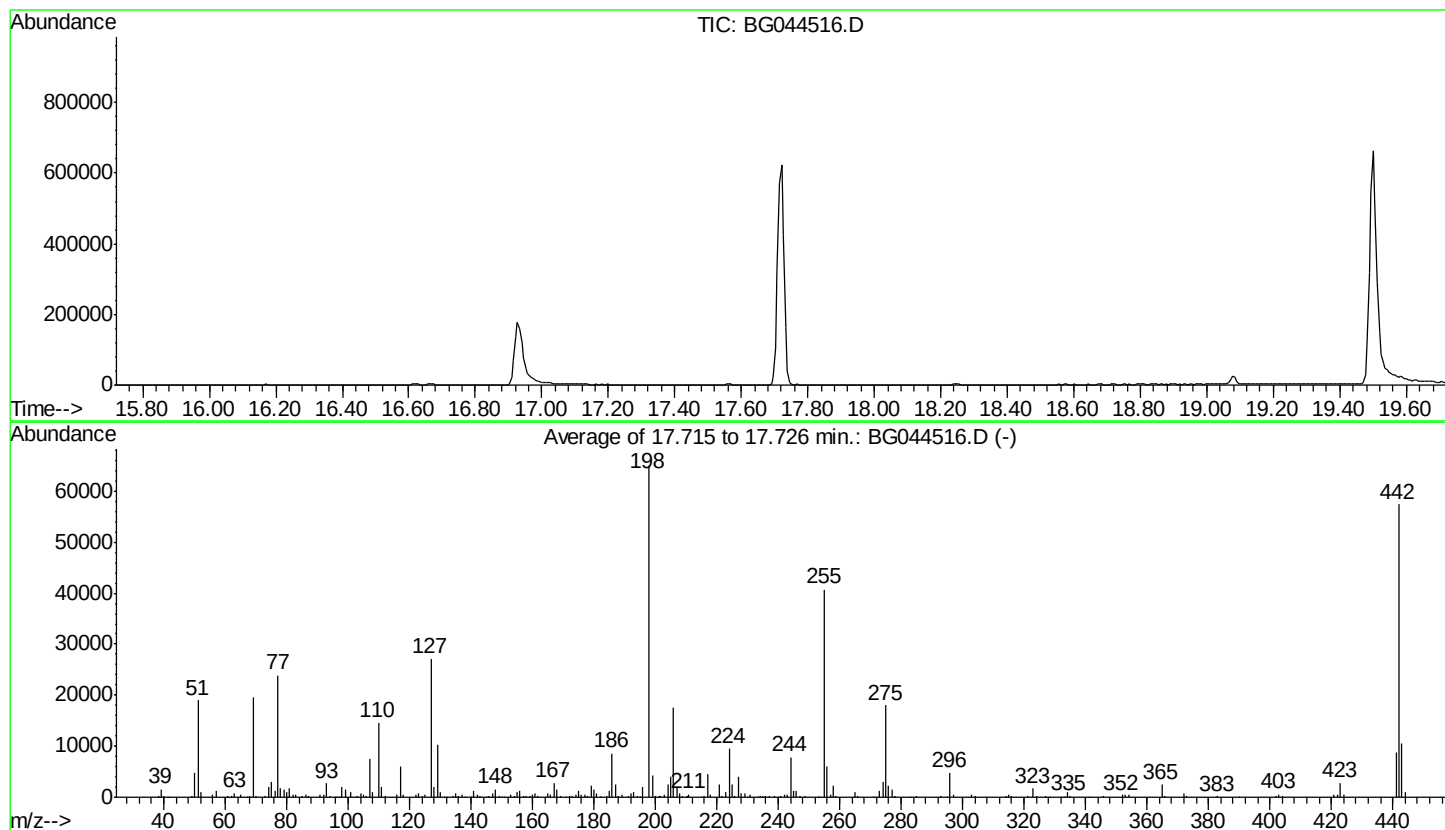

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	19007	PASS
68	69	0.00	2	1.7	335	PASS
69	198	0.00	100	29.9	19464	PASS
70	69	0.00	2	0.7	141	PASS
127	198	10	80	41.8	27192	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64994	PASS
199	198	5	9	6.7	4338	PASS
275	198	10	60	27.7	18033	PASS
365	198	1	100	3.8	2442	PASS
441	198	0.01	100	13.4	8723	PASS
442	198	50	100	88.2	57352	PASS
443	442	15	24	18.4	10527	PASS