


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022020\
 Data File : BG044522.D
 Acq On : 20 Feb 2020 15:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

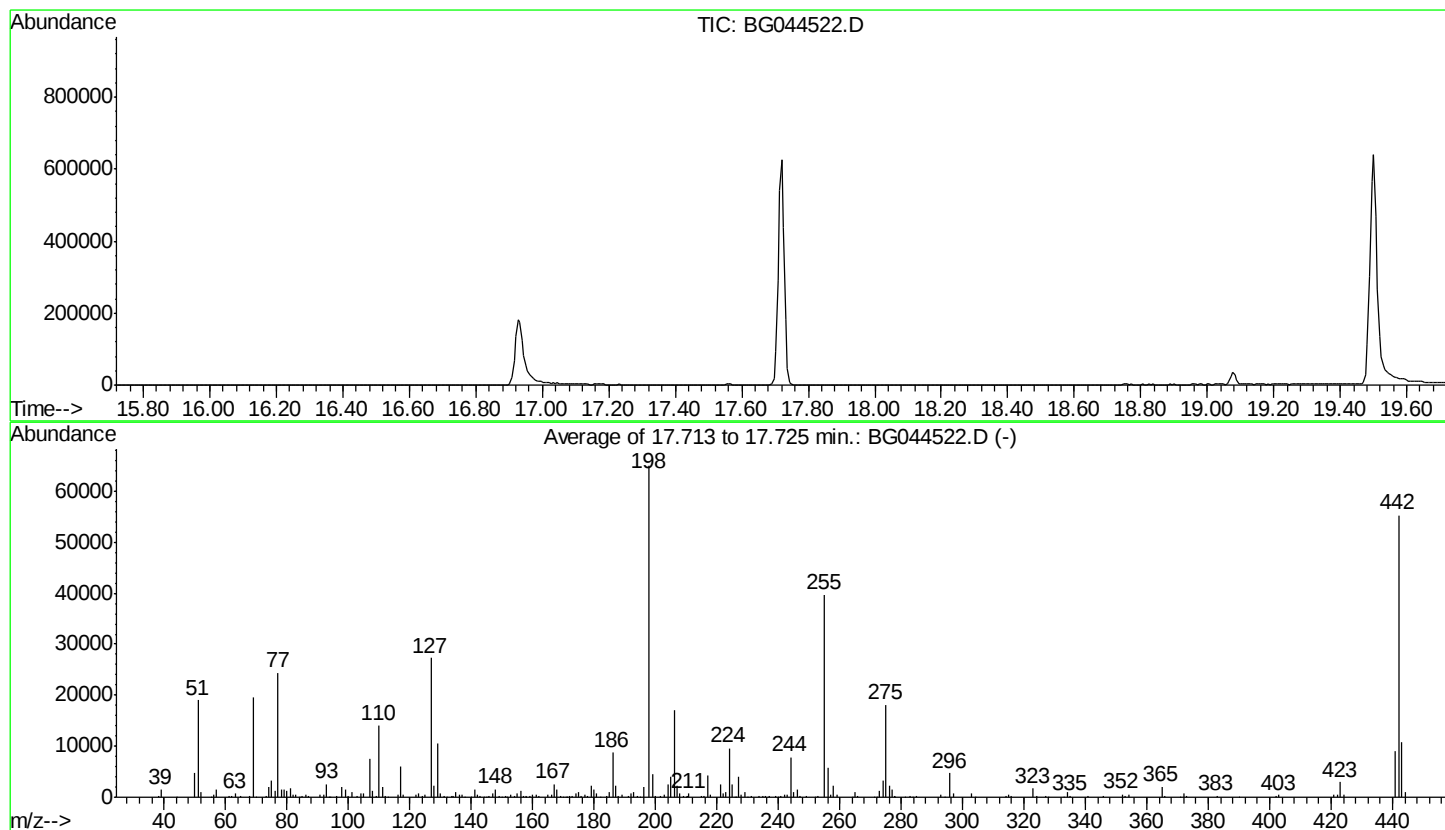

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	19011	PASS
68	69	0.00	2	0.8	162	PASS
69	198	0.00	100	30.0	19524	PASS
70	69	0.00	2	0.3	50	PASS
127	198	10	80	41.9	27240	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65002	PASS
199	198	5	9	6.9	4460	PASS
275	198	10	60	27.8	18082	PASS
365	198	1	100	3.3	2130	PASS
441	198	0.01	100	13.8	8944	PASS
442	198	50	100	84.9	55216	PASS
443	442	15	24	19.4	10717	PASS