

Data File : BG025919.D
Acq On : 22 Feb 2017 00:26
Operator : SJ/MA
Sample : I1901-07MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DABF2MS

Quant Time: Feb 22 02:48:26 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.3-EPA-BG021617MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 21 23:44:02 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	169870	20.00	ng/ul	0.00
2) Naphthalene-d8	10.89	136	786231	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.68	164	446868	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.42	188	909125	20.00	ng/ul	0.00
17) Chrysene-d12	21.68	240	903705	20.00	ng/ul	0.00
22) Perylene-d12	24.92	264	847106	20.00	ng/ul	0.03

System Monitoring Compounds						
7) Acenaphthylene-d8	14.38	160	697296	18.84	ng/ul	0.00
10) Fluorene-d10	15.67	176	500314	17.61	ng/ul	0.00
14) Anthracene-d10	17.52	188	689561	16.78	ng/ul	0.00
18) Pyrene-d10	19.79	212	721201	16.56	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.69	264	624311	16.65	ng/ul	0.03

Target Compounds				Qvalue		
9) Acenaphthene	14.75	153	497686	18.37	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG025919.D

Acq On : 22 Feb 2017 00:26

Operator : SJ/MA

Sample : I1901-07MS

Misc :

ALS Vial : 23 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

DABF2MS


Quant Time: Feb 22 02:48:26 2017


Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.3-EPA-BG021617MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Feb 21 23:44:02 2017

Response via : Initial Calibration

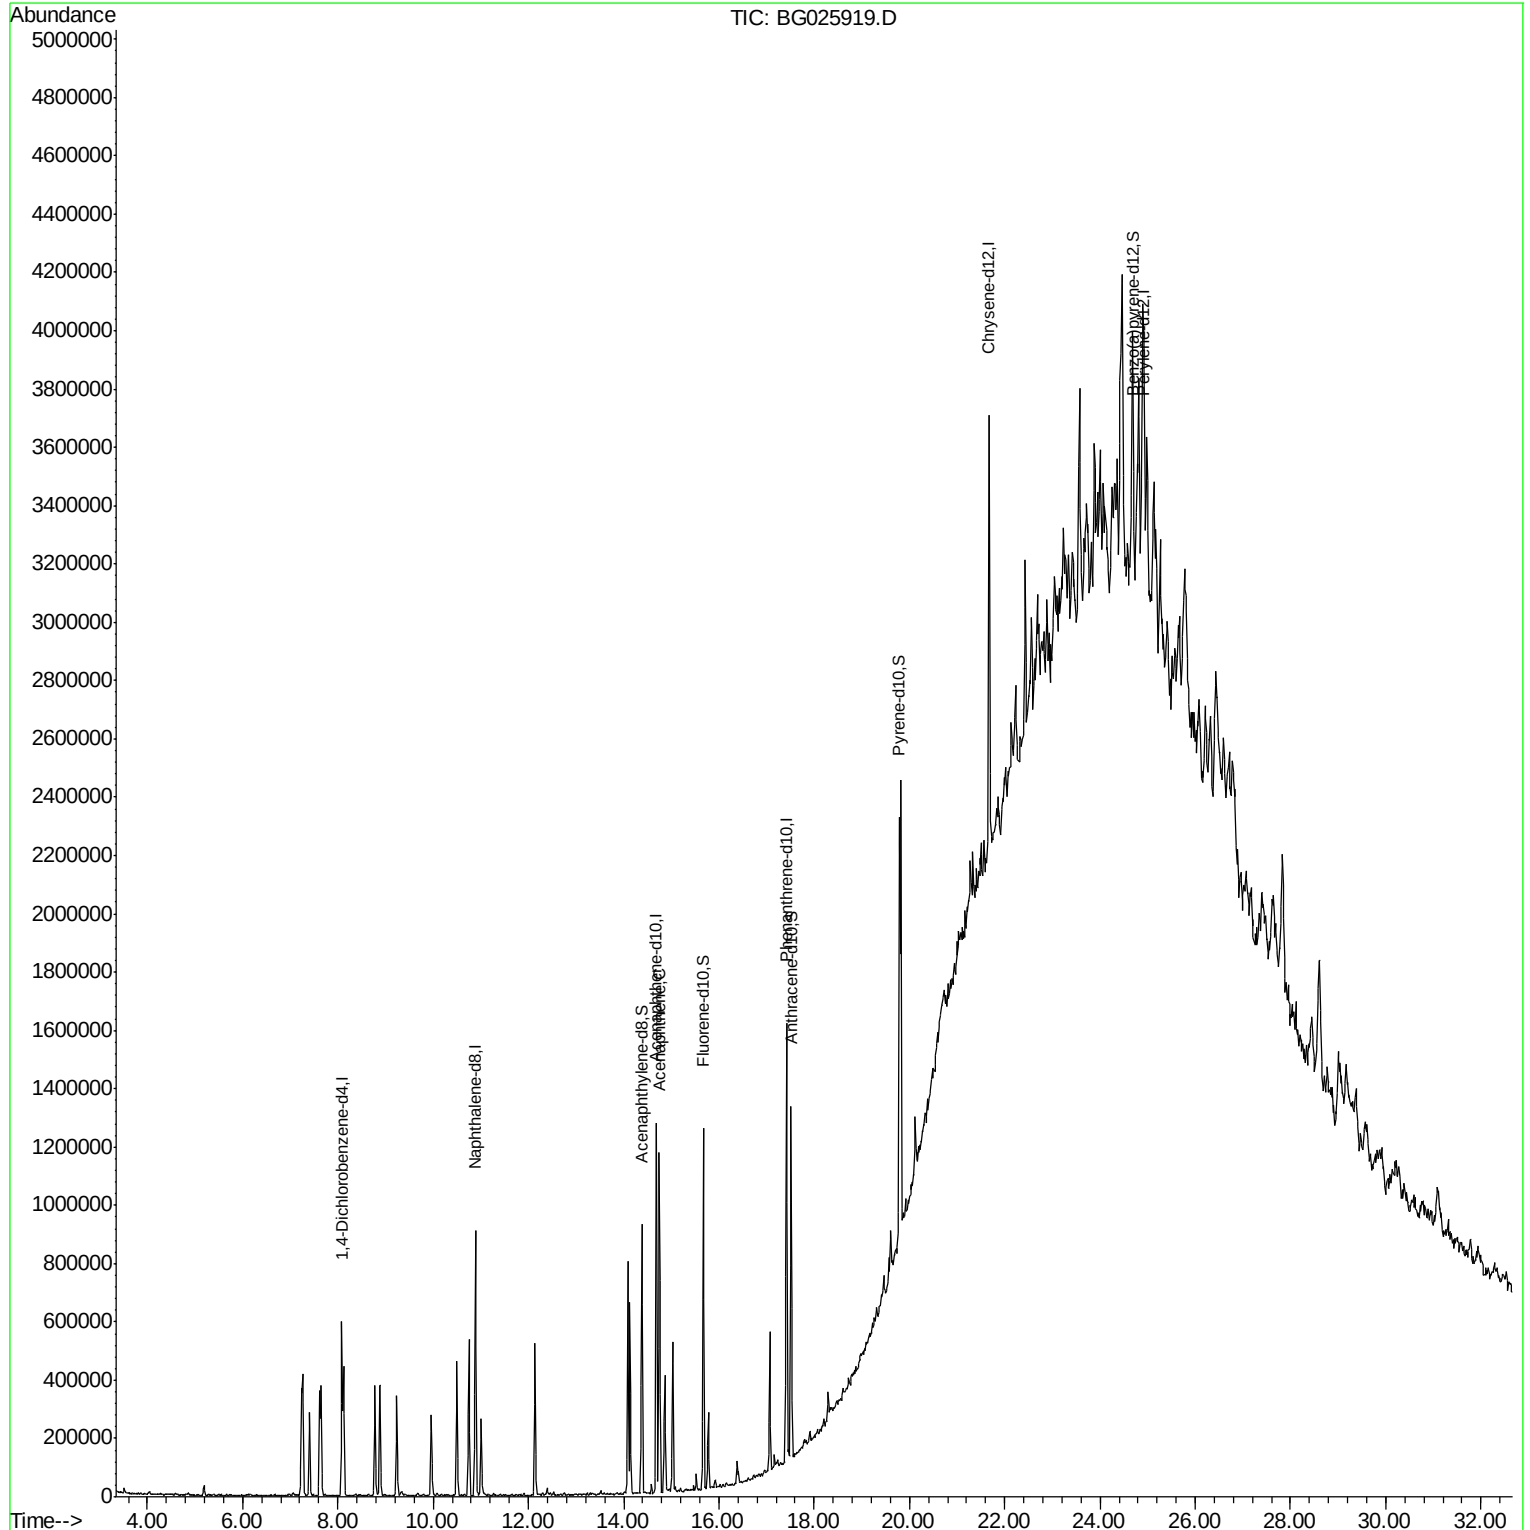

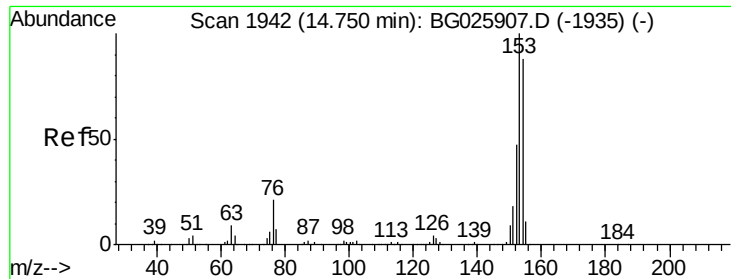

#9

Acenaphthene

Concen: 18.37 ng/ul

RT: 14.75 min Scan# 1942

Delta R.T. -0.00 min

Lab File: BG025919.D

Acq: 22 Feb 2017 00:26

Instrument :

BNA_G

ClientSampleId :

DABF2MS



Tgt Ion:153 Resp: 497686

Ion Ratio Lower Upper

153 100

152 47.6 39.0 58.6

154 91.0 66.8 100.2

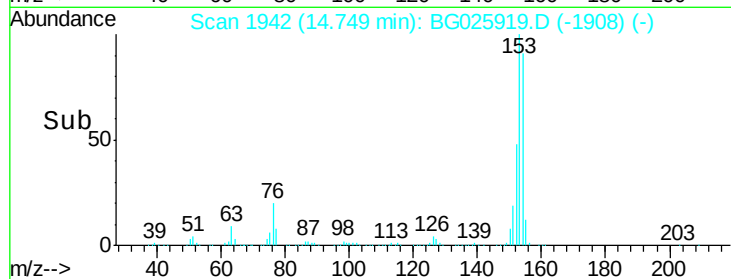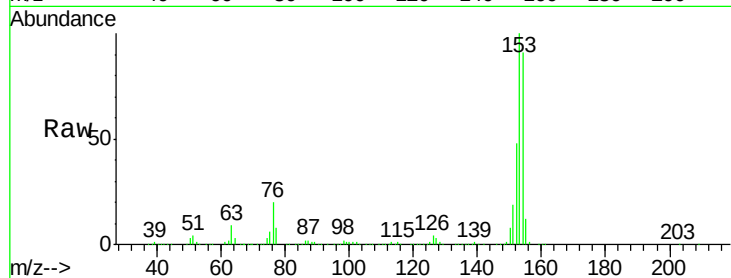

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

