
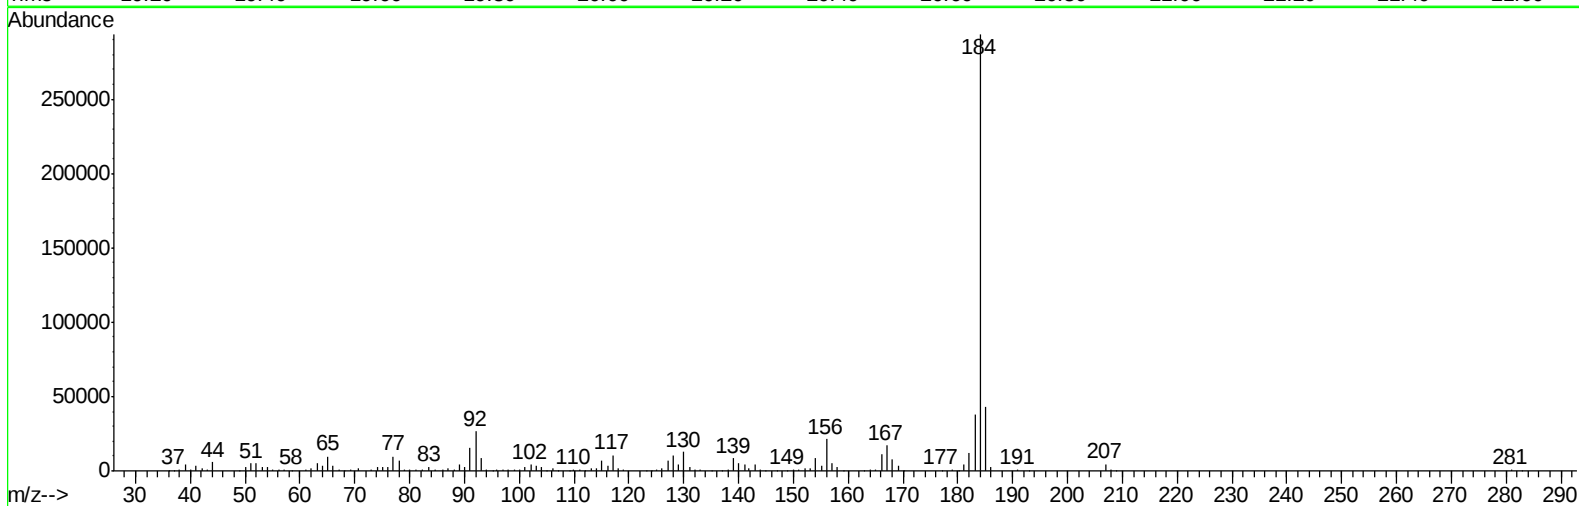


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022118\
Data File : BG032754.D
Acq On : 21 Feb 2018 10:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 08:03:20 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 21 15:45:53 2018
Response via : Initial Calibration

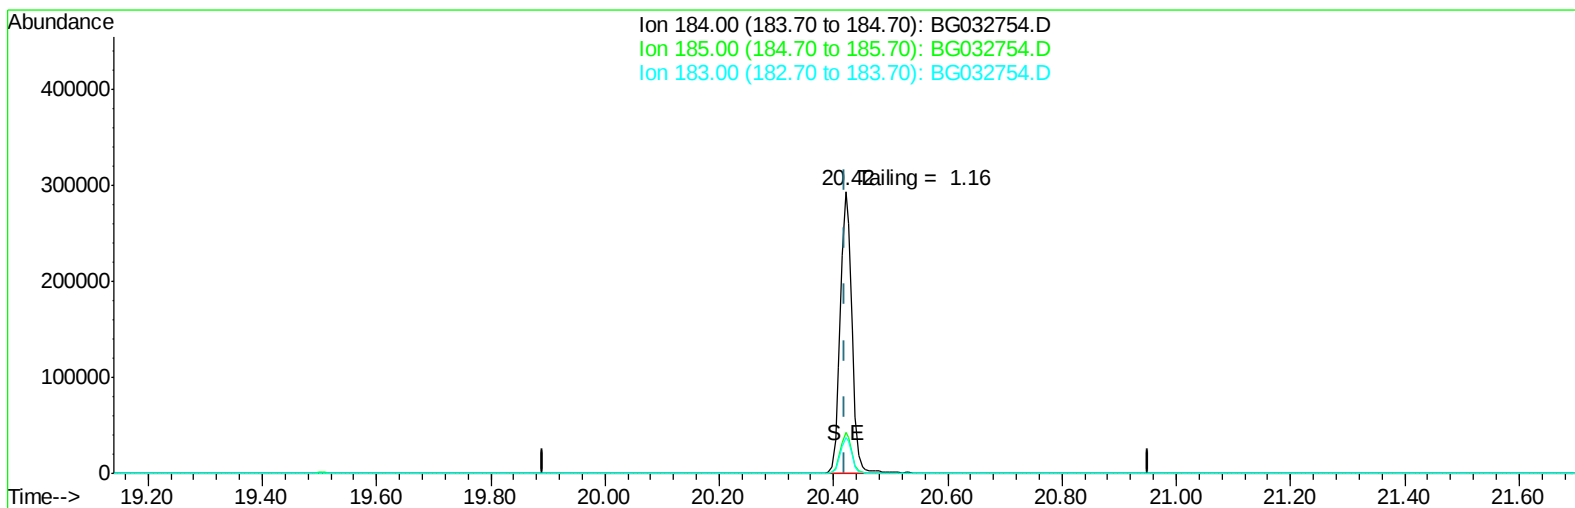

TIC: BG032754.D

(76) Benzidine



20.421min (-0.000) 0.00ng

response 420014

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.73
183.00	13.30	12.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022118\
Data File : BG032754.D
Acq On : 21 Feb 2018 10:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 08:03:20 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 21 15:45:53 2018
Response via : Initial Calibration

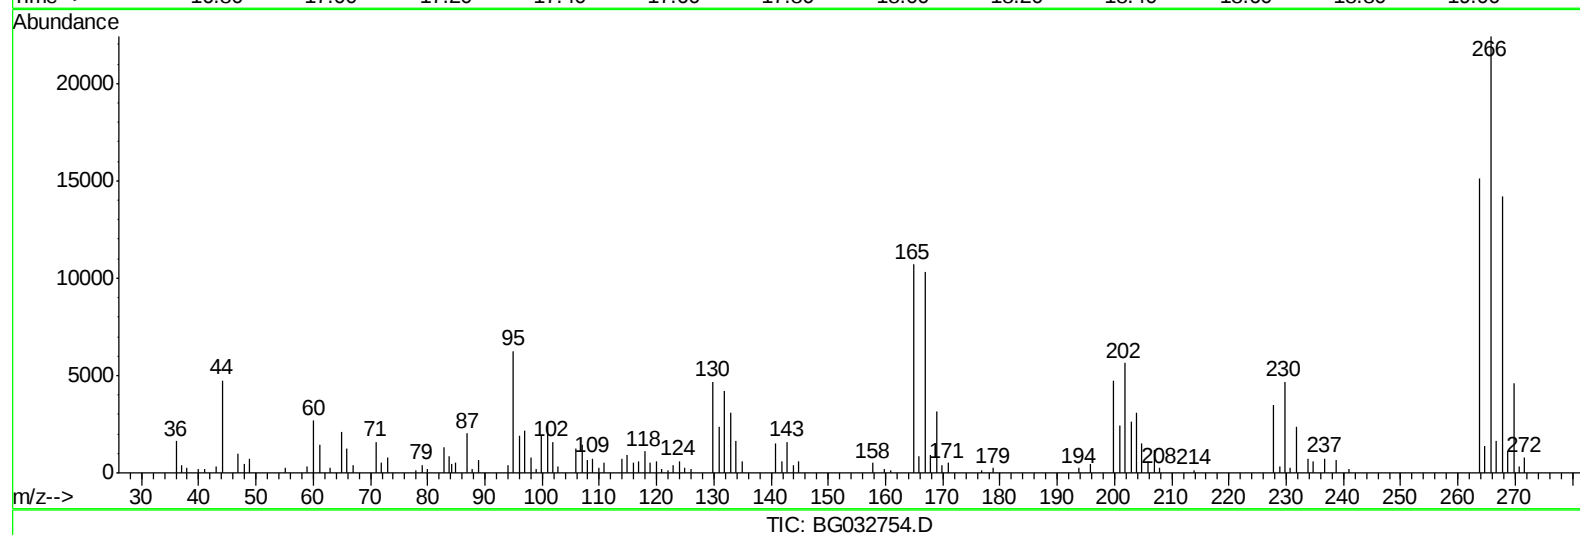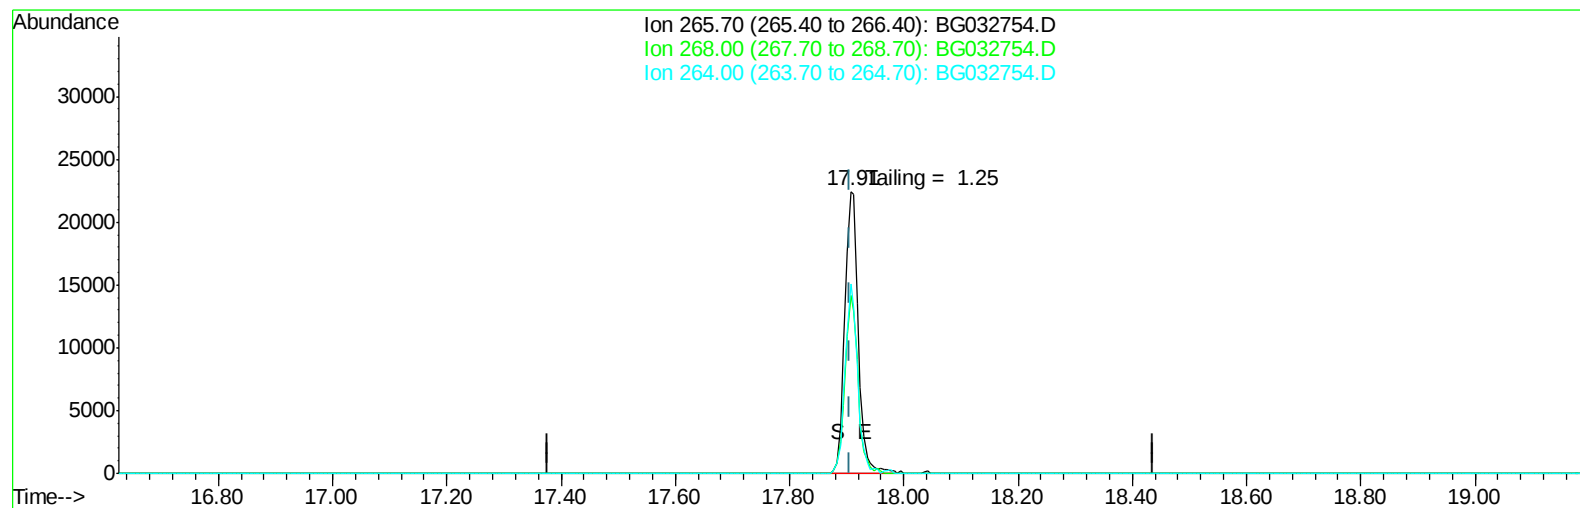

(69) Pentachlorophenol (C)

17.906min (-0.000) 28893.33ng

response 37017

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.23
264.00	62.00	67.46
0.00	0.00	0.00