


Nitrobenzene-d5

Response Ratio

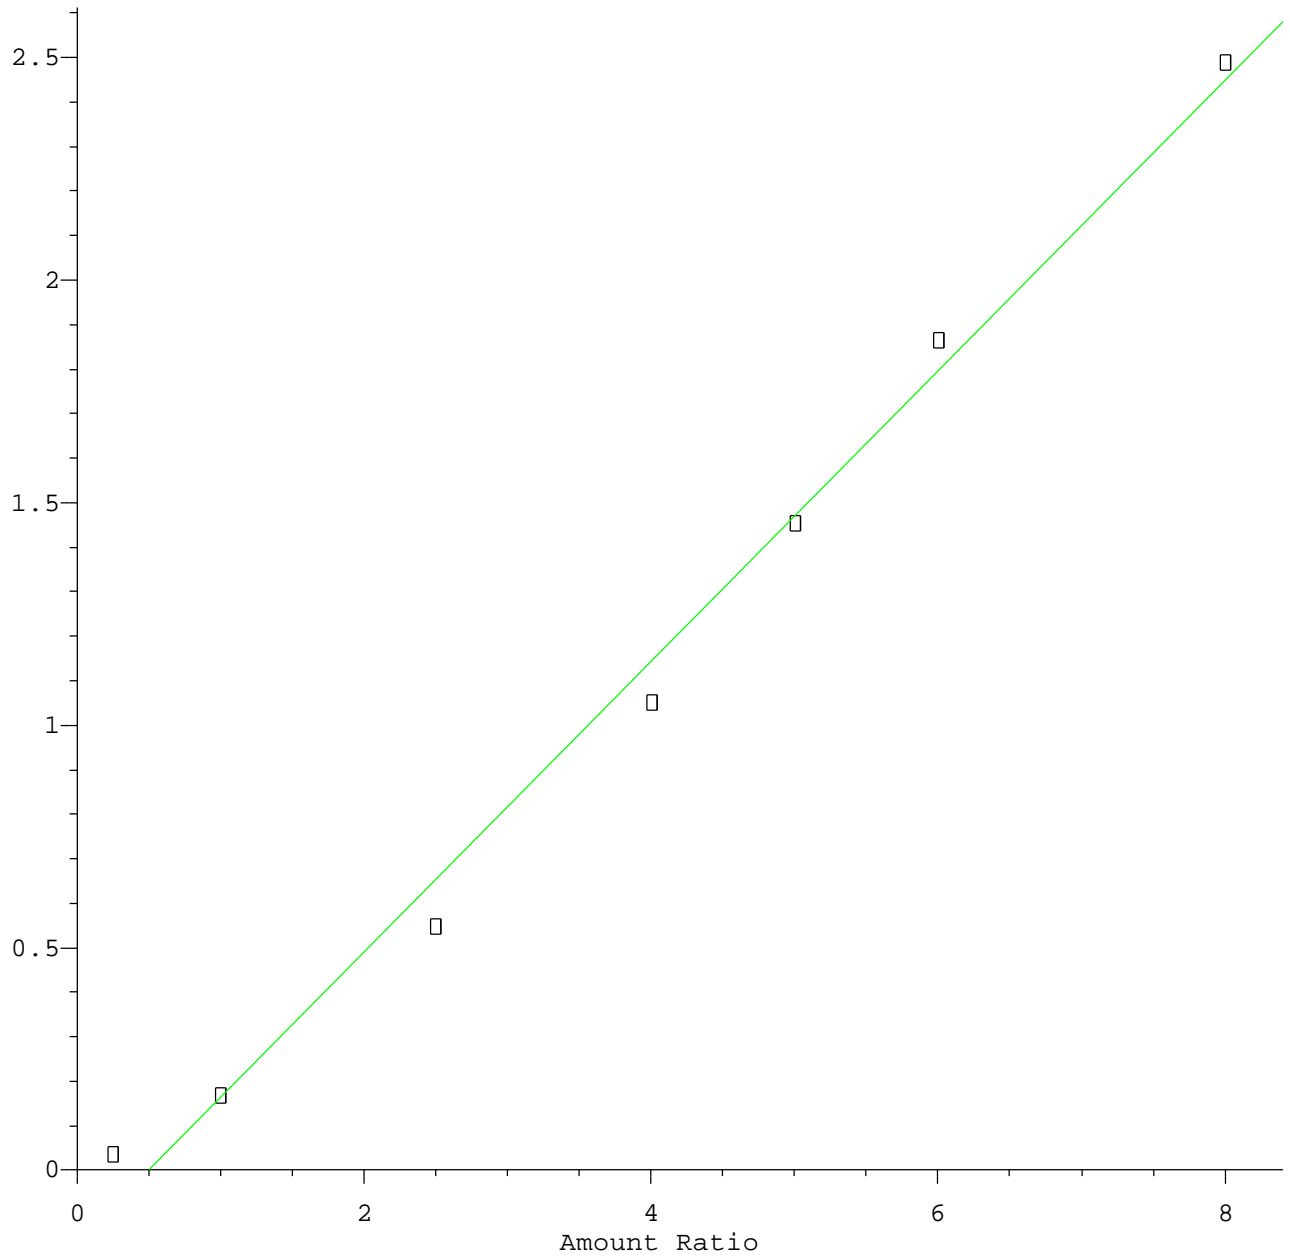


Resp Ratio = 3.26e-001 * Amt - 1.62e-001
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

Nitrobenzene

Response Ratio

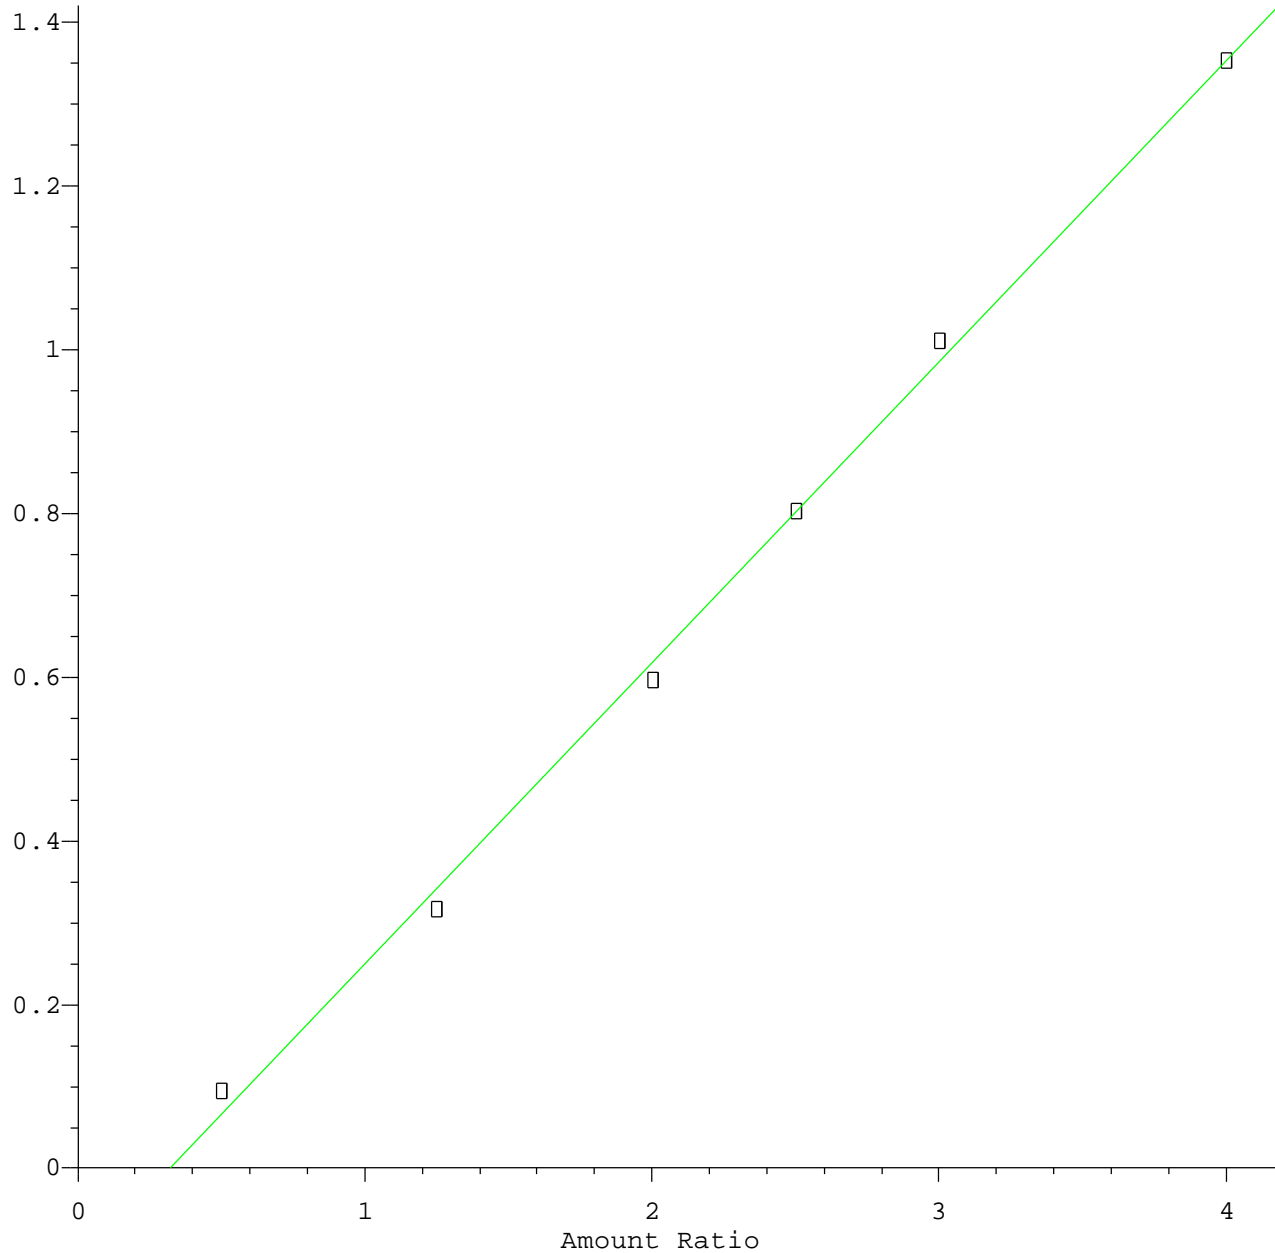


Resp Ratio = 3.68e-001 * Amt - 1.17e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

2-Nitroaniline

Response Ratio

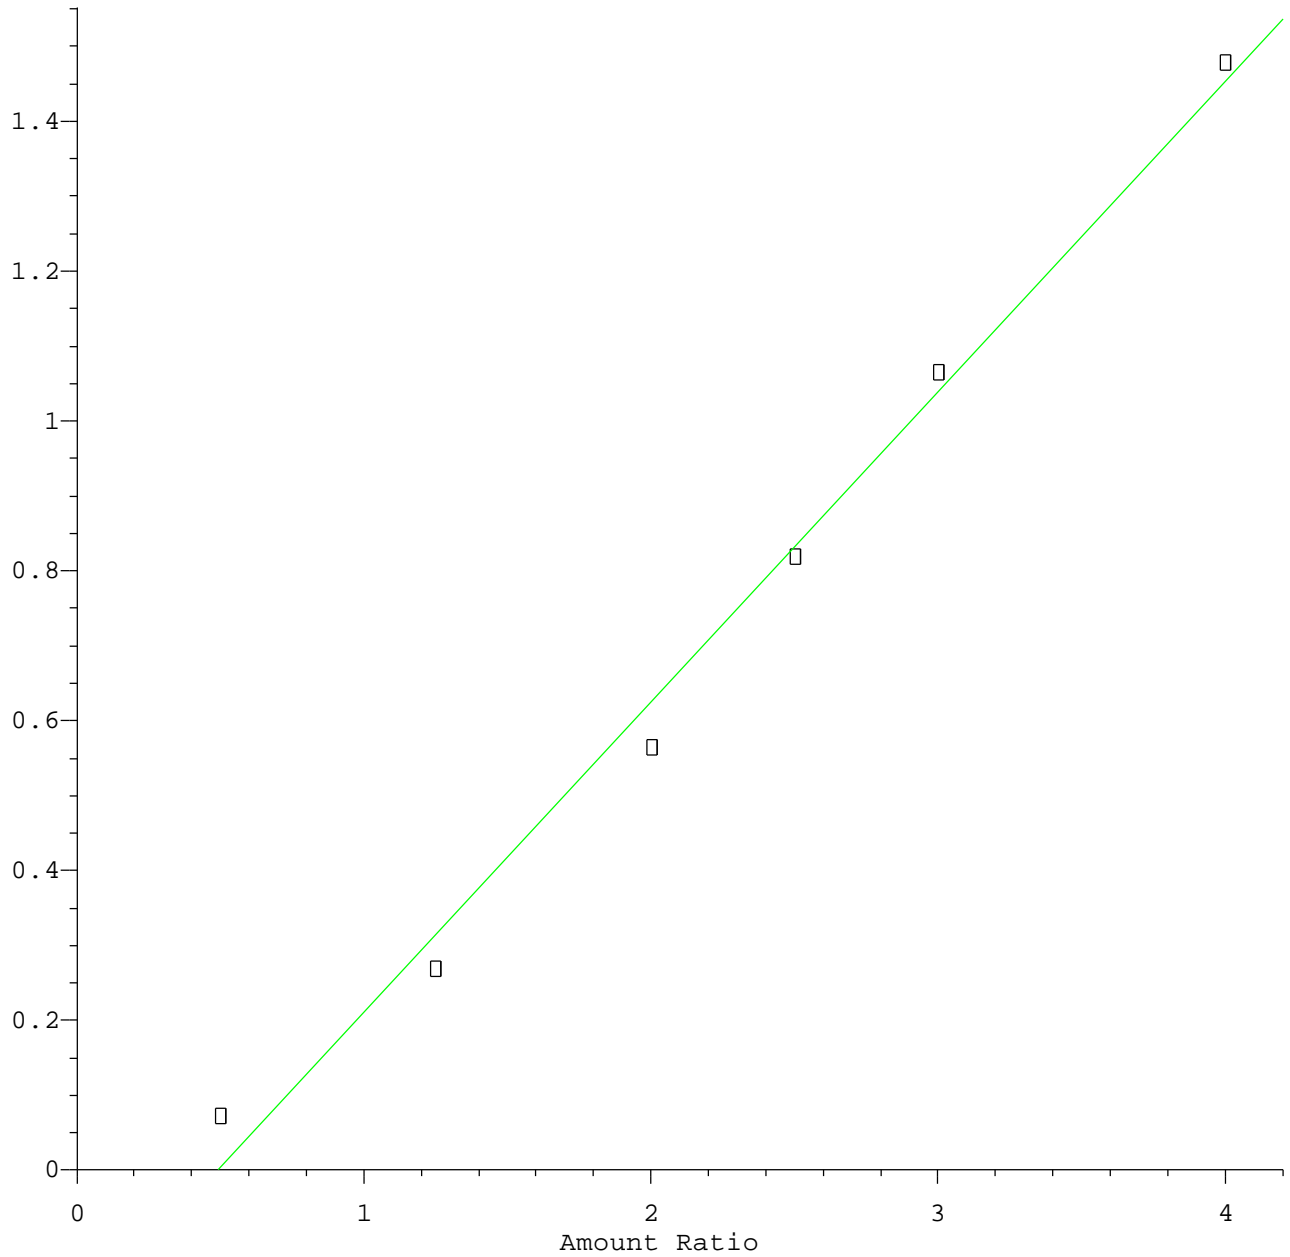


Resp Ratio = 4.14e-001 * Amt - 2.04e-001
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

2-Nitroaniline

Response Ratio

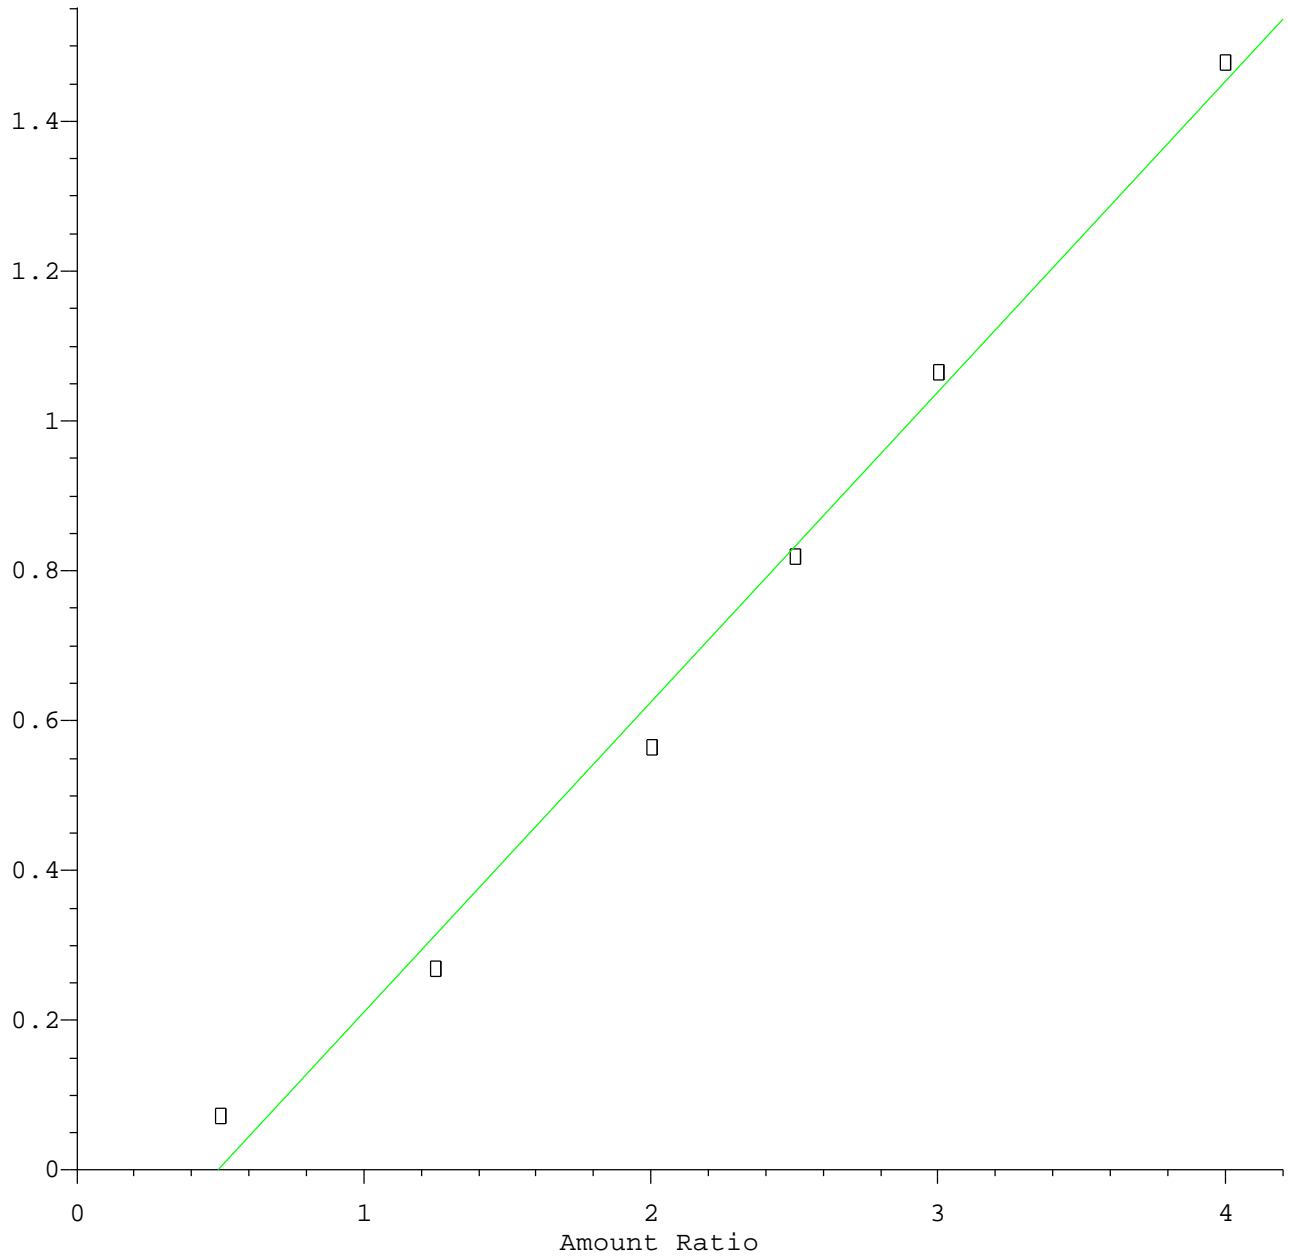


Resp Ratio = 4.14e-001 * Amt - 2.04e-001
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

2,6-Dinitrotoluene

Response Ratio

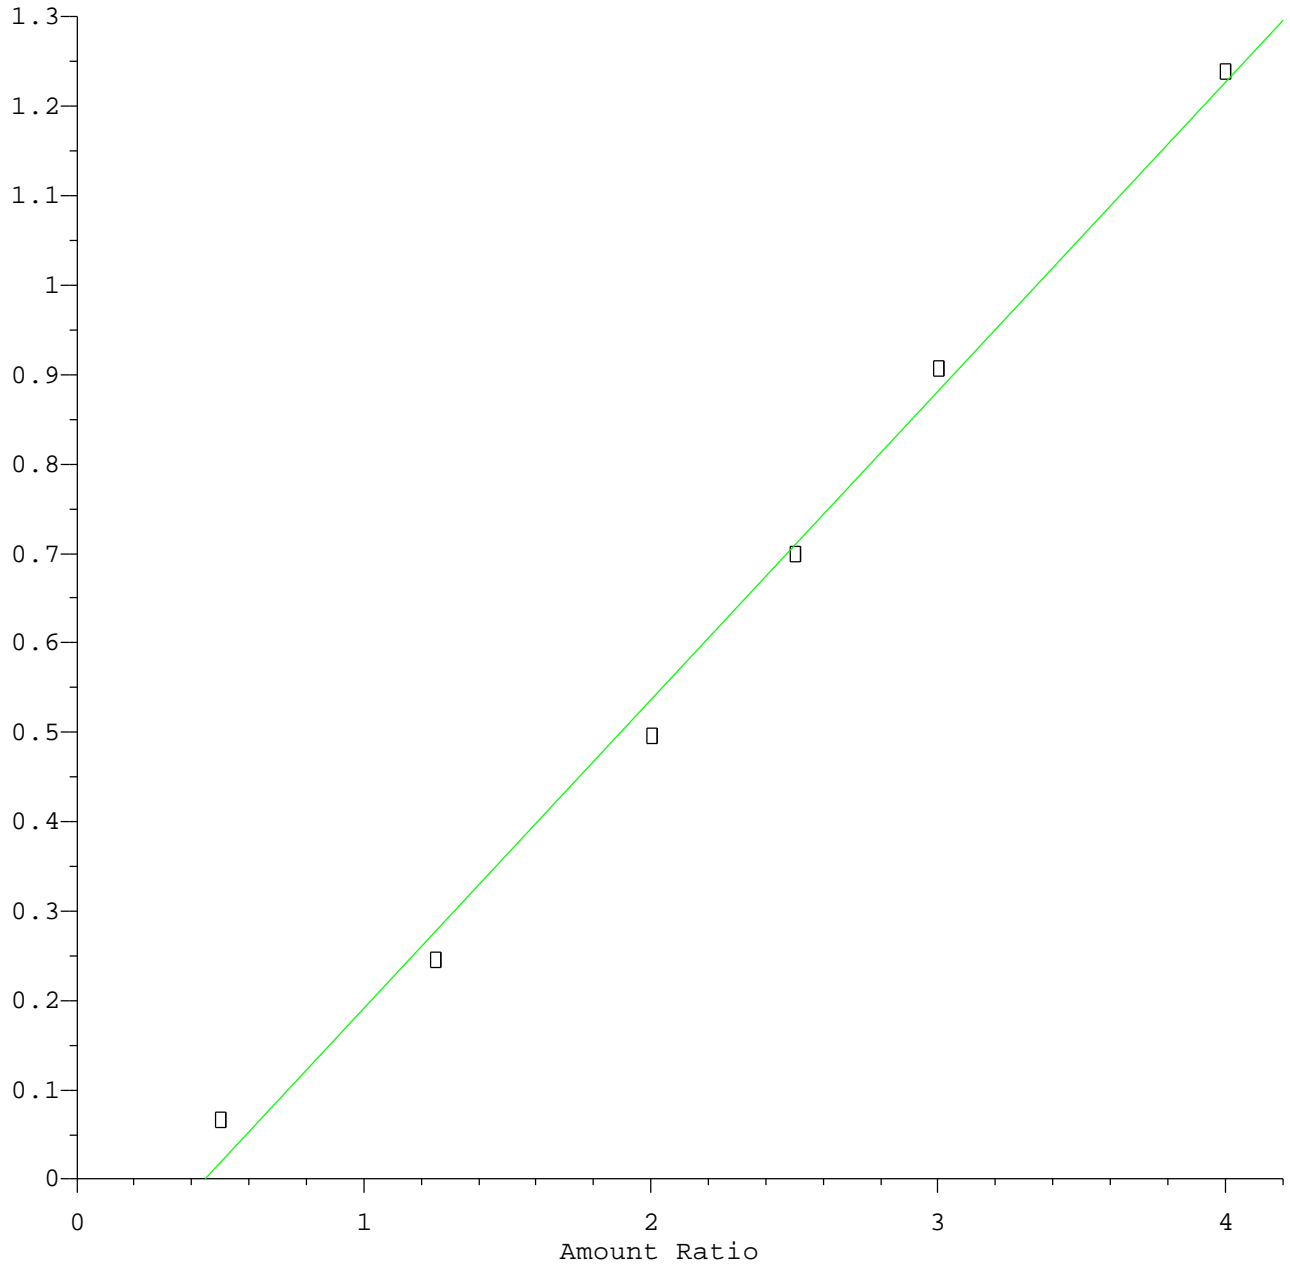


Resp Ratio = 3.45e-001 * Amt - 1.54e-001
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

2,6-Dinitrotoluene

Response Ratio

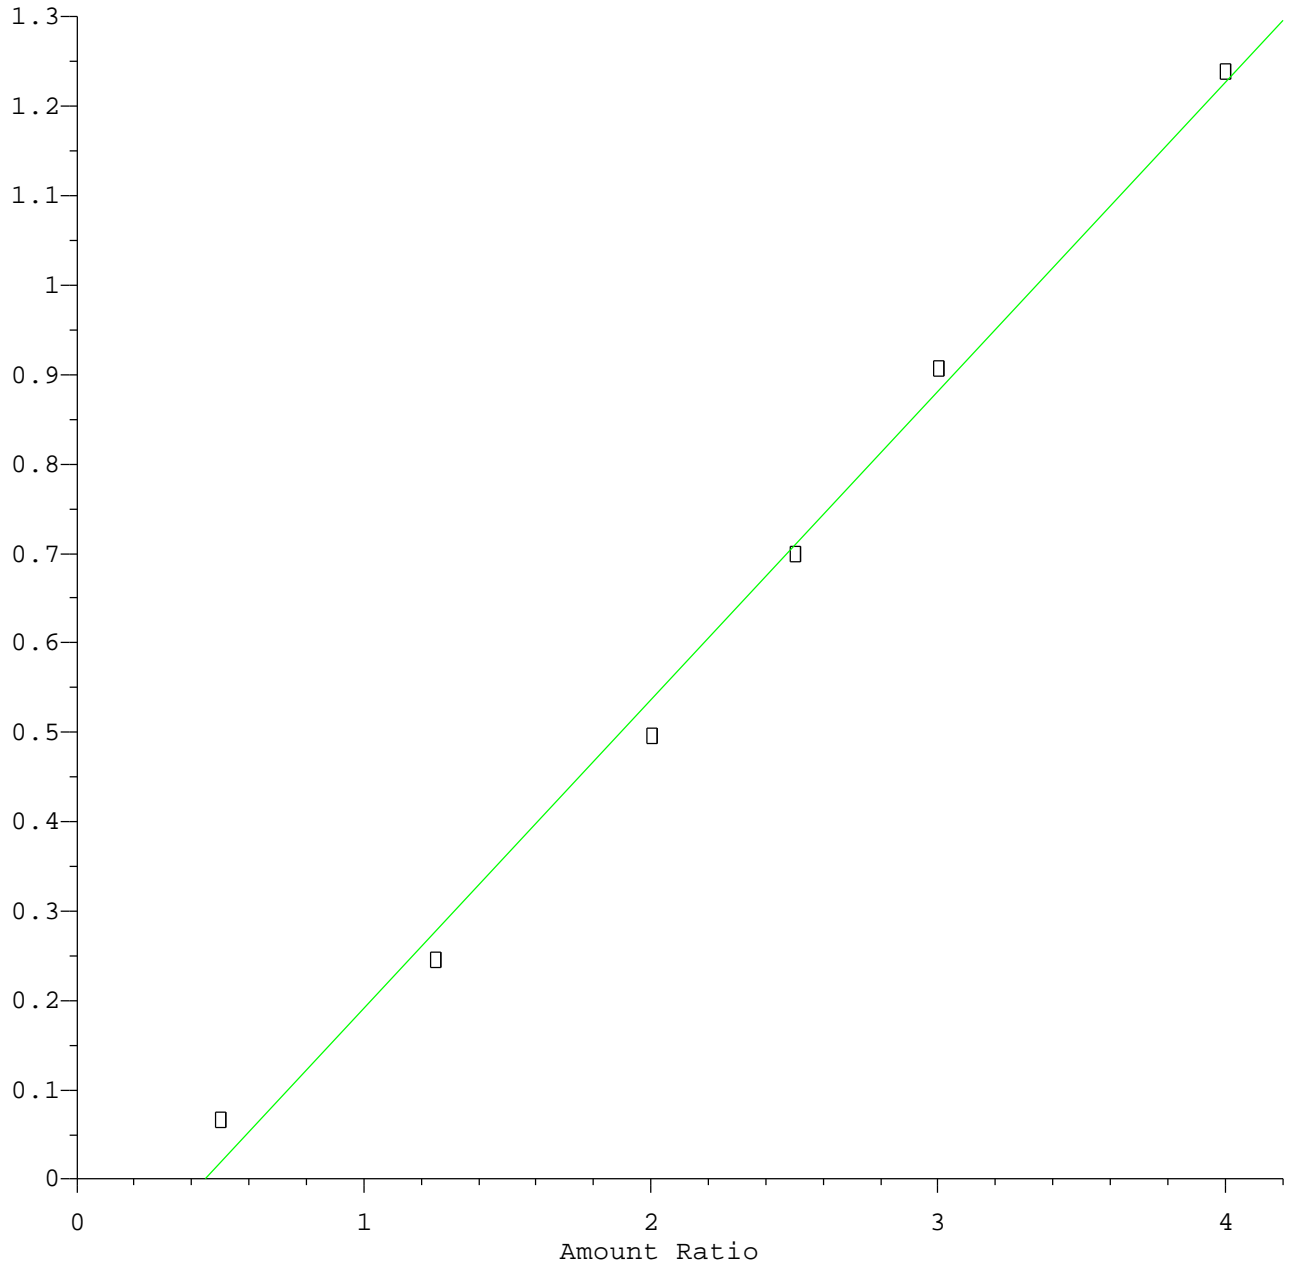


Resp Ratio = 3.45e-001 * Amt - 1.54e-001
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

3-Nitroaniline

Response Ratio

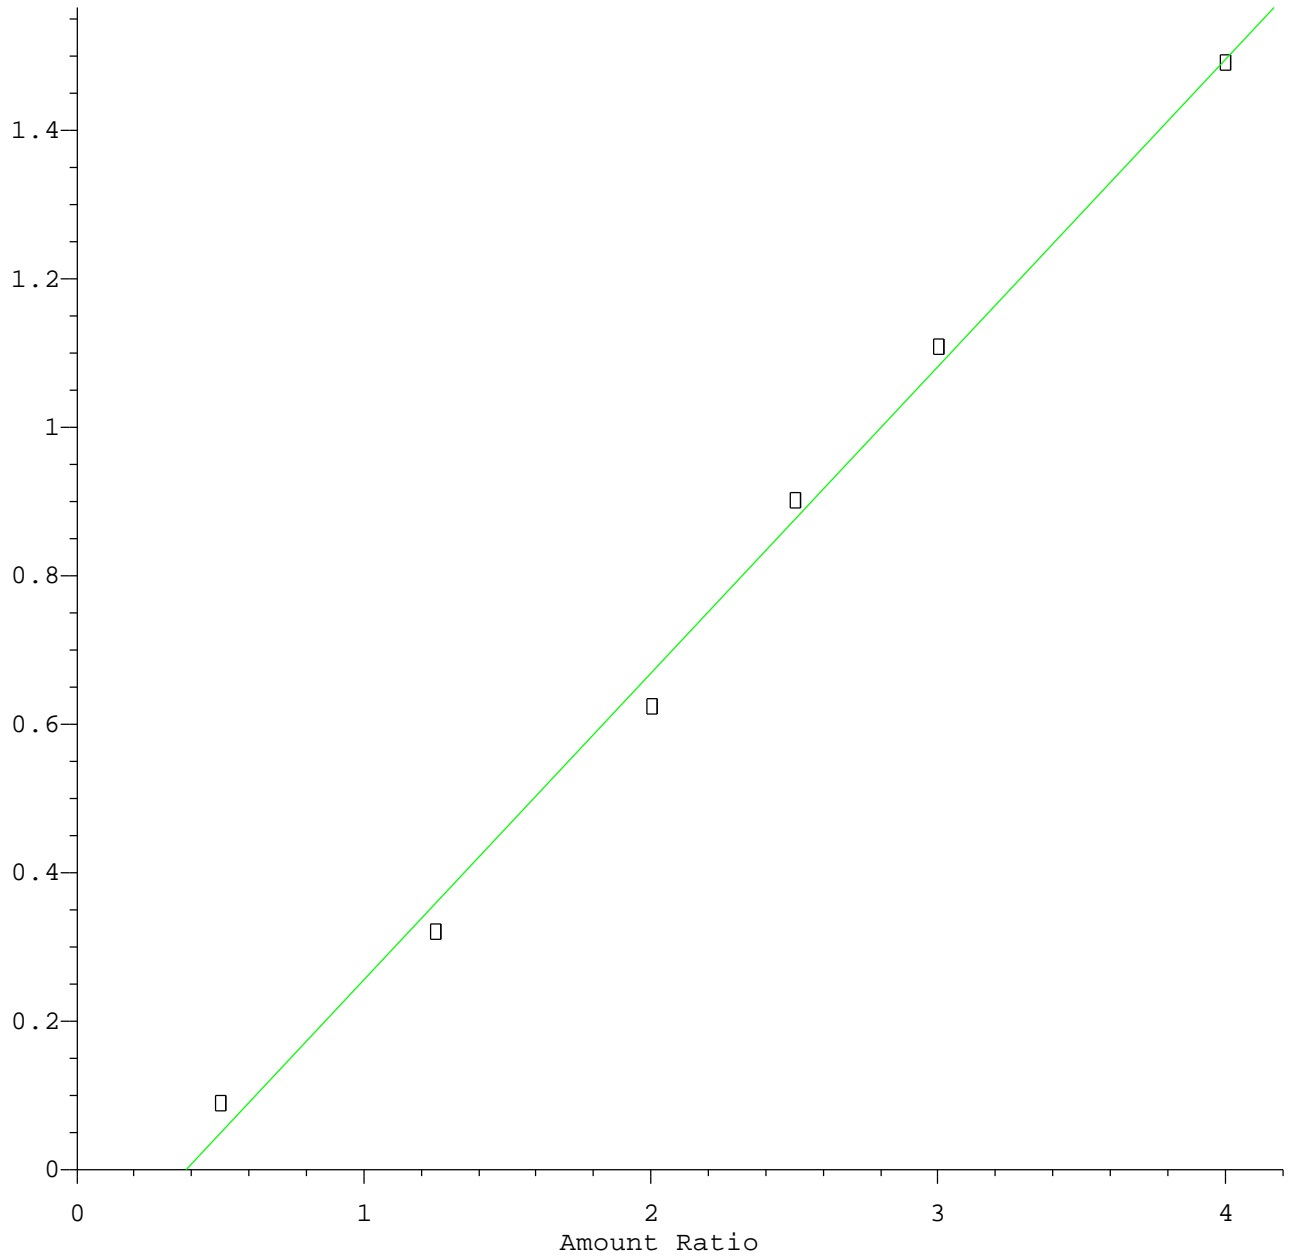


Resp Ratio = 4.13e-001 * Amt - 1.56e-001
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

4-Nitrophenol

Response Ratio

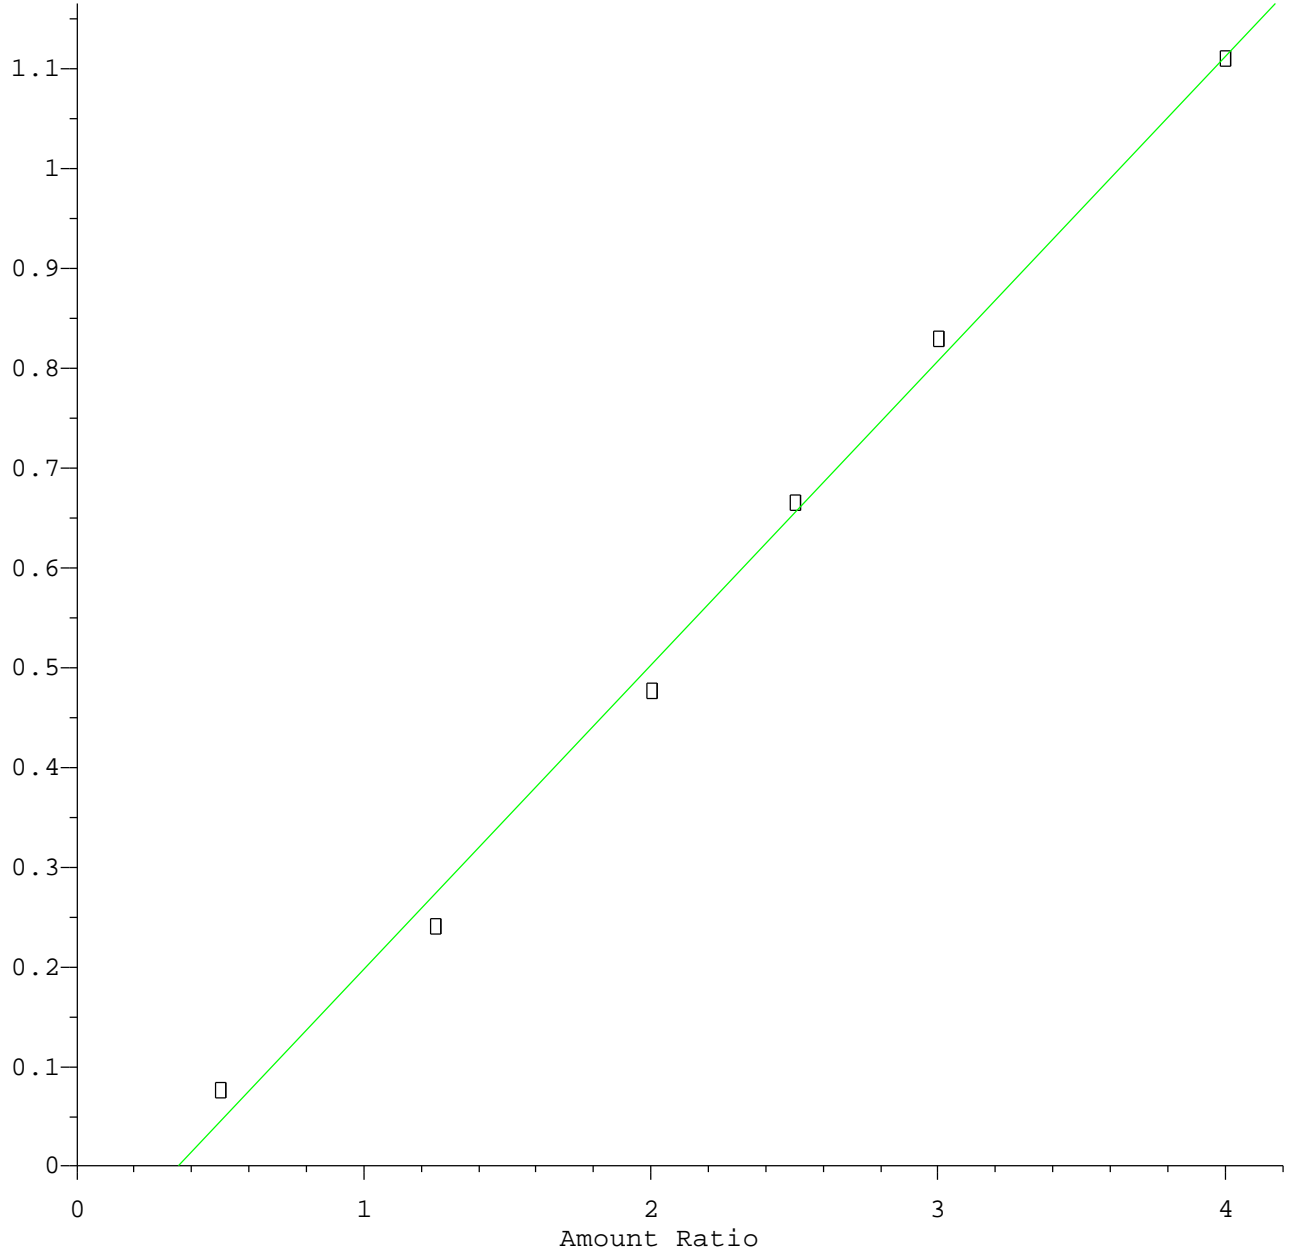


Resp Ratio = 3.05e-001 * Amt - 1.08e-001
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

4-Nitroaniline


Response Ratio

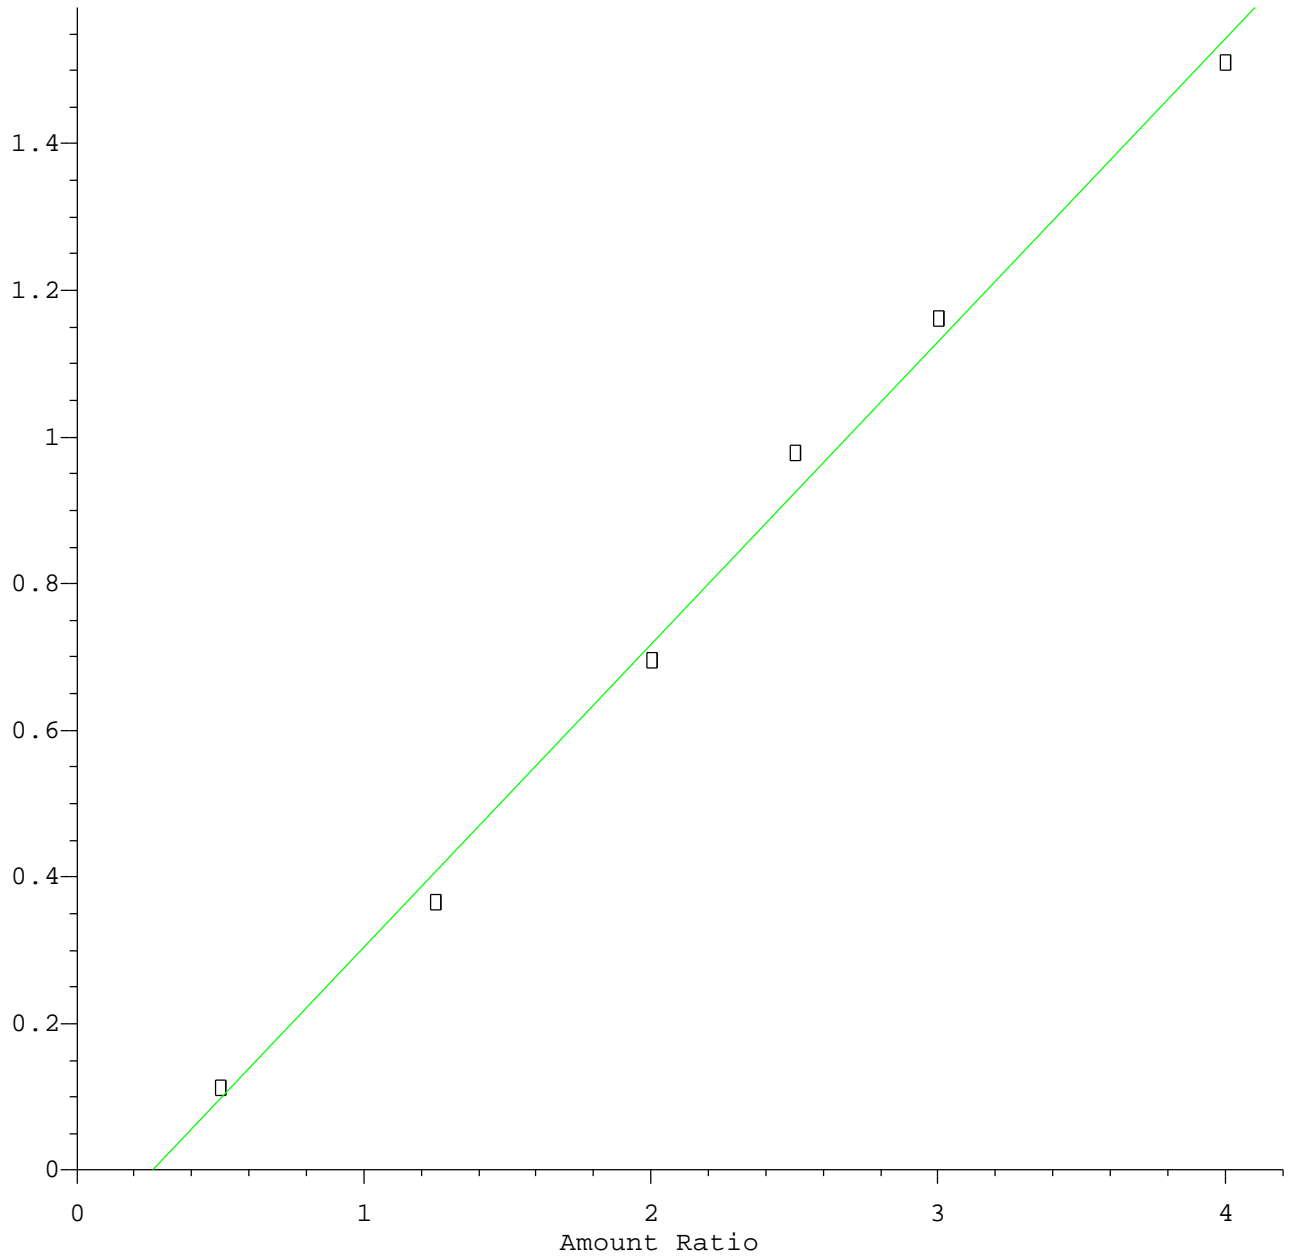

Resp Ratio = 4.13e-001 * Amt - 1.10e-001
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

2-Nitrophenol

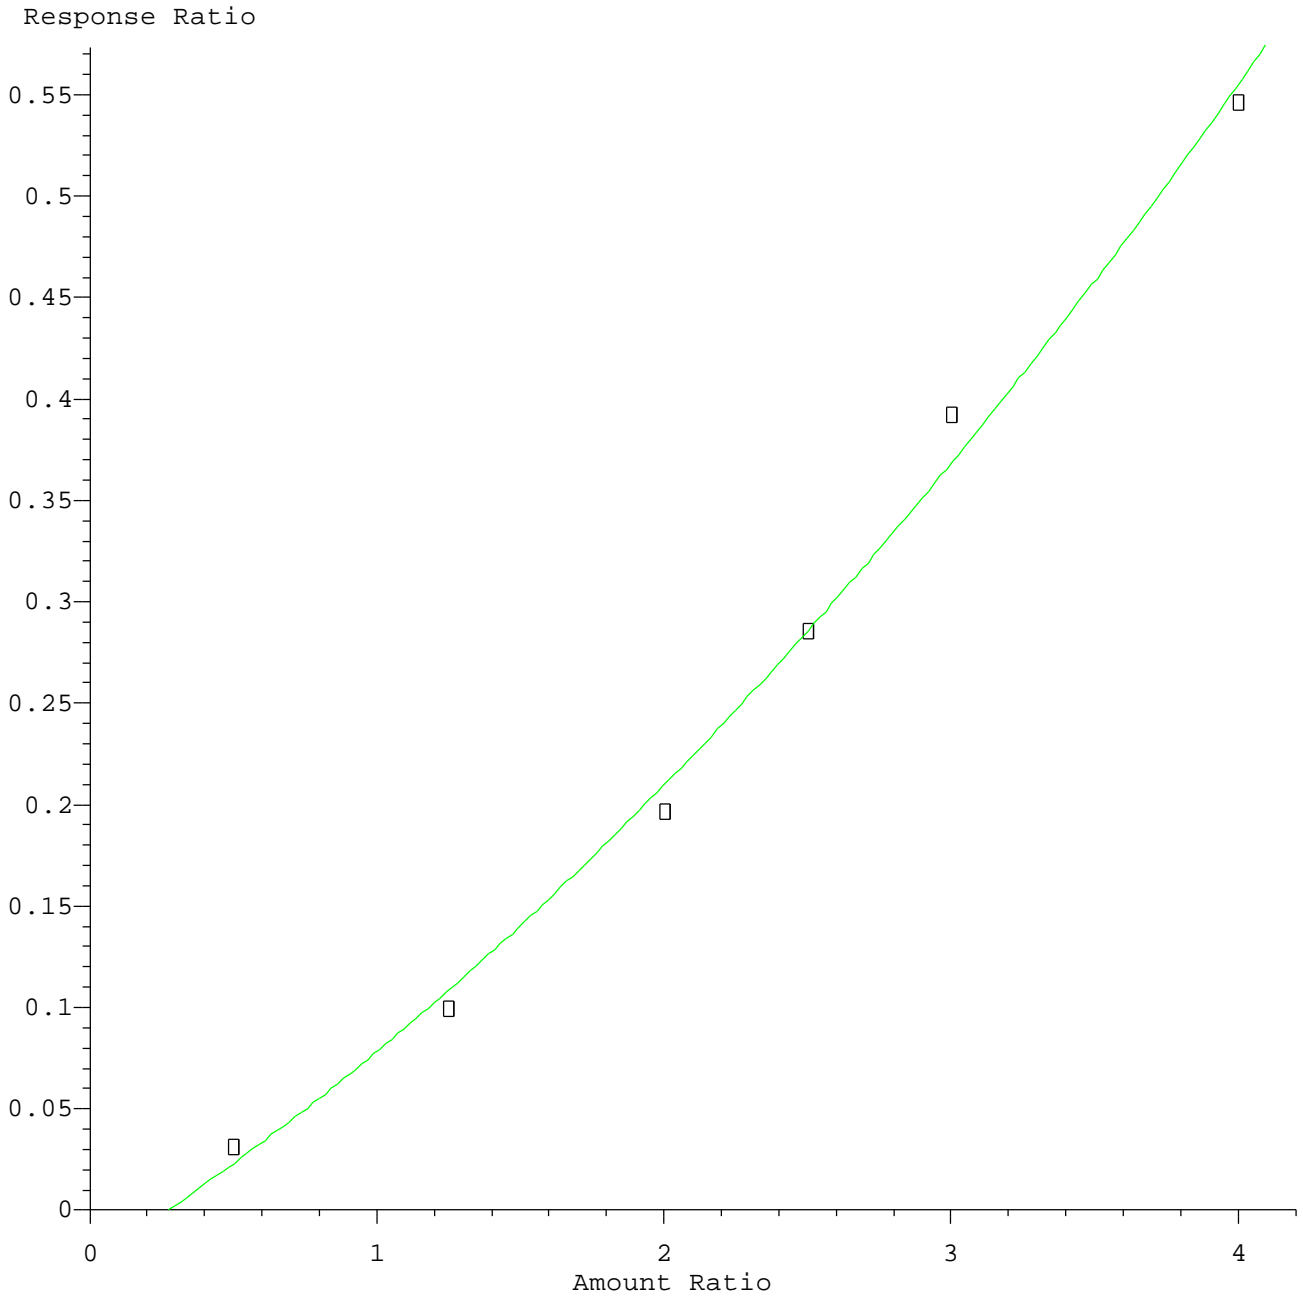


$R = 1.38e-002 A^2 + 8.97e-002 A - 2.54e-002$
Coef of Det (r^2) = 0.995 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

Benzoic acid


Response Ratio

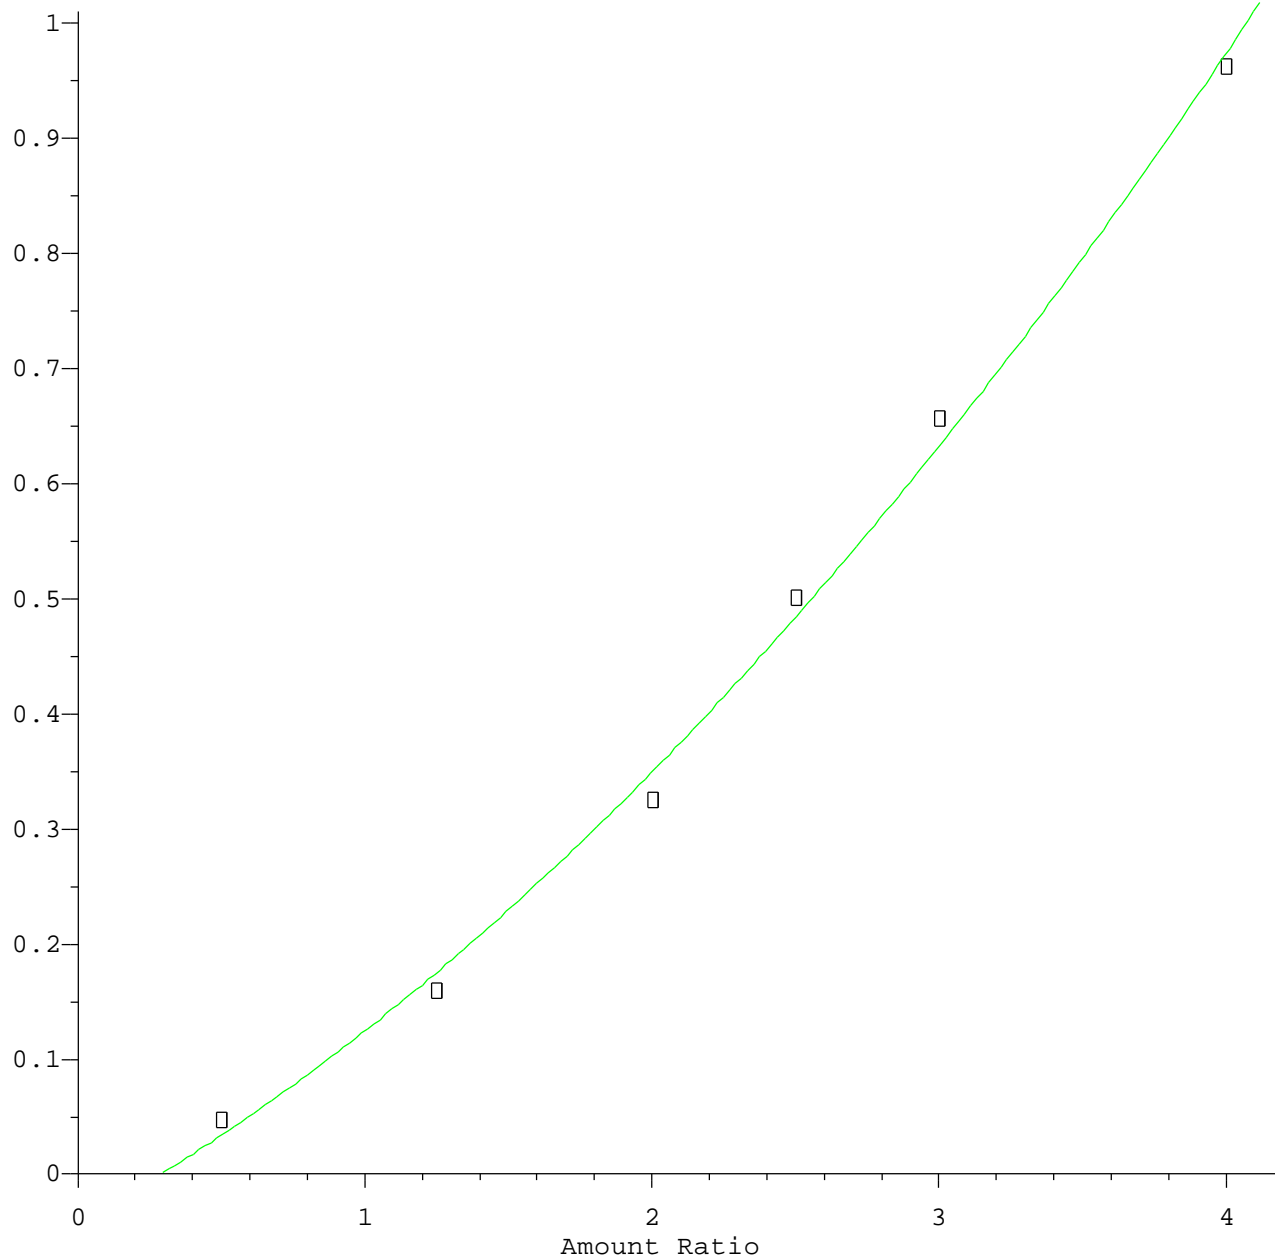

$R = 2.91e-002 A^2 + 1.38e-001 A - 4.26e-002$
Coef of Det (r^2) = 0.996 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

2,4-Dinitrophenol

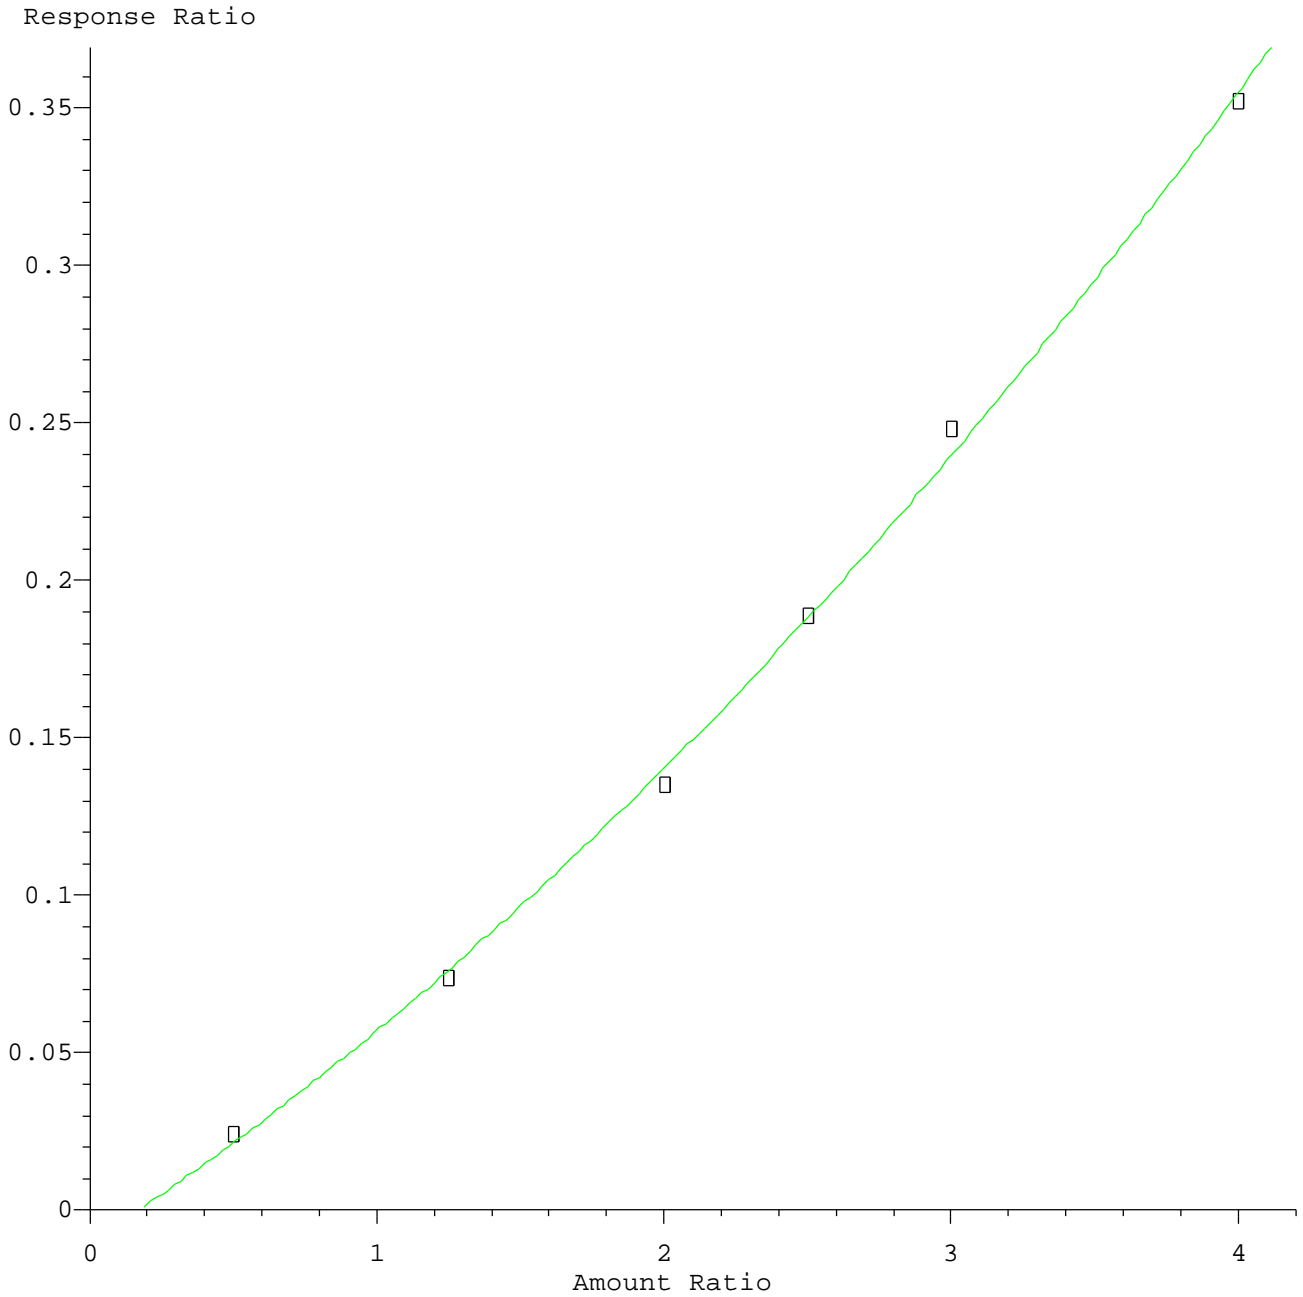


$R = 8.02e-003 A^2 + 5.92e-002 A - 1.03e-002$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

2,4-Dinitrotoluene

Response Ratio

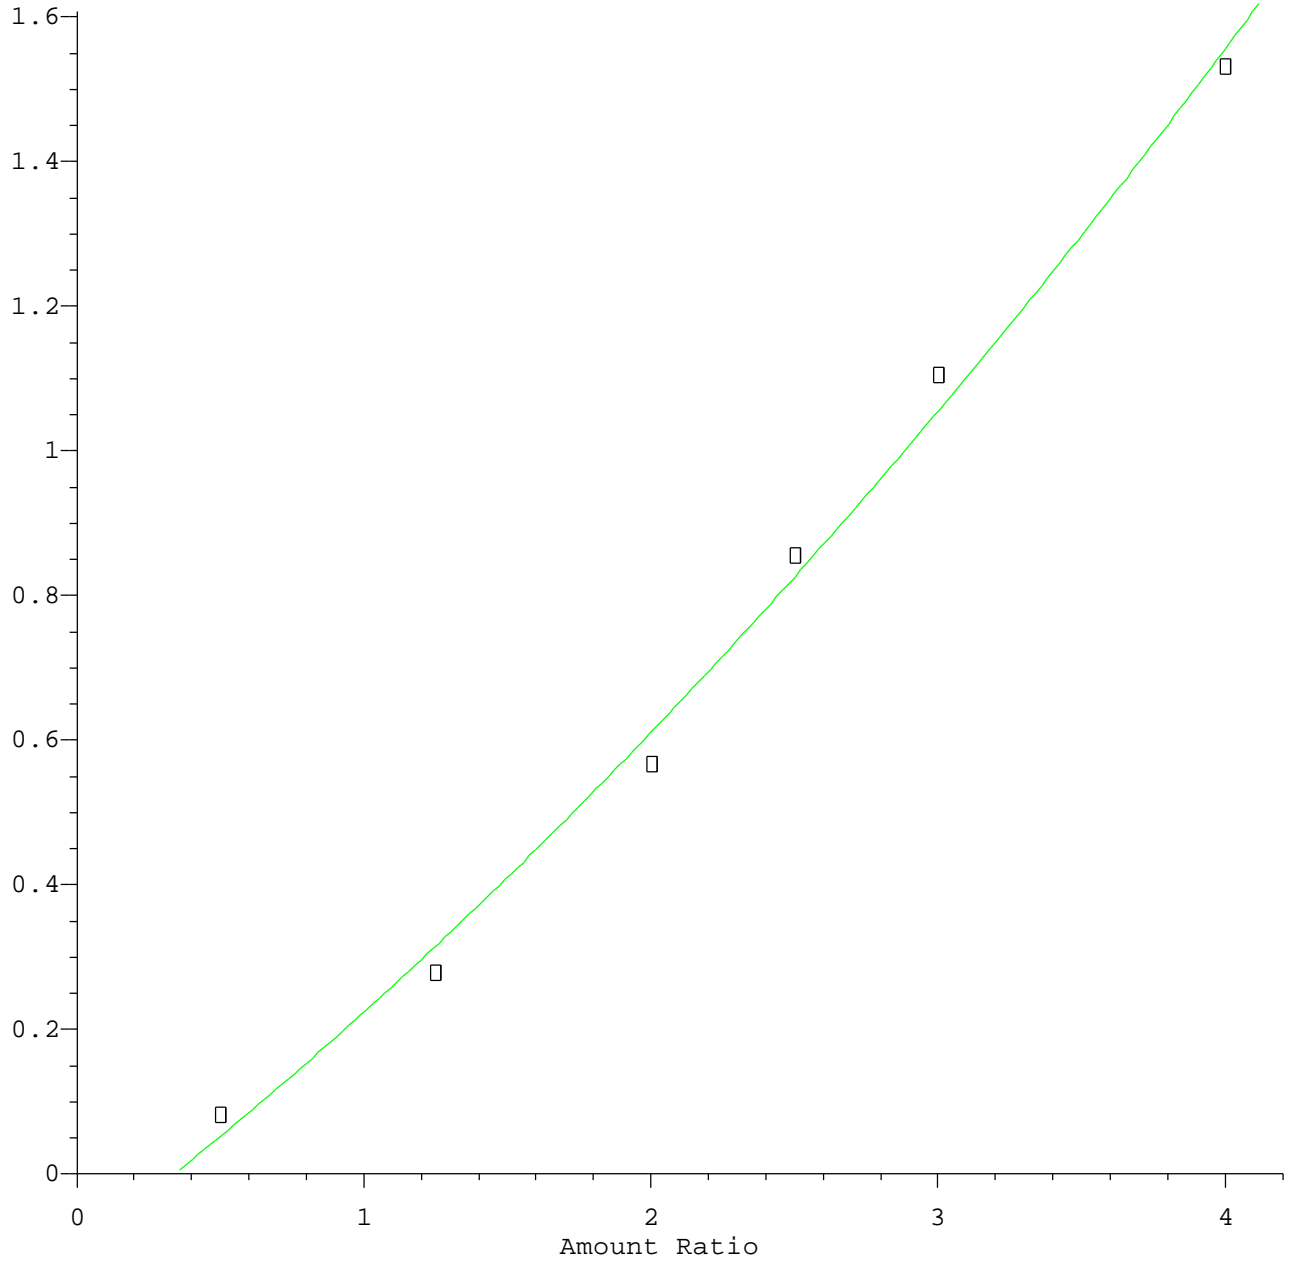


$R = 2.85e-002 A^2 + 3.01e-001 A - 1.06e-001$
Coef of Det (r^2) = 0.994 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018

4,6-Dinitro-2-methylphenol

Response Ratio

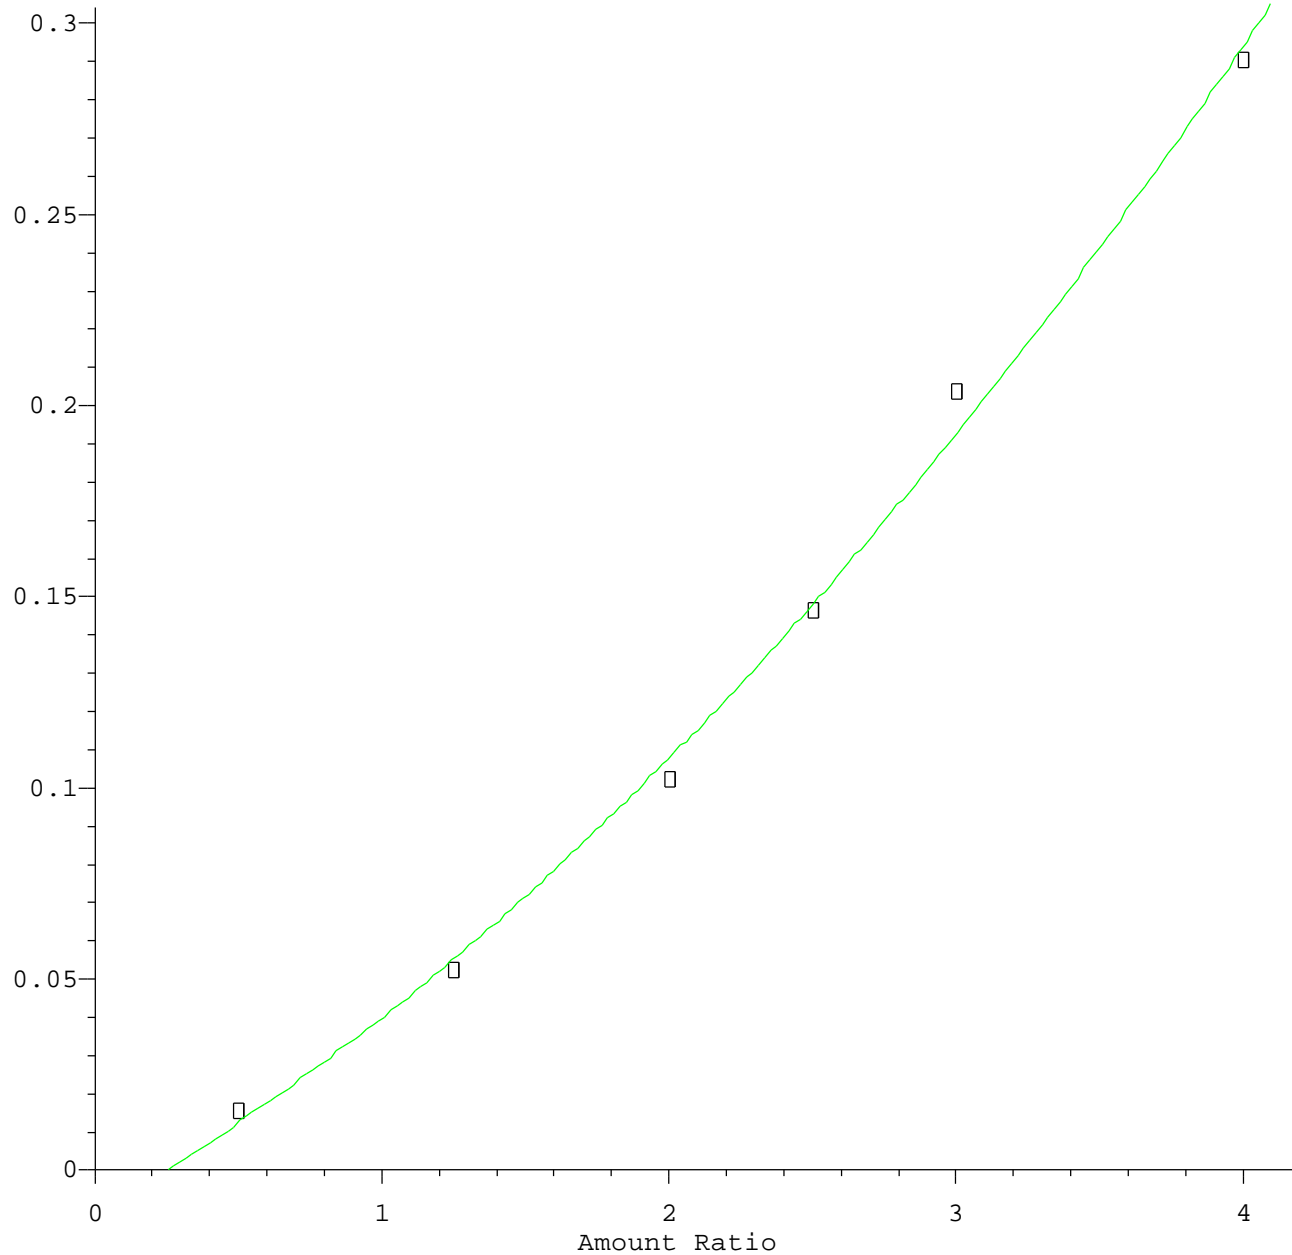

$R = 8.47e-003 A^2 + 4.24e-002 A - 1.10e-002$
Coef of Det (r^2) = 0.996 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Calibration Table Last Updated: Wed Feb 21 15:45:53 2018